

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012925\
 Data File : PD087604.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2025 17:05
 Operator : AR\AJ
 Sample : Q1174-16MSD
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E2944MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/30/2025
 Supervised By :Ankita Jodhani 01/30/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 07:42:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 16 13:39:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.556	2.882	41383457	284.7E6	20.306	23.020
27)	SA Decachlor...	9.091	8.087	68147495	318.2E6	20.383	21.970
Target Compounds							
2)	A alpha-BHC	4.006	3.396	240.5E6	1114.4E6	57.903	56.276
3)	MA gamma-BHC...	4.338	3.734	229.8E6	1017.4E6	57.120	55.547
4)	MA Heptachlor	4.938	4.089	213.1E6	955.0E6	52.140	51.167
5)	MB Aldrin	5.280	4.375	207.8E6	949.9E6	51.894	52.556
6)	B beta-BHC	4.522	4.030	85264529	423.0E6	47.474	49.587
7)	B delta-BHC	4.771	4.267	227.7E6	1013.0E6	55.110	54.279
8)	B Heptachlo...	5.700	4.880	191.1E6	879.5E6	51.136	51.960
9)	A Endosulfan I	6.082	5.255	173.4E6	824.5E6	49.774m	51.947
10)	B trans-Chl...	5.955	5.134	182.9E6	920.9E6	49.648	51.222
11)	B cis-Chlor...	6.035	5.198	186.2E6	899.5E6	50.093m	51.972
12)	B 4,4'-DDE	6.204	5.384	358.9E6	1679.4E6	101.900m	102.533
13)	MA Dieldrin	6.357	5.521	398.1E6	1733.4E6	104.426	103.854
14)	MA Endrin	6.585	5.798	327.8E6	1562.9E6	100.987	104.596
15)	B Endosulfa...	6.796	6.089	315.8E6	1472.2E6	98.107	99.374
16)	A 4,4'-DDD	6.715	5.939	281.2E6	1412.1E6	102.288	105.619
17)	MA 4,4'-DDT	7.032	6.193	284.0E6	1336.5E6	98.002	96.981
18)	B Endrin al...	6.925	6.268	225.6E6	1078.8E6	89.532	93.577
19)	B Endosulfa...	7.158	6.492	298.3E6	1446.5E6	96.638m	99.502
20)	A Methoxychlor	7.504	6.766	709.6E6	2850.3E6	447.908	462.765
21)	B Endrin ke...	7.641	7.002	323.4E6	1534.1E6	93.947	96.597

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012925\
Data File : PD087604.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2025 17:05
Operator : AR\AJ
Sample : Q1174-16MSD
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 07:42:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 16 13:39:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

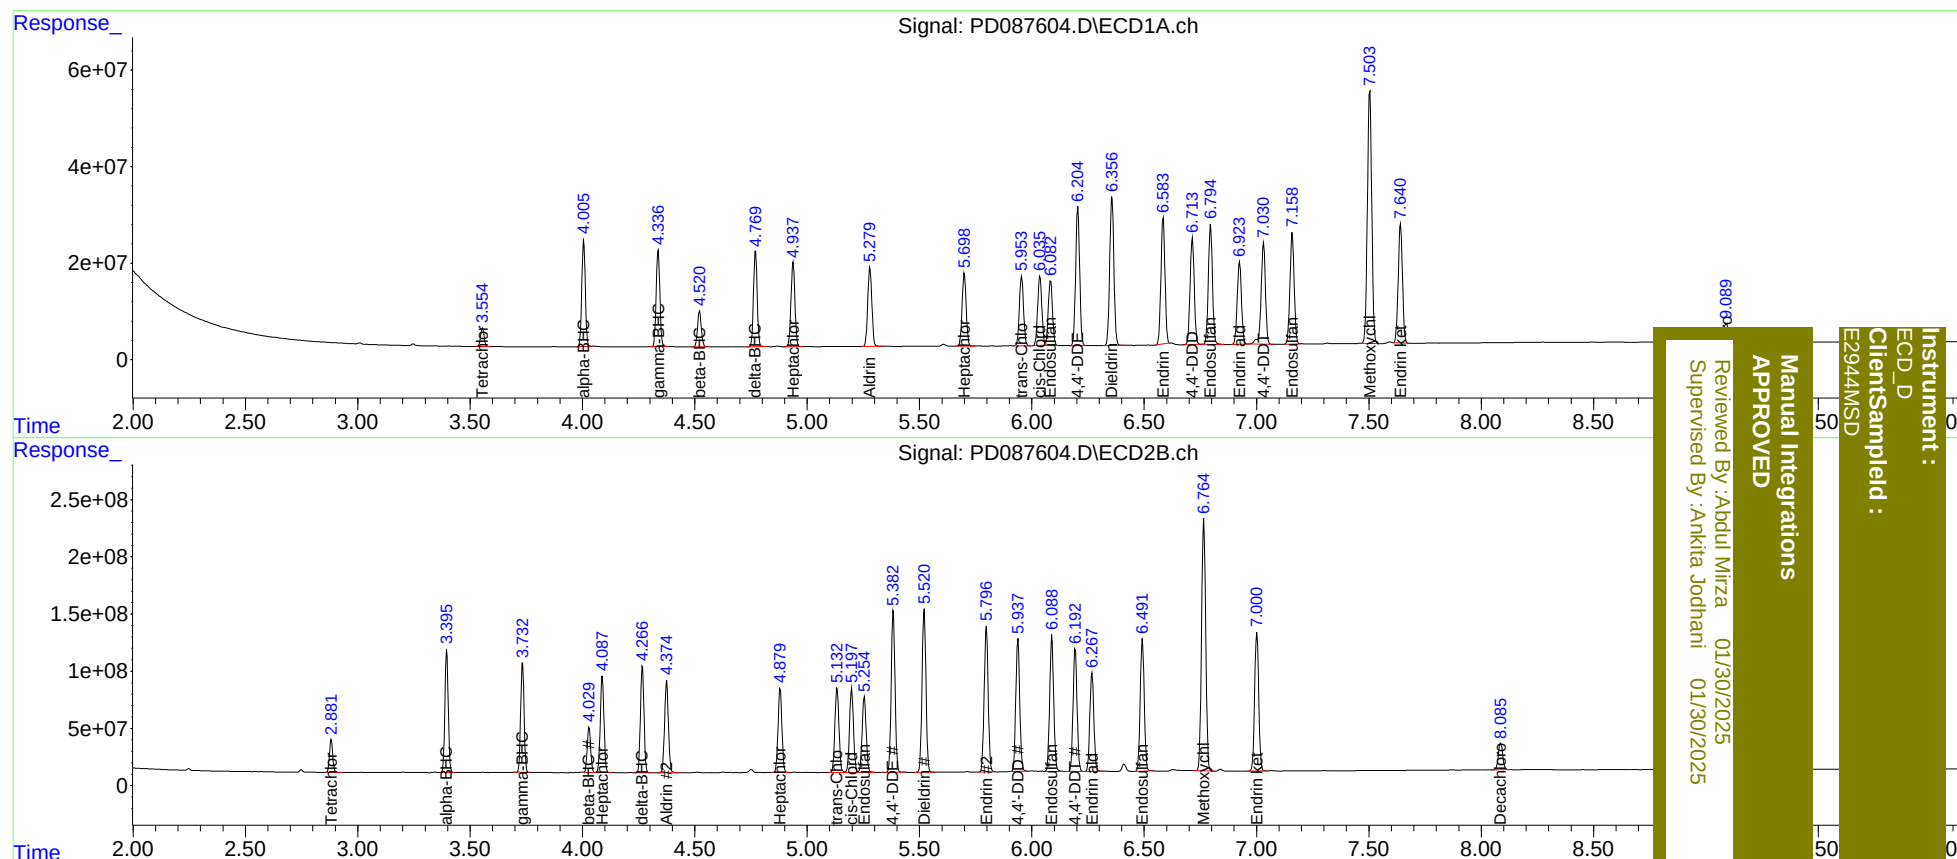

Instrument :
ECD_D
Client Sampled :
E2944MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 01/30/2025
Supervised By: Ankita Jodhani 01/30/2025