

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012925\
 Data File : PD087594.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2025 14:45
 Operator : AR\AJ
 Sample : Q1184-13
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E2967

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/30/2025
 Supervised By : Ankita Jodhani 01/30/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 12:00:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 16 13:39:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.554	2.880	33744328	365.3E6	16.558m	29.535m#
2) SA Decachlor...	9.090	8.085	54972400	274.5E6	16.443m	18.955m
Target Compounds						
7) B delta-BHC	4.765	4.244	14274411	124.9E6	3.454m	6.694m#
9) A Endosulfan I	6.083	5.270	25691769	39945210	7.374m	2.517 #
11) B cis-Chlor...	6.022	5.183	5830697	25696441	1.568m	1.485m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012925\
Data File : PD087594.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2025 14:45
Operator : AR\AJ
Sample : Q1184-13
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 12:00:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 16 13:39:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

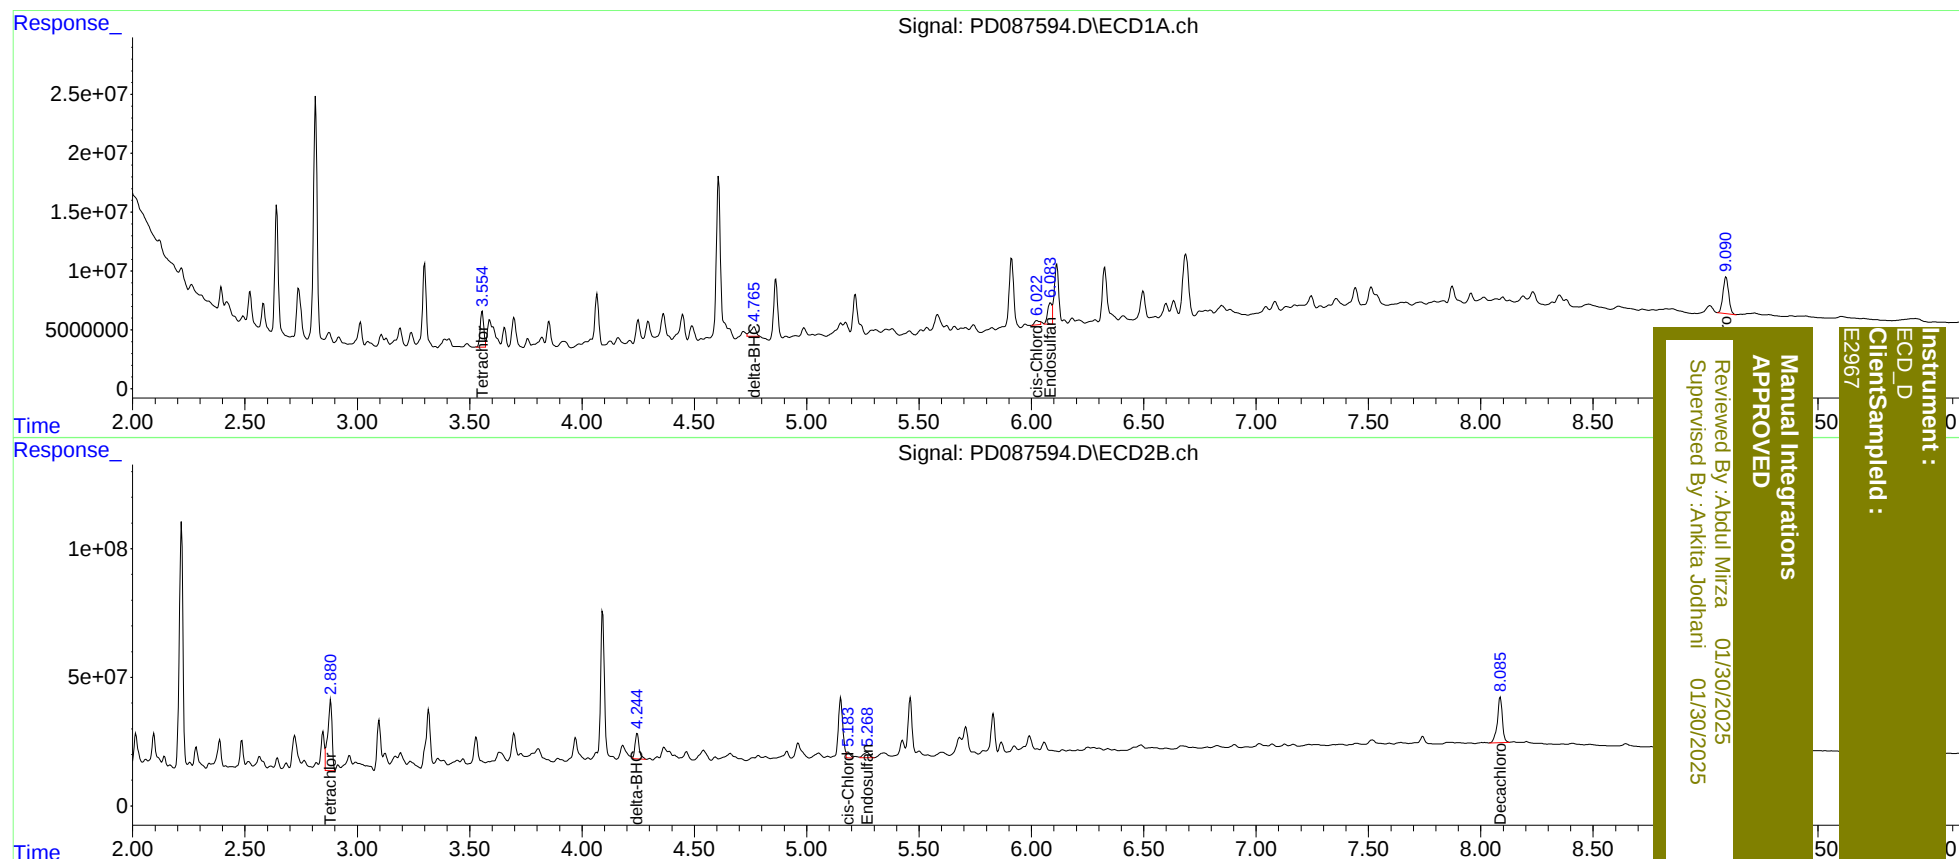

Instrument :
ECD_D
ClientSampled :
E2967

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/30/2025
Supervised By :Ankita Jodhani 01/30/2025