

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012925\
 Data File : PD087595.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2025 14:59
 Operator : AR\AJ
 Sample : Q1184-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E2965

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/30/2025
 Supervised By : Ankita Jodhani 01/30/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 07:39:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 16 13:39:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.554	2.897	13463182	902.0E6	6.606m	72.928m#
2)	SA Decachlor...	9.092	8.085	56369280	154.4E6	16.860m	10.661m#
Target Compounds							
9)	A Endosulfan I	6.085	5.252	740.1E6	369.8E6	212.443	23.298 #
10)	B trans-Chl...	5.959	5.113	42904704	539.0E6	11.646m	29.982 #
12)	B 4,4'-DDE	6.215	5.373	32674856	530.6E6	9.277m	32.397m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012925\
Data File : PD087595.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2025 14:59
Operator : AR\AJ
Sample : Q1184-14
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 07:39:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 16 13:39:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

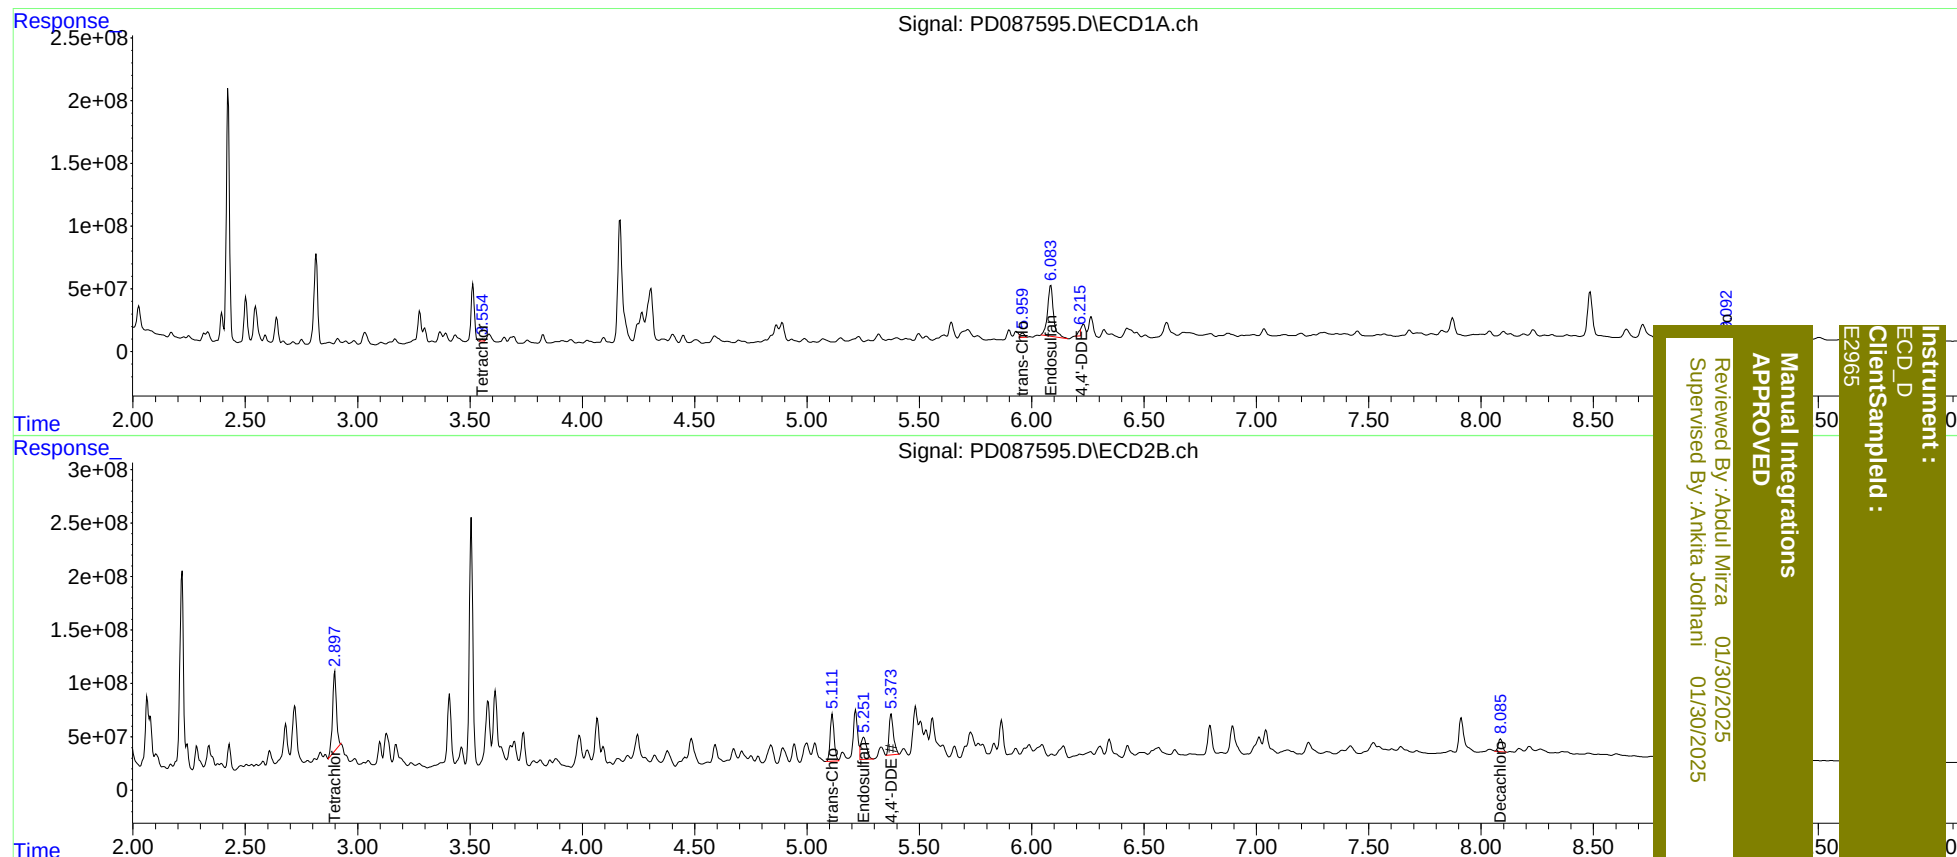

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 01/30/2025
Supervised By: Ankita Jodhani 01/30/2025

Instrument :
ECD_D
ClientSampled :
E2965