

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012925\
 Data File : PD087596.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2025 15:13
 Operator : AR\AJ
 Sample : Q1184-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E2966

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/30/2025
 Supervised By : Ankita Jodhani 01/30/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 07:40:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 16 13:39:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.896	10714668	1072.2E6	5.257m	86.693m#
2)	SA Decachlor...	9.092	8.085	37229327	129.2E6	11.136m	8.917m
Target Compounds							
6)	B beta-BHC	4.513	4.022	23086541	117.9E6	12.854m	13.819m
7)	B delta-BHC	4.776	4.273	30063239	125.8E6	7.275m	6.743m
9)	A Endosulfan I	6.085	5.257	567.8E6	344.5E6	162.967	21.707 #
12)	B 4,4'-DDE	6.216	5.373	29674408	316.9E6	8.425m	19.349m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012925\
Data File : PD087596.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2025 15:13
Operator : AR\AJ
Sample : Q1184-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 07:40:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 16 13:39:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

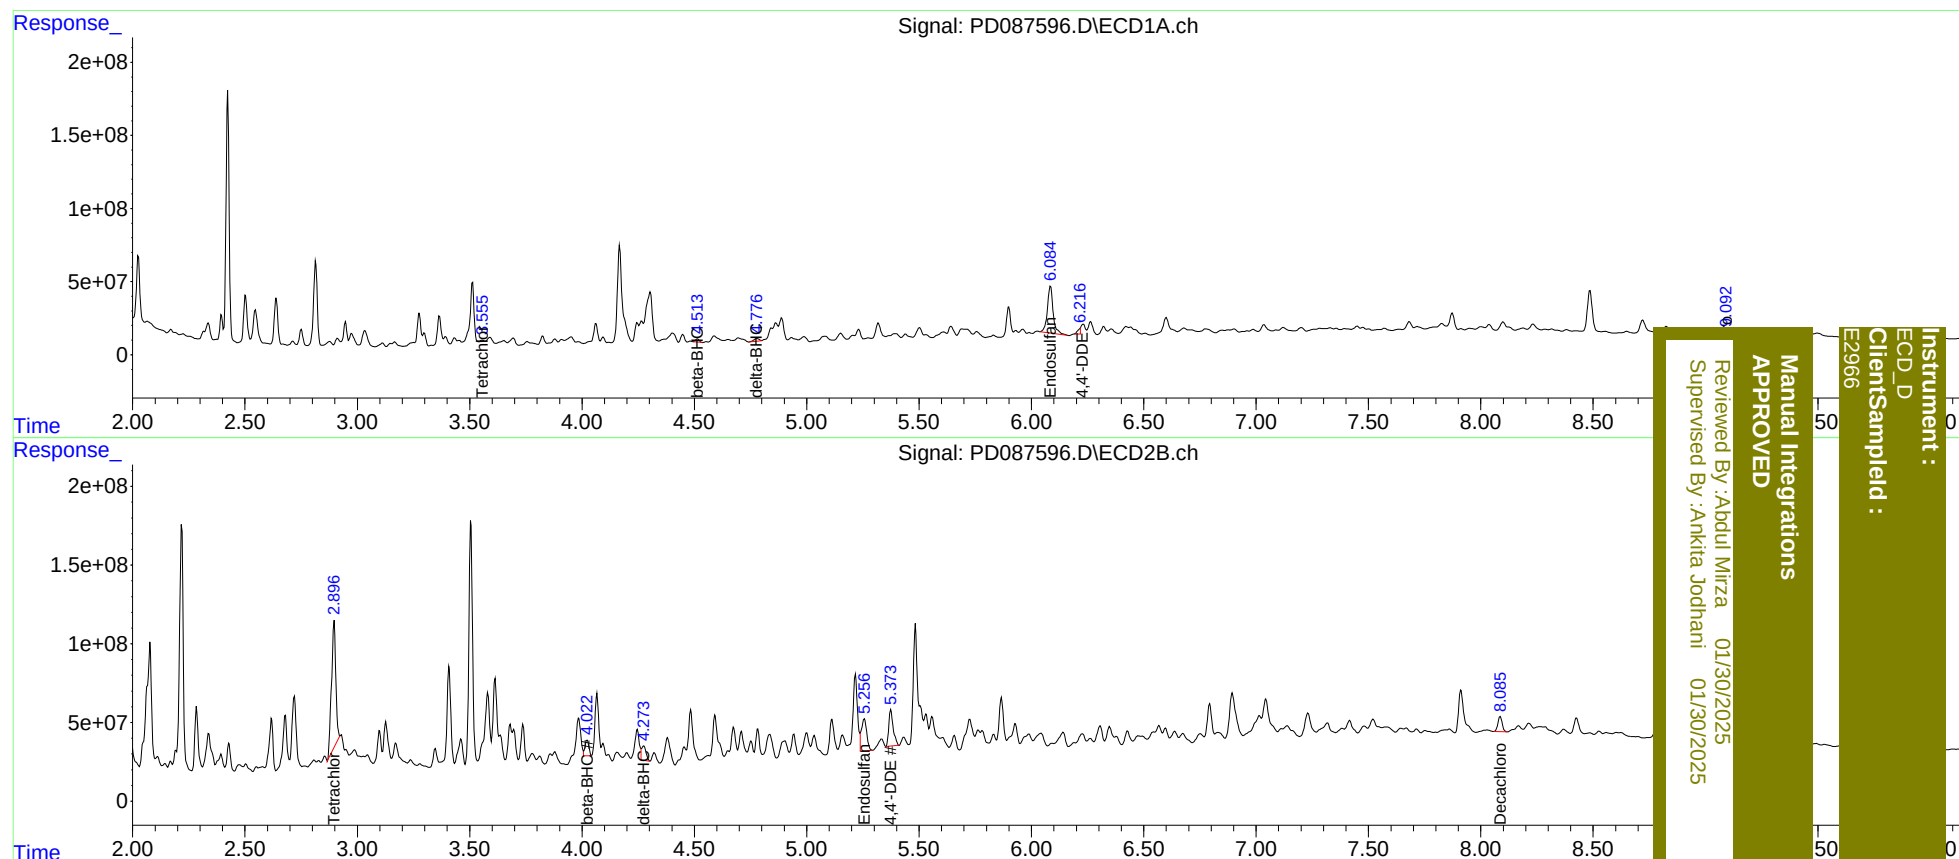

Instrument :
ECD_D
ClientSampled :
E2966

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 01/30/2025
Supervised By: Ankita Jodhani 01/30/2025