

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD013024\
 Data File : PD080975.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jan 2024 14:01
 Operator : AR\AJ
 Sample : P1265-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PEST-GPC2-BLANK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 21:15:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 10 14:12:04 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	0.000	2.787	0	407316	N.D.	0.160
Target Compounds						
3) MA gamma-BHC...	0.000	3.640	0	143872	N.D.	<MDL
4) MA Heptachlor	0.000	3.957	0	157144	N.D.	<MDL
5) MB Aldrin	0.000	4.227	0	175872	N.D.	<MDL
6) B beta-BHC	0.000	3.957f	0	157144	N.D.	<MDL
14) MA Endrin	0.000	5.675	0	83320	N.D.	<MDL

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD013024\
Data File : PD080975.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jan 2024 14:01
Operator : AR\AJ
Sample : P1265-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 21:15:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jan 10 14:12:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

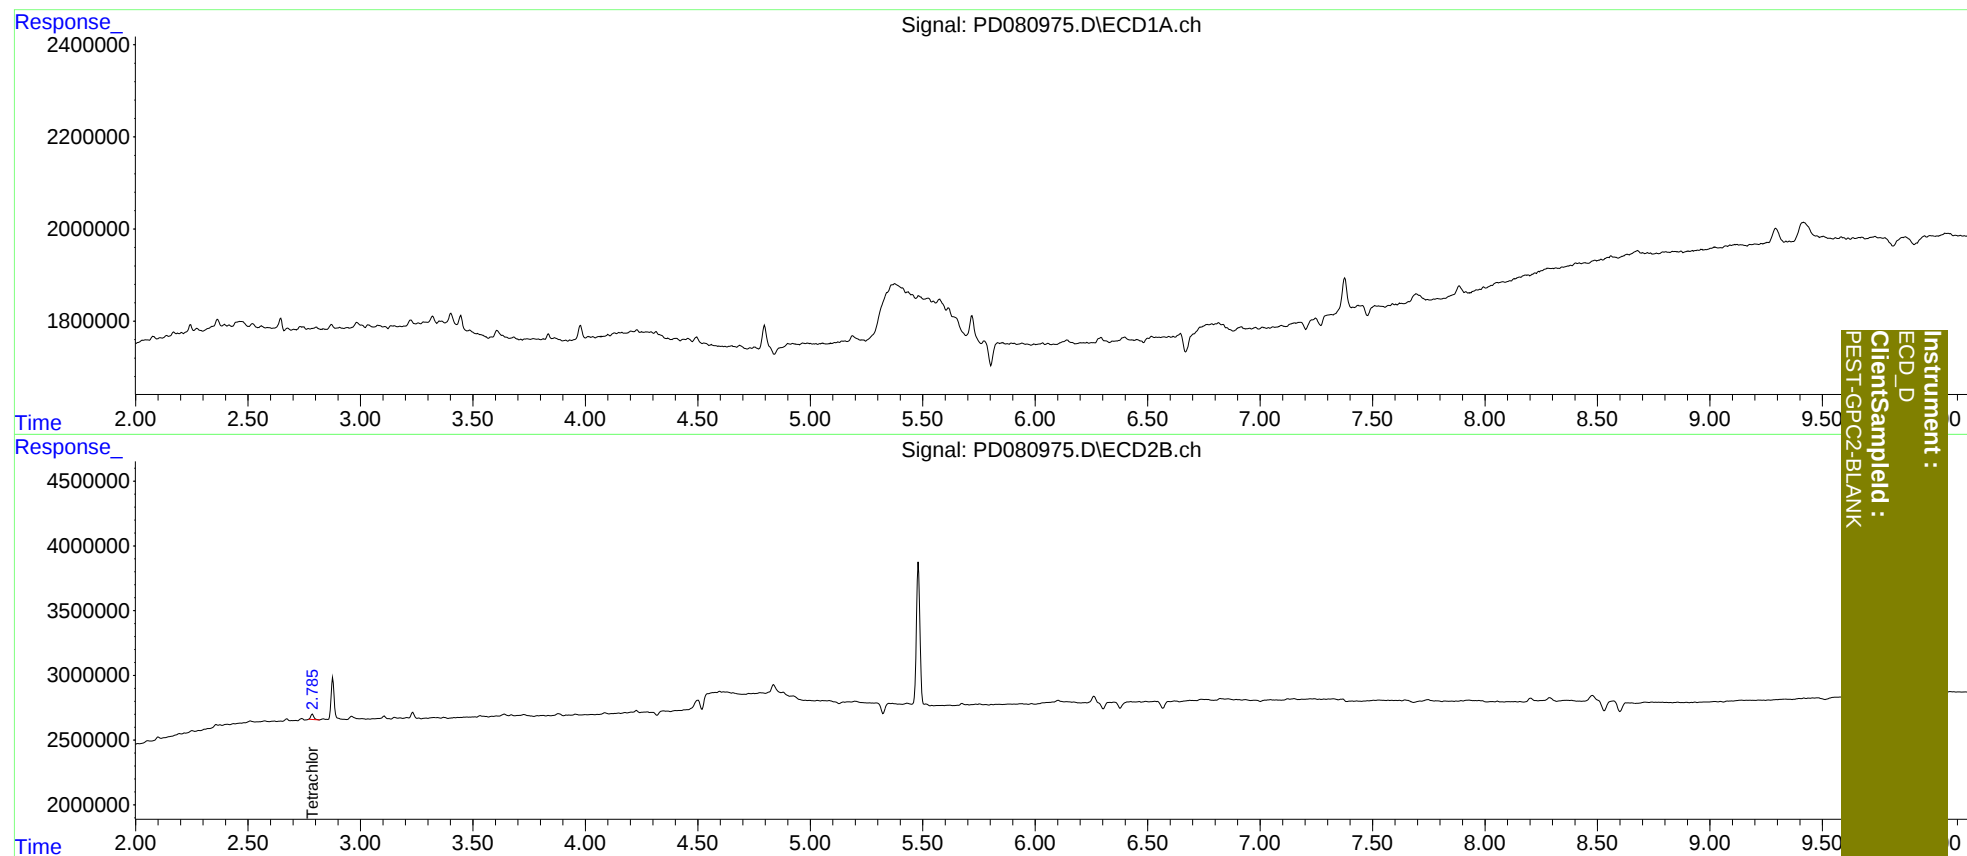


Instrument :
ECD_D
ClientSample :
PEST-GPC2-BLANK

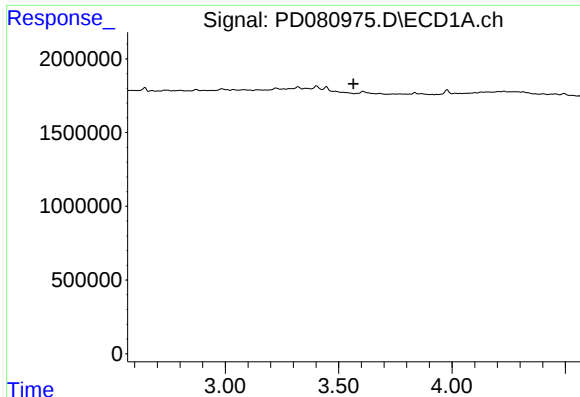

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.566 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PEST-GPC2-BLANK

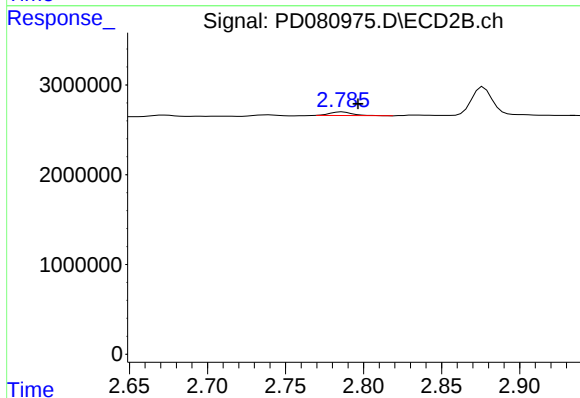


#1 Tetrachloro-m-xylene

R.T.: 2.787 min
Delta R.T.: -0.010 min
Response: 407316
Conc: 0.16 ng/ml

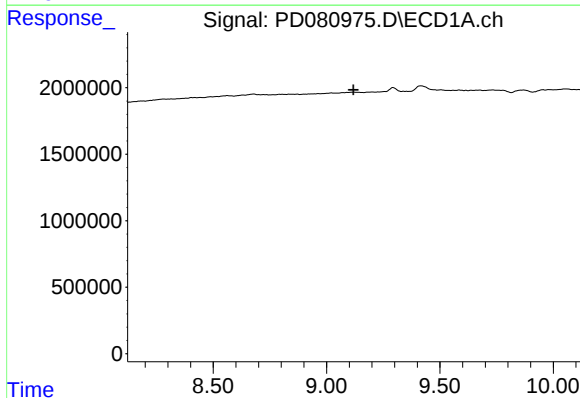

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.119 min
Response: 0
Conc: N.D.

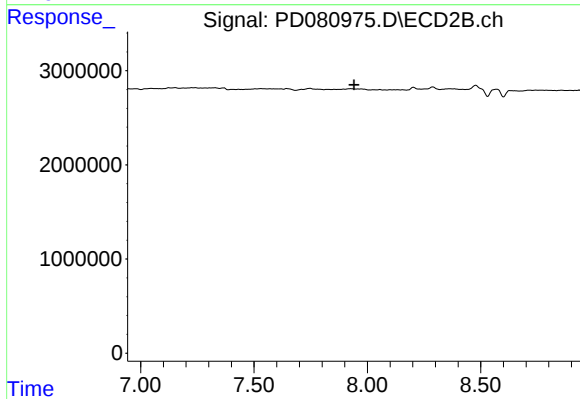

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.941 min
Response: 0
Conc: N.D.