

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD013120\
 Data File : PD057121.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2020 18:57
 Operator : AJ\MA
 Sample : L1300-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C5AP6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 21:58:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012320CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 24 08:33:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.961	9932452	21509562	10.985	11.623
27)	SA Decachlor...	7.956	8.996	13480809	23758558	12.383	12.713
Target Compounds							
10)	B trans-Chl...	0.000	6.045	0	2222157	N.D.	0.946

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD013120\
Data File : PD057121.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2020 18:57
Operator : AJ\MA
Sample : L1300-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 21:58:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012320CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 24 08:33:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

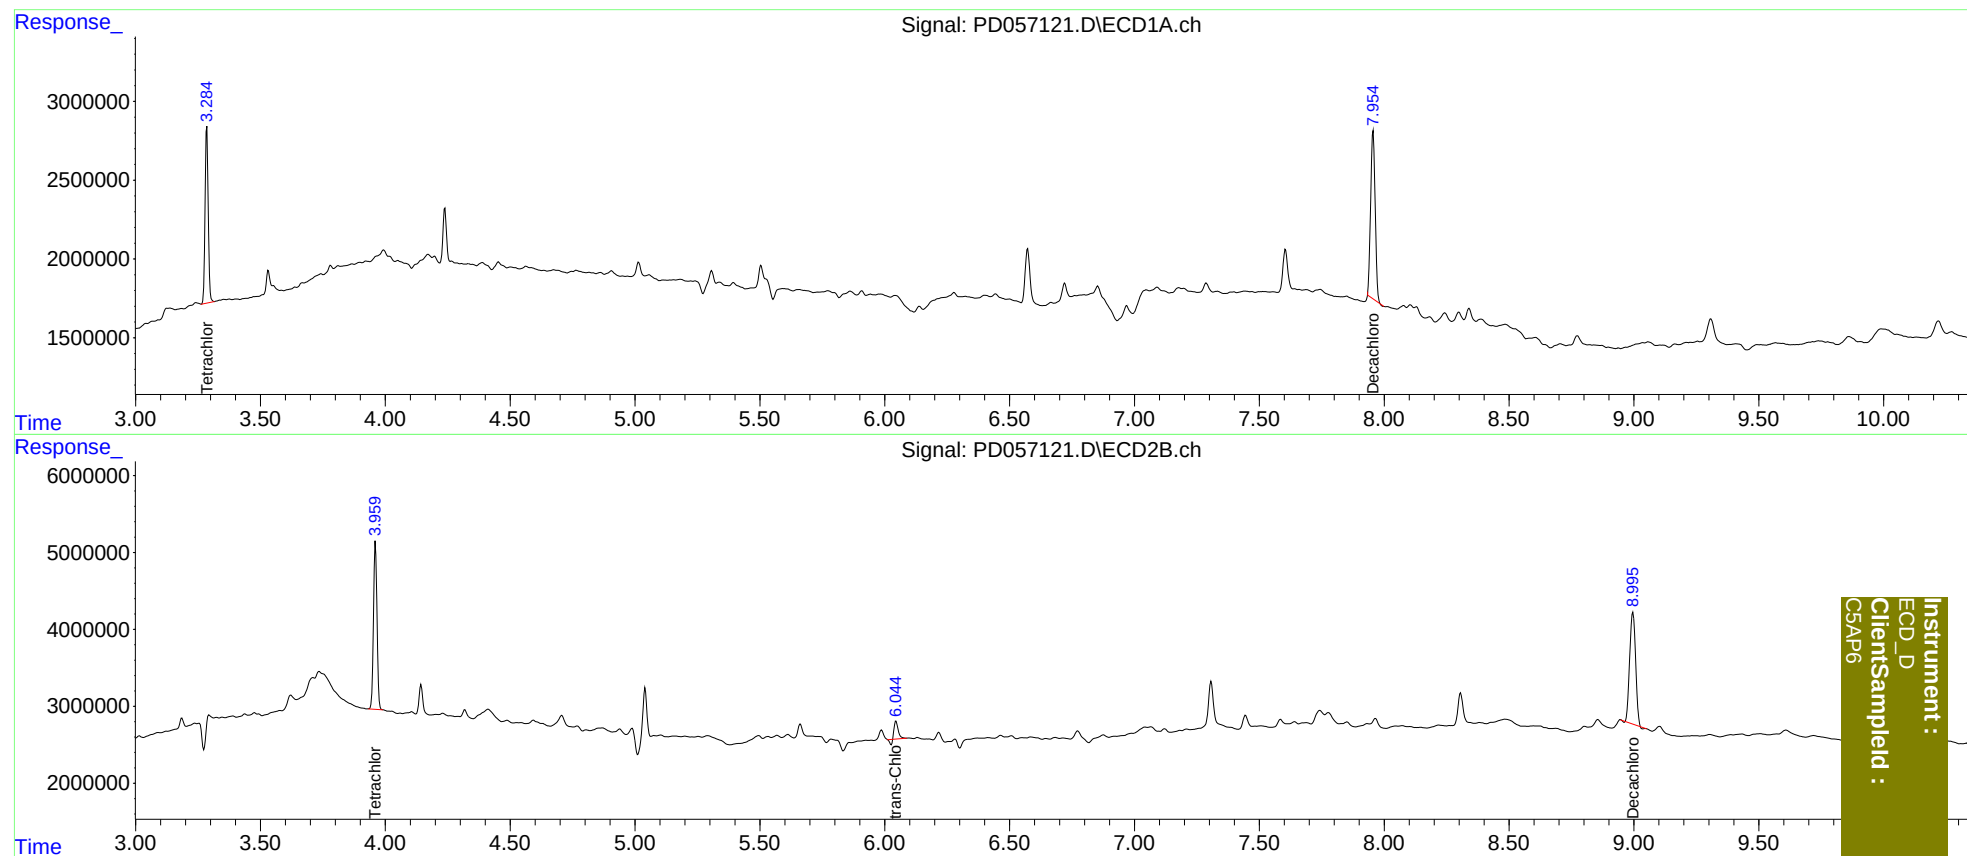


Instrument :
ECD_D
ClientSampleId :
C5AP6

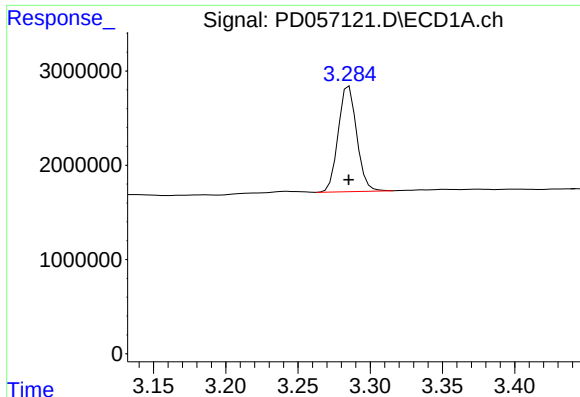

#1 Tetrachloro-m-xylene


R.T.: 3.285 min
Delta R.T.: 0.000 min
Response: 9932452
Conc: 10.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
C5AP6

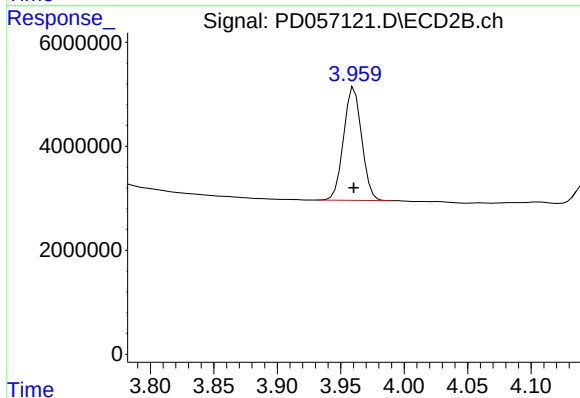


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: 0.000 min
Response: 21509562
Conc: 11.62 ng/ml

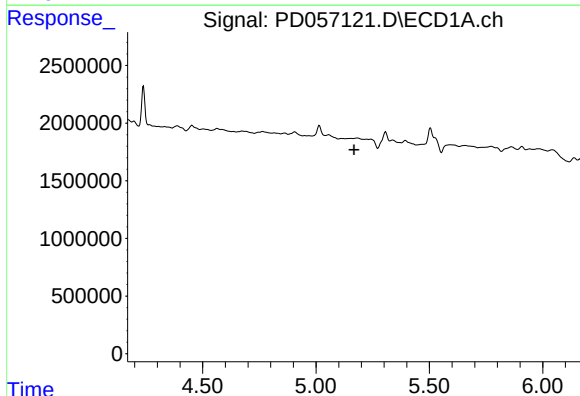


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.168 min
Response: 0
Conc: N.D.

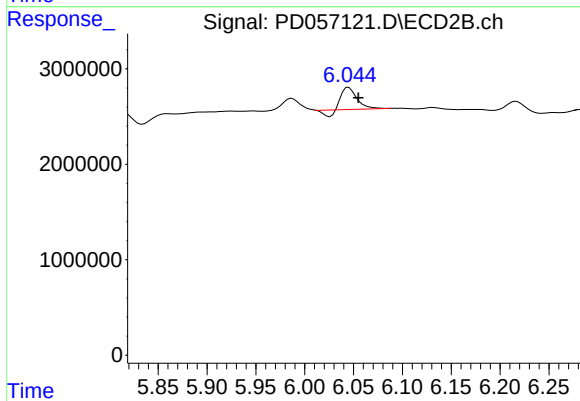

#10 trans-Chlordane


R.T.: 6.045 min
Delta R.T.: -0.010 min
Response: 2222157
Conc: 0.95 ng/ml

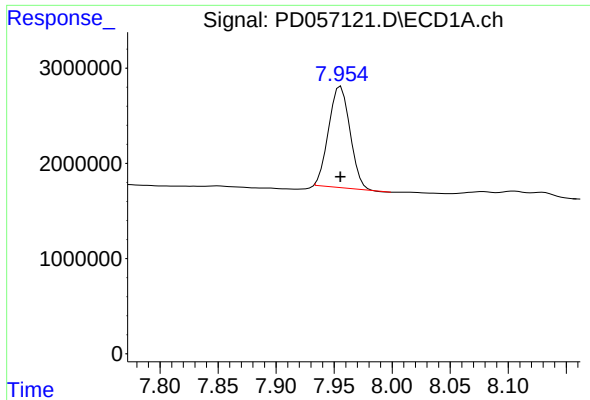

#27 Decachlorobiphenyl

R.T.: 7.956 min
Delta R.T.: 0.000 min
Response: 13480809
Conc: 12.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
C5AP6

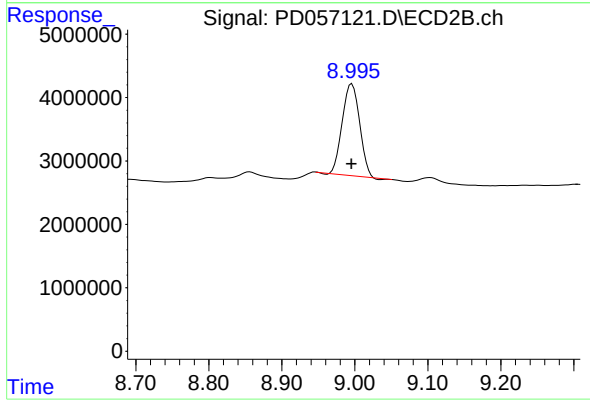

#27 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: 0.000 min
Response: 23758558
Conc: 12.71 ng/ml