

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD013120\
 Data File : PD057123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2020 19:26
 Operator : AJ\MA
 Sample : L1300-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C5AR8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 21:58:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012320CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 24 08:33:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.285	3.961	9708055	20640661	10.737	11.154
27) SA Decachlor...	7.955	8.996	14491485	24952204	13.311	13.352
Target Compounds						
10) B trans-Chl...	0.000	6.045	0	2375299	N.D.	1.011

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD013120\
Data File : PD057123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2020 19:26
Operator : AJ\MA
Sample : L1300-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 21:58:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012320CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 24 08:33:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

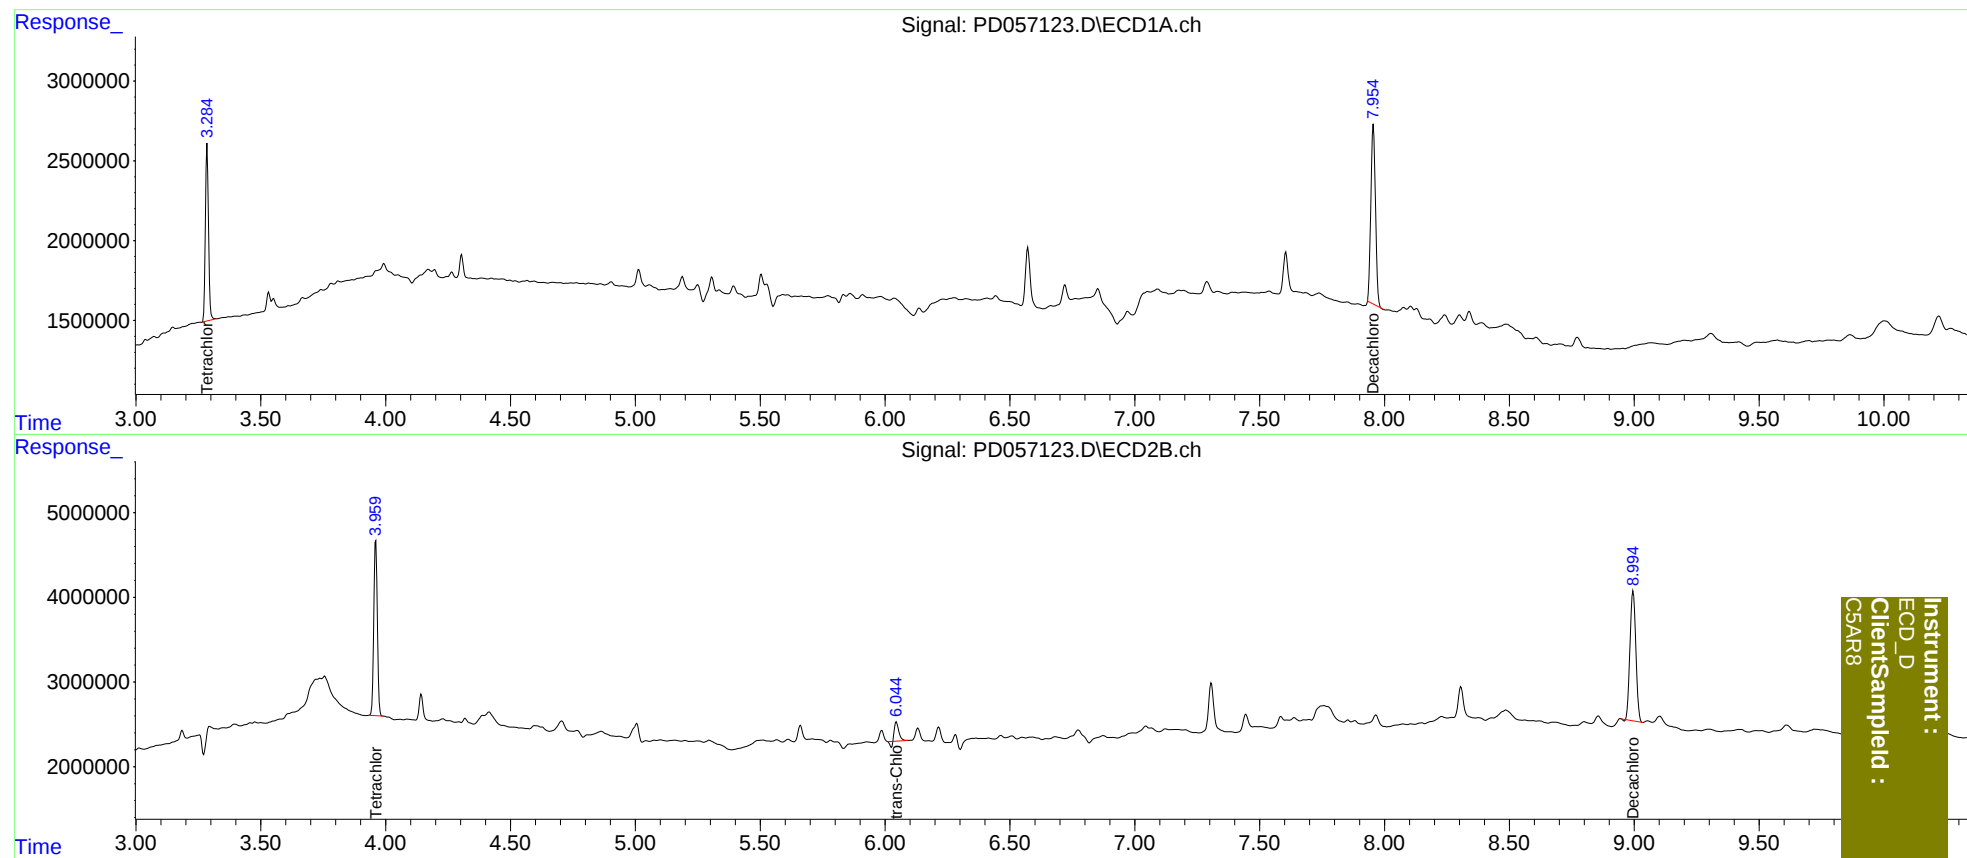


Instrument :
ECD_D
ClientSampleId :
C5AR8

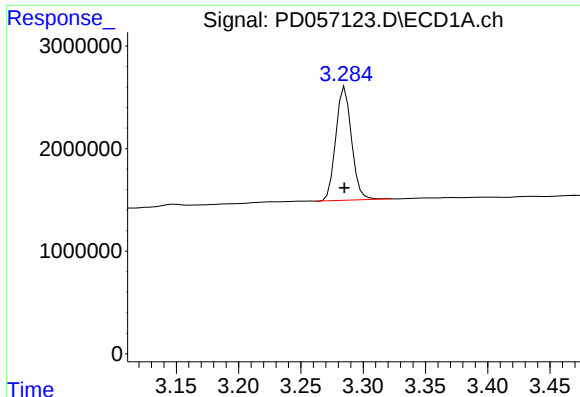

#1 Tetrachloro-m-xylene


R.T.: 3.285 min
Delta R.T.: 0.000 min
Response: 9708055
Conc: 10.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
C5AR8

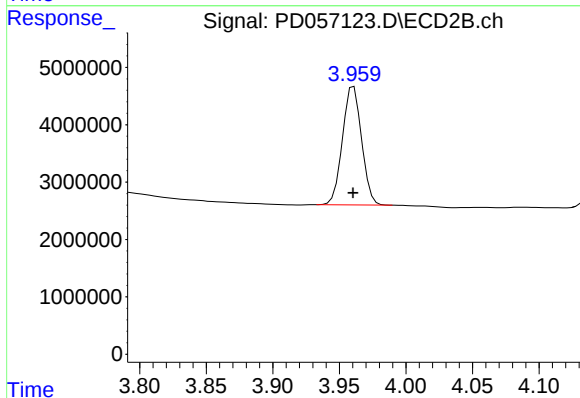


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: 0.000 min
Response: 20640661
Conc: 11.15 ng/ml

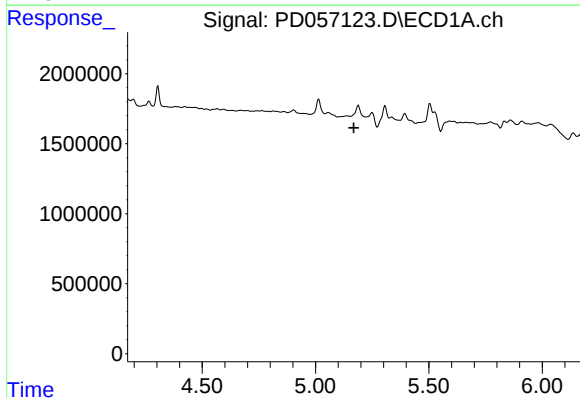


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.168 min
Response: 0
Conc: N.D.

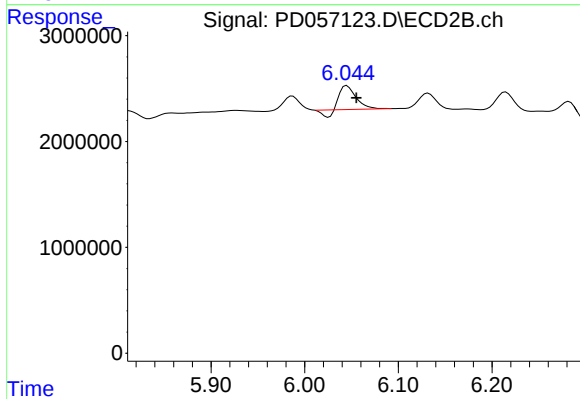

#10 trans-Chlordane


R.T.: 6.045 min
Delta R.T.: -0.010 min
Response: 2375299
Conc: 1.01 ng/ml

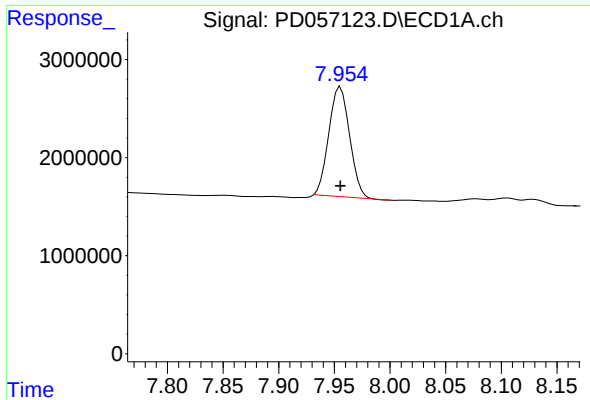

#27 Decachlorobiphenyl

R.T.: 7.955 min
Delta R.T.: 0.000 min
Response: 14491485
Conc: 13.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
C5AR8

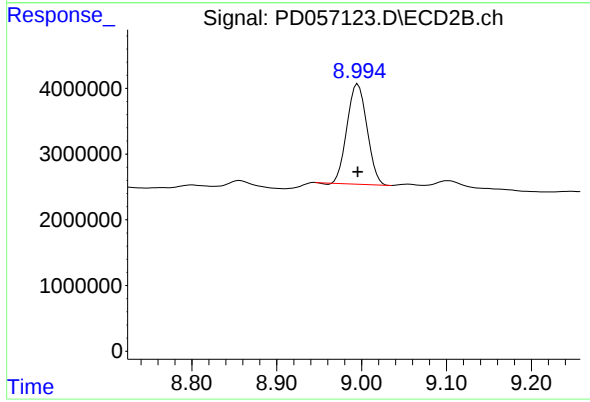

#27 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: 0.000 min
Response: 24952204
Conc: 13.35 ng/ml