

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD013120\
 Data File : PD057125.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2020 19:54
 Operator : AJ\MA
 Sample : L1300-18
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C5AS0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 21:59:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012320CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 24 08:33:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.960	10200825	21633373	11.282	11.690
27)	SA Decachlor...	7.956	8.996	14568098	24227993	13.382	12.965
Target Compounds							
9)	A Endosulfan I	0.000	6.132f	0	4091622	N.D.	1.879
10)	B trans-Chl...	0.000	6.045	0	6732021	N.D.	2.865
11)	B cis-Chlor...	0.000	6.132	0	4091622	N.D.	1.736
20)	A Methoxychlor	0.000	7.583f	0	5386464	N.D.	5.337
21)	B Endrin ke...	0.000	7.733f	0	5707107	N.D.	2.694
26)	Toxaphene-5	0.000	7.583	0	5386464	N.D.	208.622

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD013120\
Data File : PD057125.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2020 19:54
Operator : AJ\MA
Sample : L1300-18
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 21:59:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012320CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 24 08:33:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

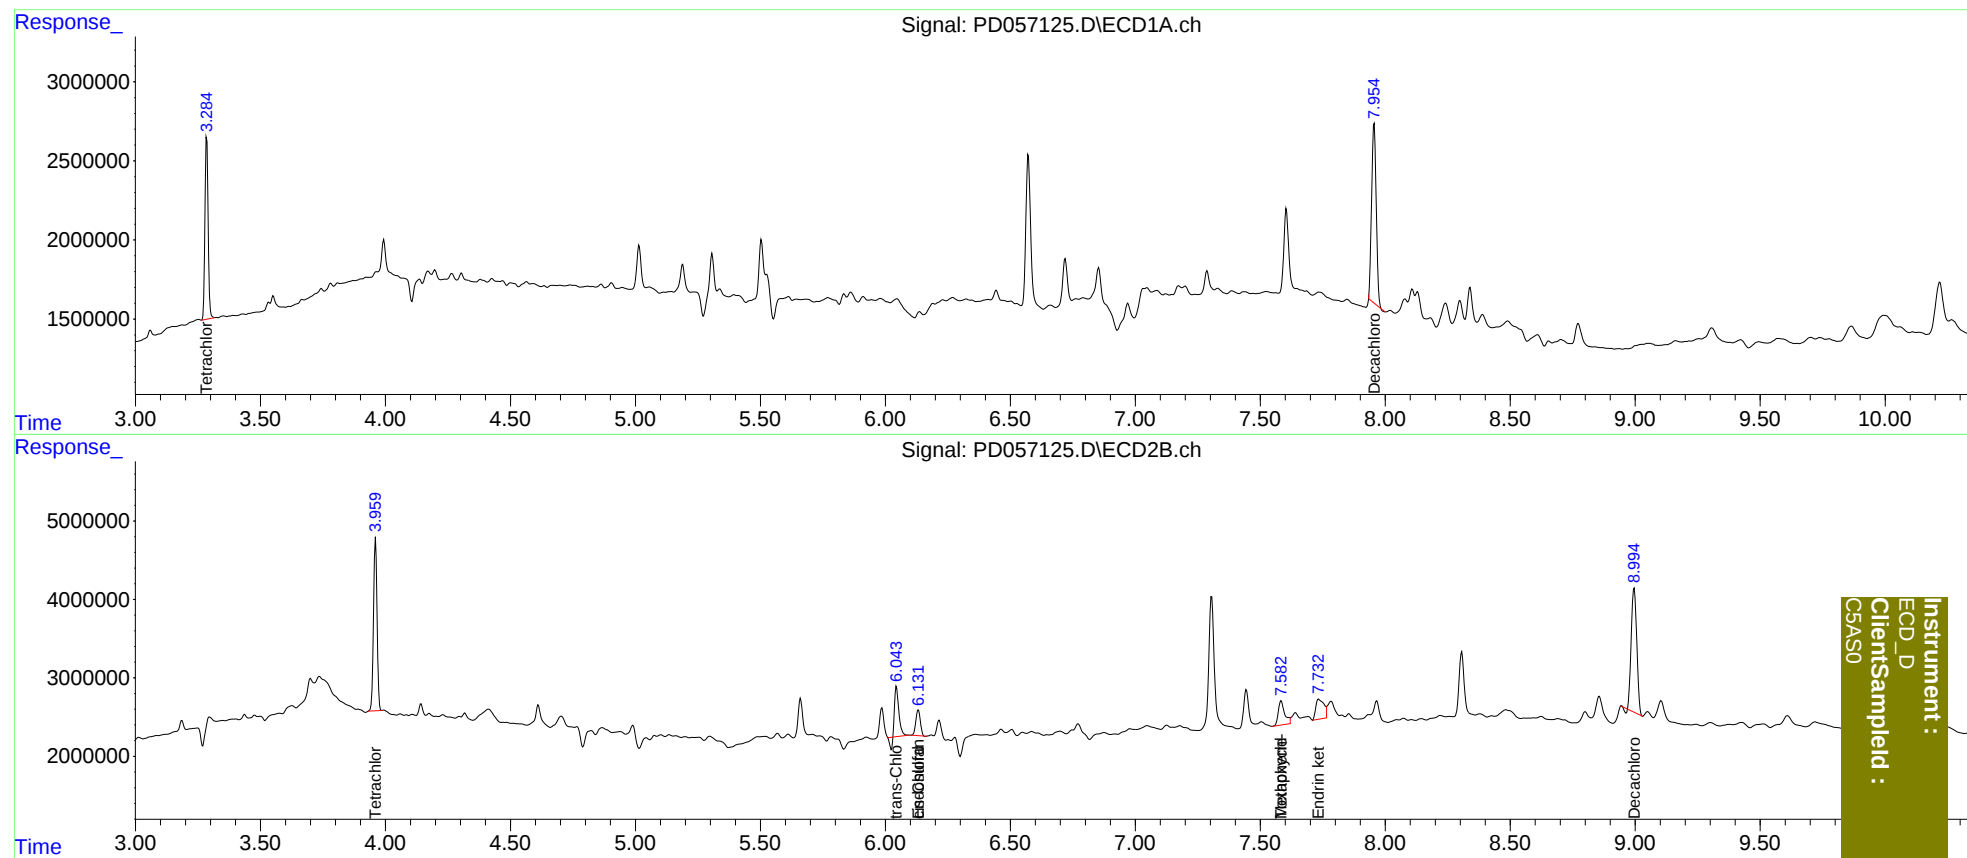


Instrument :
ECD_D
ClientSampleId :
C5AS0

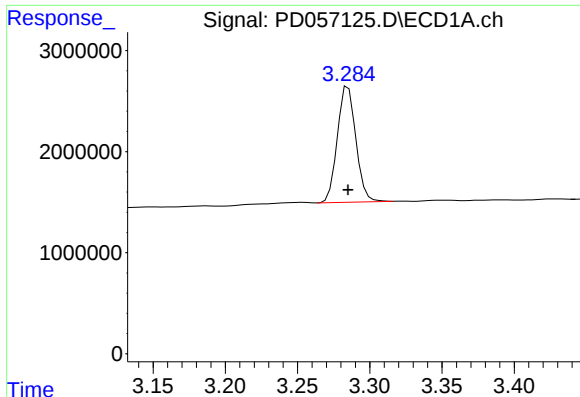

#1 Tetrachloro-m-xylene


R.T.: 3.285 min
Delta R.T.: 0.000 min
Response: 10200825
Conc: 11.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
C5AS0

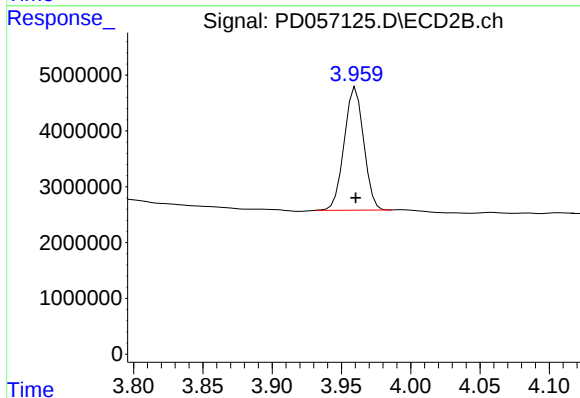


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: 0.000 min
Response: 21633373
Conc: 11.69 ng/ml

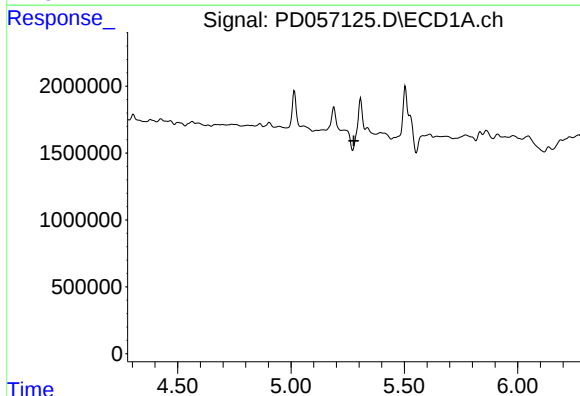


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.277 min
Response: 0
Conc: N.D.

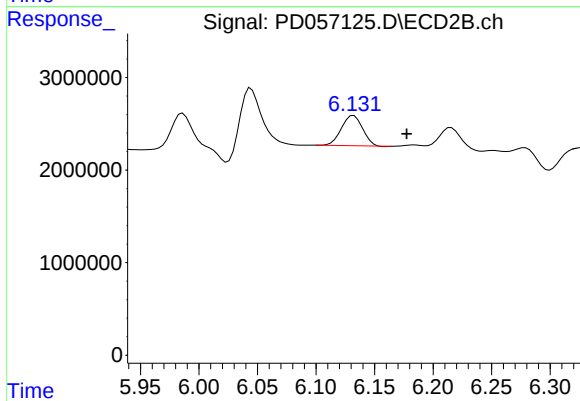

#9 Endosulfan I


R.T.: 6.132 min
Delta R.T.: -0.045 min
Response: 4091622
Conc: 1.88 ng/ml

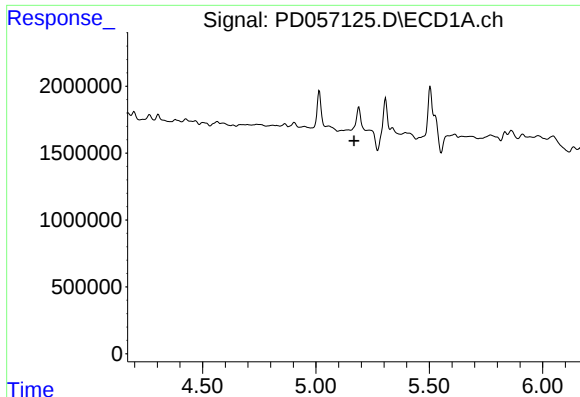

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.168 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C5AS0

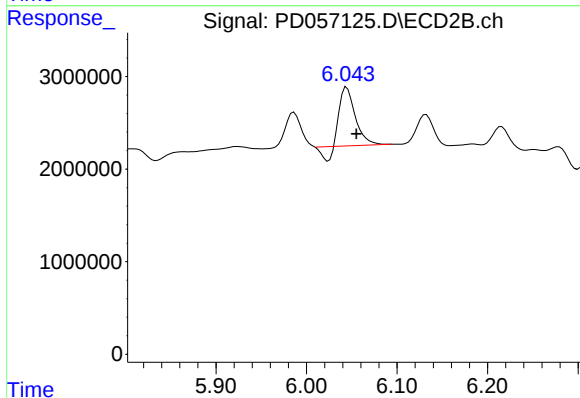


#10 trans-Chlordane

R.T.: 6.045 min
Delta R.T.: -0.011 min
Response: 6732021
Conc: 2.87 ng/ml

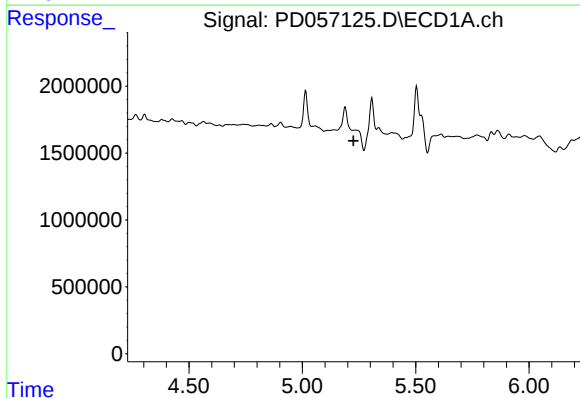


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.226 min
Response: 0
Conc: N.D.

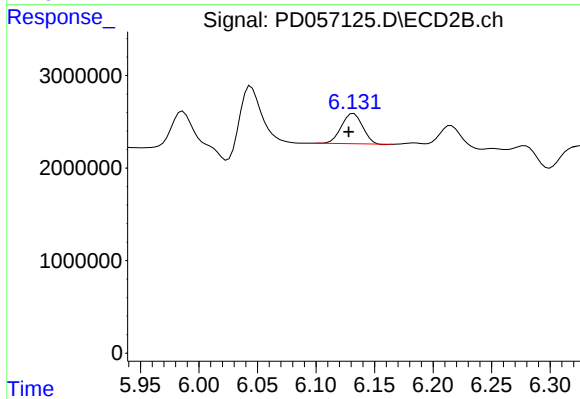

#11 cis-Chlordane


R.T.: 6.132 min
Delta R.T.: 0.004 min
Response: 4091622
Conc: 1.74 ng/ml

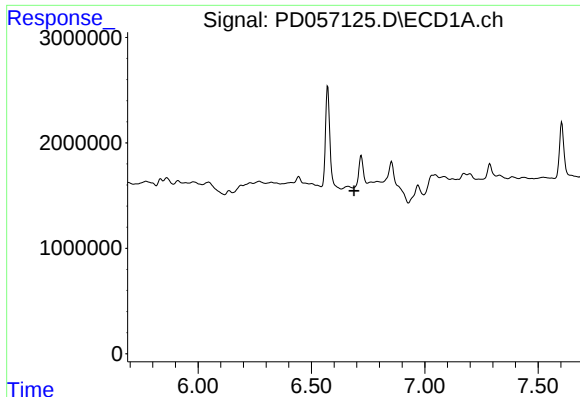

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.688 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C5AS0

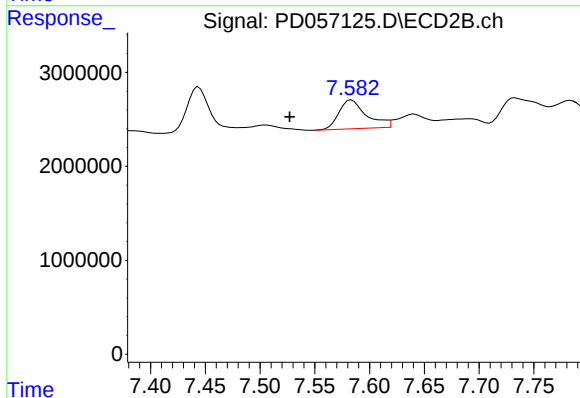


#20 Methoxychlor

R.T.: 7.583 min
Delta R.T.: 0.056 min
Response: 5386464
Conc: 5.34 ng/ml

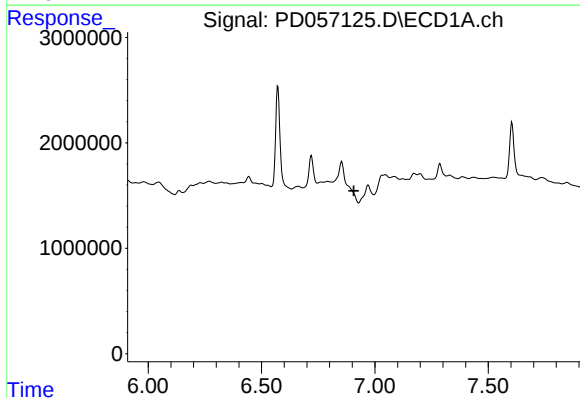


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 6.907 min
Response: 0
Conc: N.D.

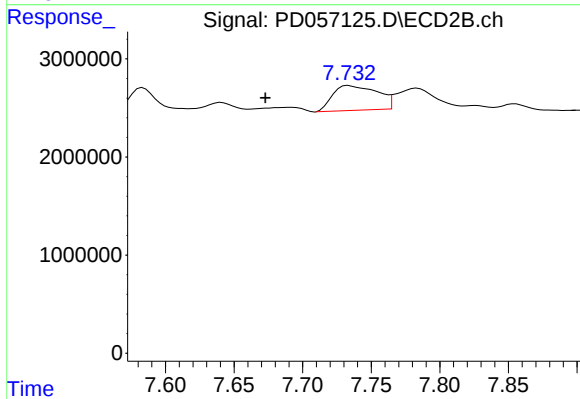

#21 Endrin ketone


R.T.: 7.733 min
Delta R.T.: 0.061 min
Response: 5707107
Conc: 2.69 ng/ml

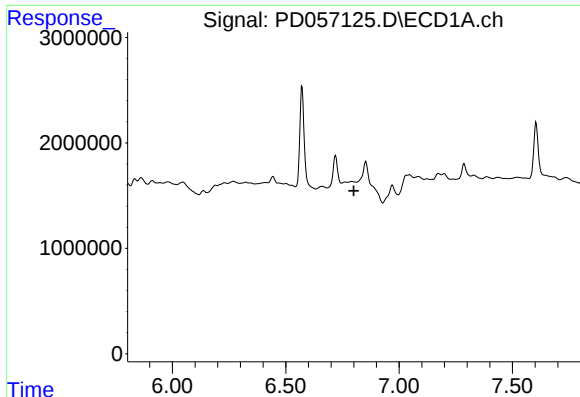

#26 Toxaphene-5


R.T.: 0.000 min
Exp R.T.: 6.800 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C5AS0

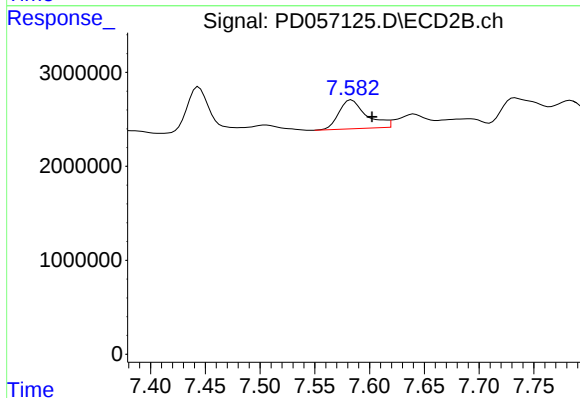


#26 Toxaphene-5

R.T.: 7.583 min
Delta R.T.: -0.019 min
Response: 5386464
Conc: 208.62 ng/ml

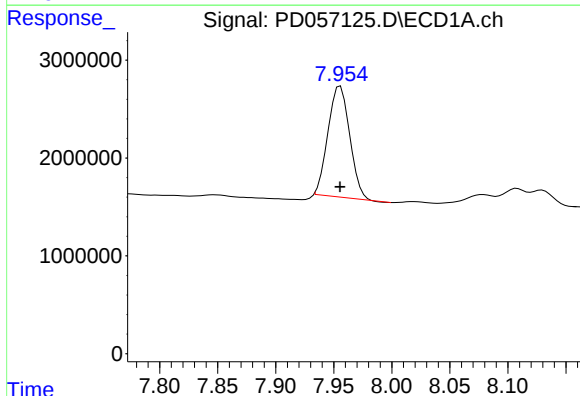

#27 Decachlorobiphenyl

R.T.: 7.956 min
Delta R.T.: 0.000 min
Response: 14568098
Conc: 13.38 ng/ml

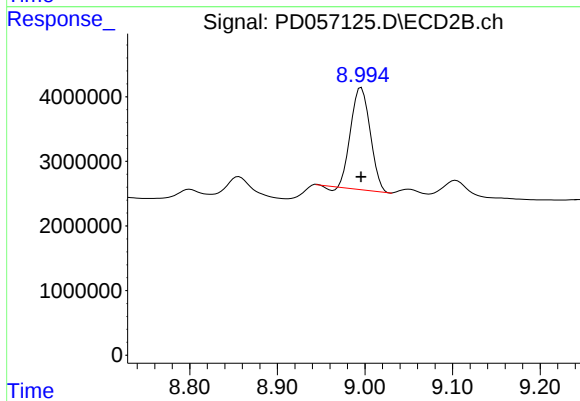

#27 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: 0.000 min
Response: 24227993
Conc: 12.96 ng/ml