

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD013120\
 Data File : PD057112.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2020 16:32
 Operator : AJ\MA
 Sample : L1300-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C5AK0

Manual Integrations
 APPROVED

mohammad
 2/3/2020 2:23:31 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 02:21:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012320CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 24 08:33:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.960	12156693	25415043	13.445	13.734
27)	SA Decachlor...	7.956	8.994	20382941	32452955	18.723	17.366m
Target Compounds							
8)	B Heptachlo...	4.946	5.819	1660106	2707905	1.497m	1.255m
12)	B 4,4'-DDE	5.393	6.283	7084203	11113333	6.284m	5.030
16)	A 4,4'-DDD	5.909	6.768	1686786	5003633	1.903m	2.709m#
17)	MA 4,4'-DDT	6.138	7.072	2105344	5868852	2.451m	3.019

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD013120\
Data File : PD057112.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2020 16:32
Operator : AJ\MA
Sample : L1300-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 02:21:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012320CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 24 08:33:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

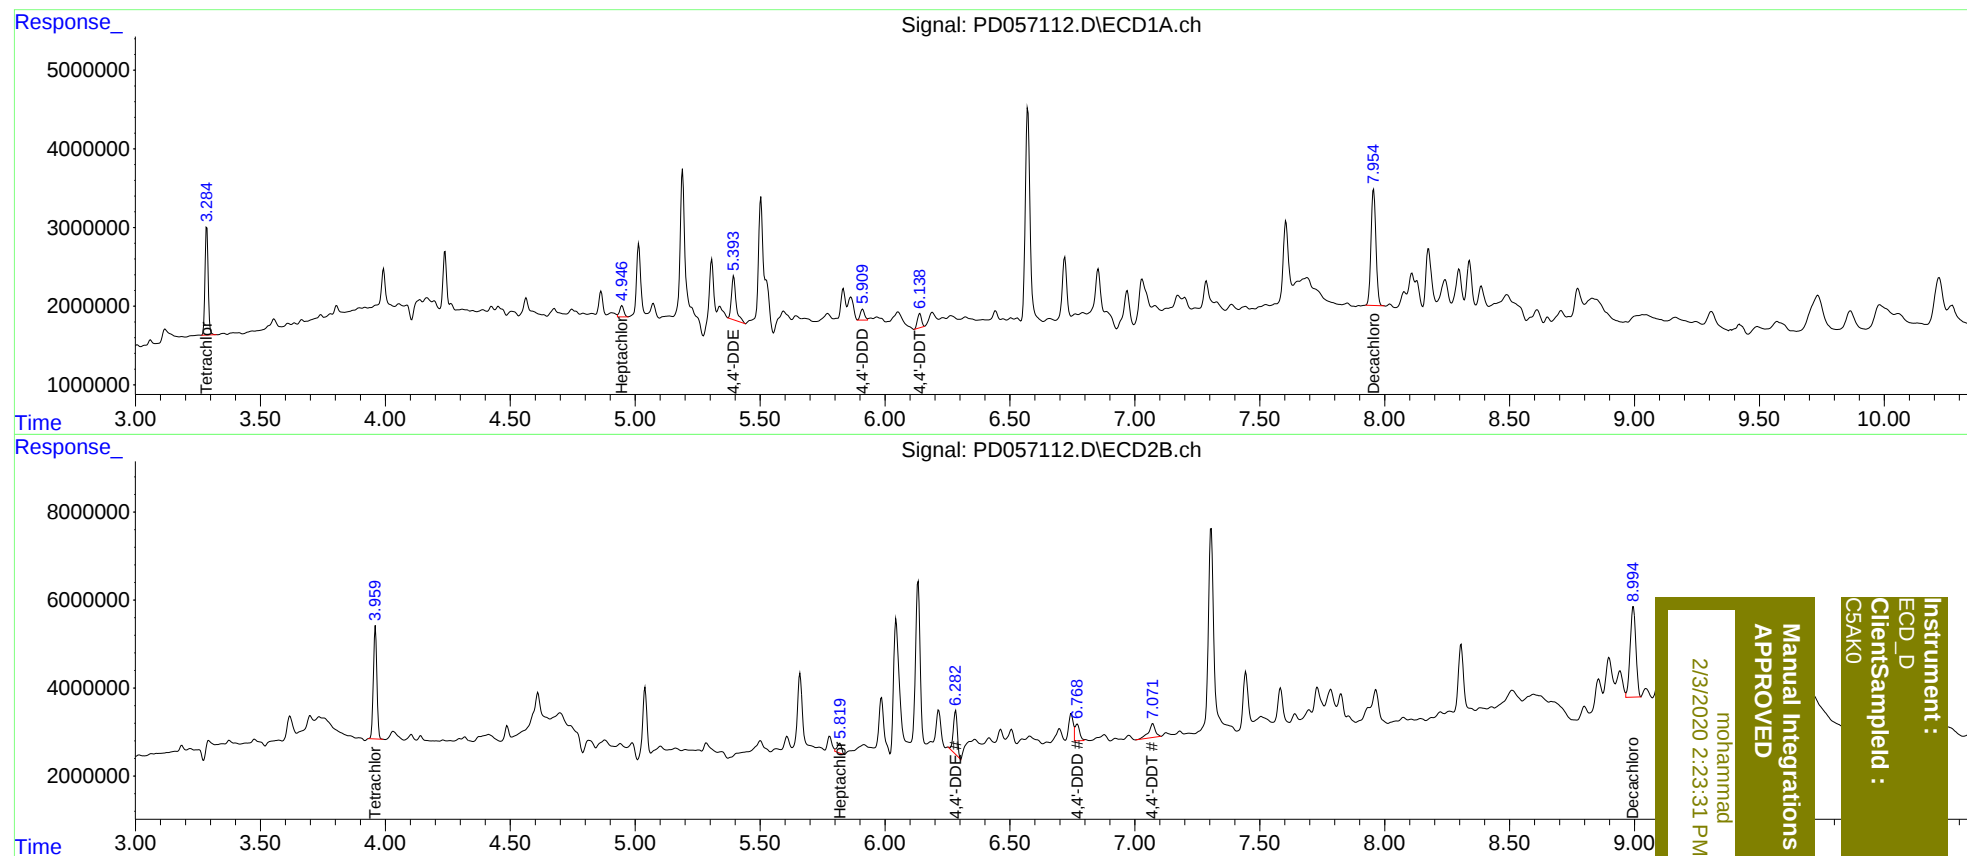

2/3/2020 2:23:31 PM

Manual Integrations
APPROVED

mohammad

Instrument :
ECD_D
ClientSampled :
C5AK0