

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD013123\
 Data File : PD073794.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2023 08:45
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 20:34:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 25 02:23:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
3) MA	gamma-BHC...	0.000	3.655f	0	79918	N.D. <MDL
4) MA	Heptachlor	0.000	3.973	0	141598	N.D. <MDL
5) MB	Aldrin	0.000	4.216	0	139027	N.D. <MDL
6) B	beta-BHC	4.487f	3.889	127818	149851	<MDL 0.183 #
7) B	delta-BHC	4.791	0.000	945979	0	0.289 N.D. #
8) B	Heptachlo...	5.712	0.000	1903568	0	0.585 N.D. #
14) MA	Endrin	6.541f	0.000	26086	0	<MDL N.D. #
15) B	Endosulfa...	6.804	0.000	183115	0	<MDL N.D. #
20) A	Methoxychlor	7.455f	0.000	828500	0	0.557 N.D. #
22)	Toxaphene-1	6.283	0.000	266204	0	11.829 N.D. #
23)	Toxaphene-2	6.510f	0.000	207655	0	7.055 N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD013123\
Data File : PD073794.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2023 08:45
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 20:34:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jan 25 02:23:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

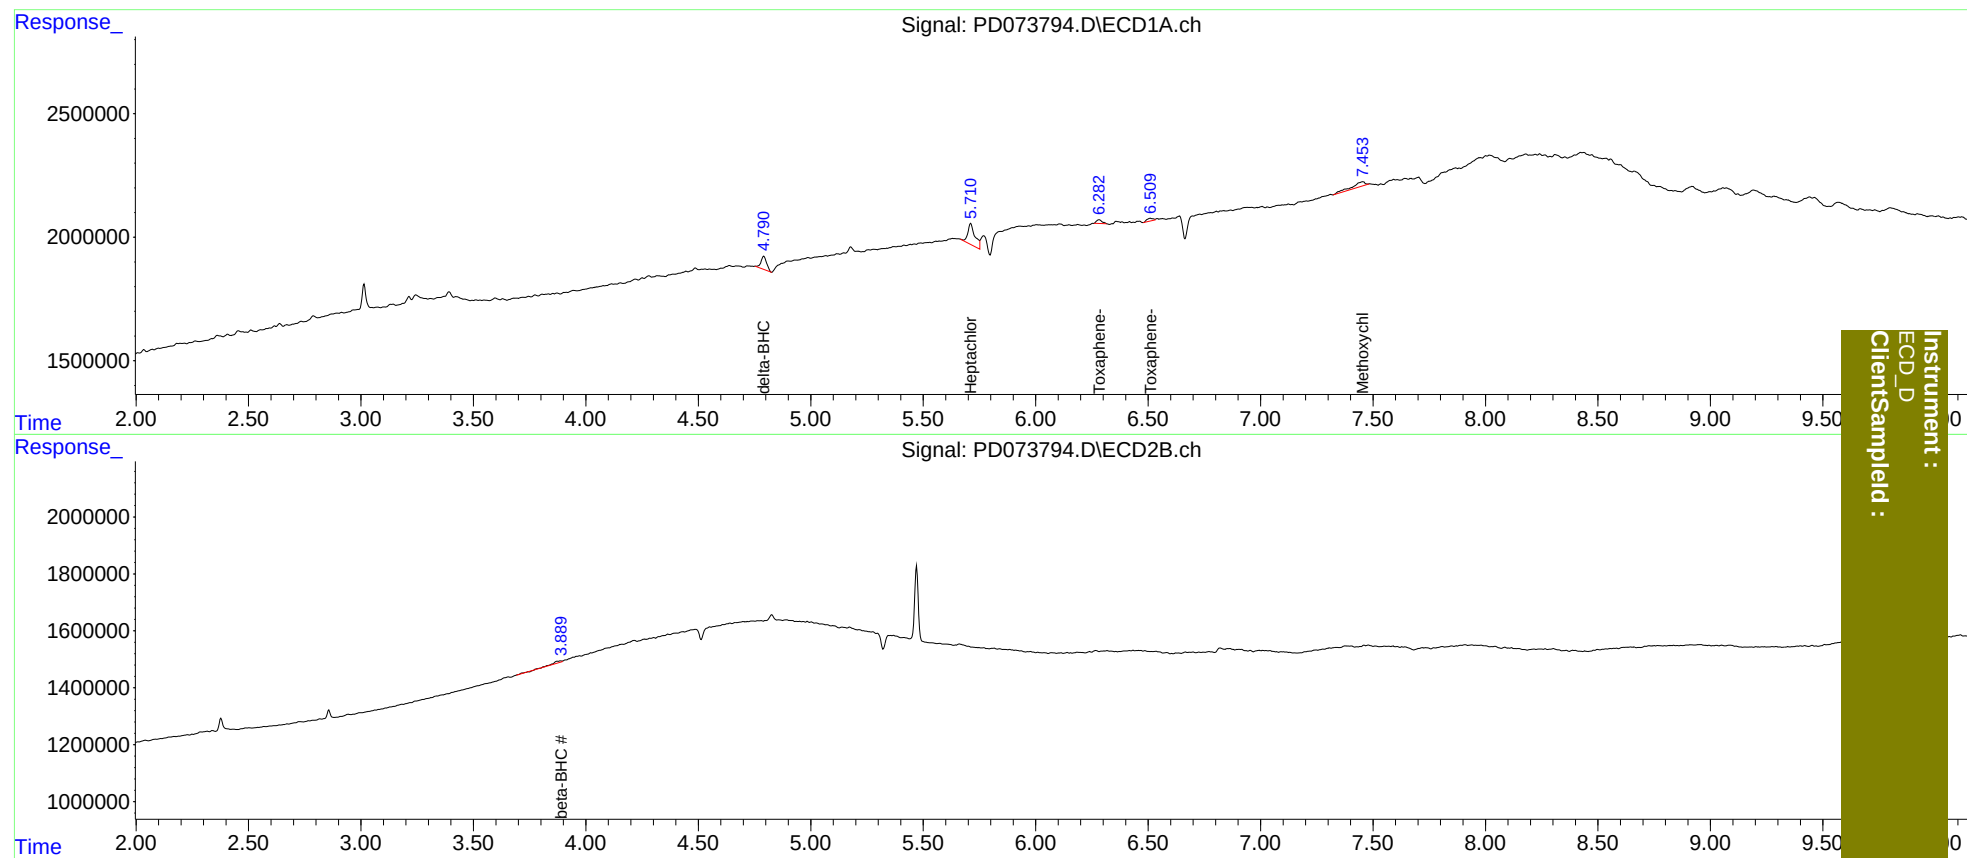


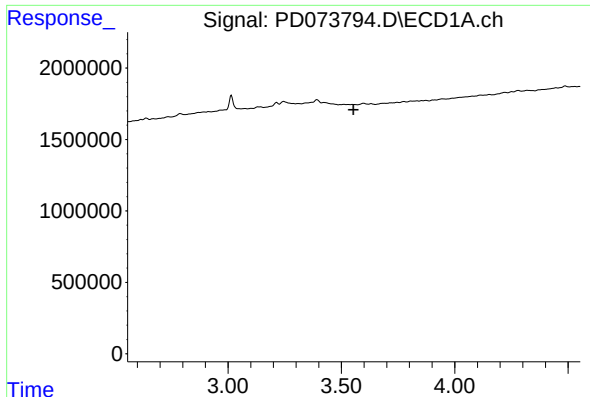

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.554 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

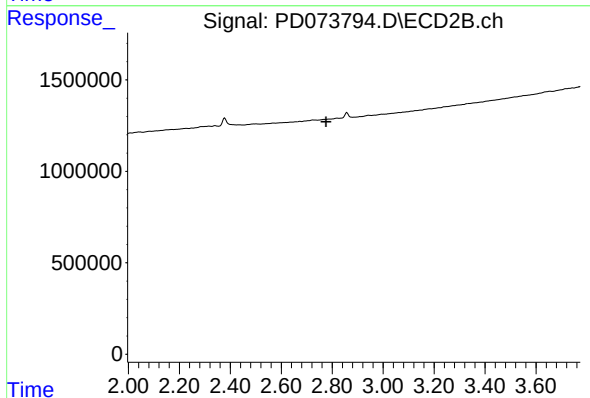


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.776 min
Response: 0
Conc: N.D.

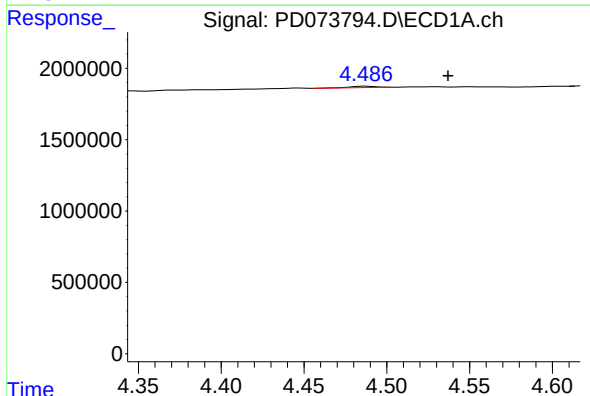


#6 beta-BHC

R.T.: 4.487 min
Delta R.T.: -0.050 min
Response: 127818
Conc: N.D.

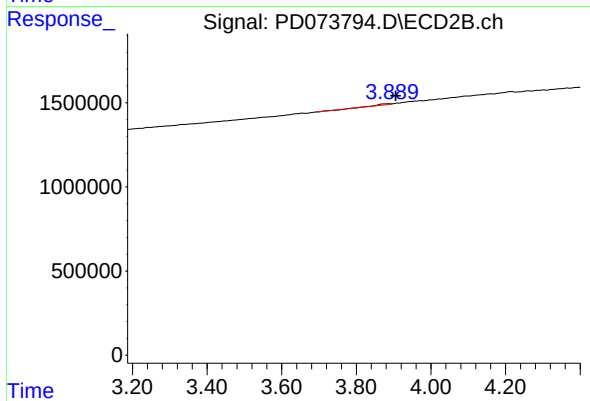

#6 beta-BHC


R.T.: 3.889 min
Delta R.T.: -0.017 min
Response: 149851
Conc: 0.18 ng/ml

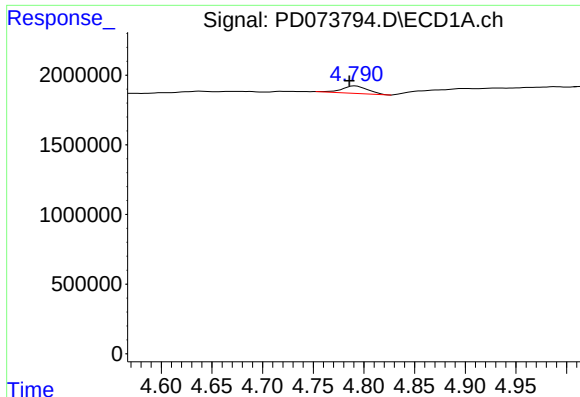

#7 delta-BHC


R.T.: 4.791 min
Delta R.T.: 0.006 min
Response: 945979
Conc: 0.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

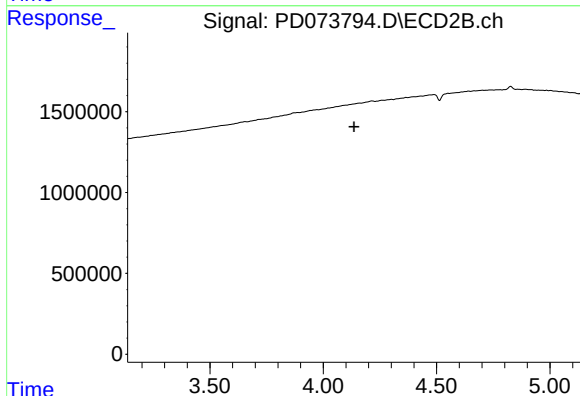


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.137 min
Response: 0
Conc: N.D.

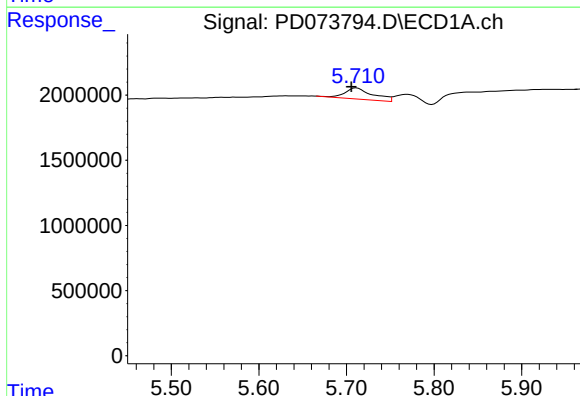


#8 Heptachlor epoxide

R.T.: 5.712 min
Delta R.T.: 0.006 min
Response: 1903568
Conc: 0.59 ng/ml

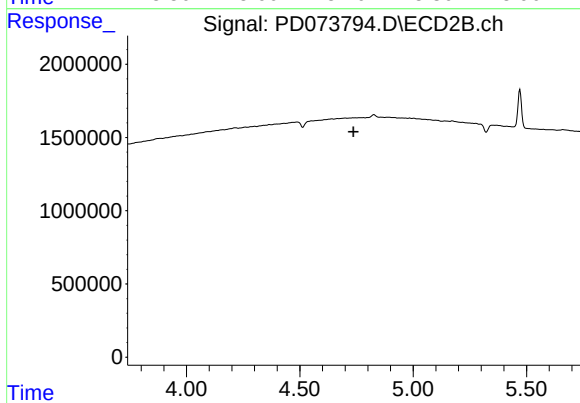

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.737 min
Response: 0
Conc: N.D.

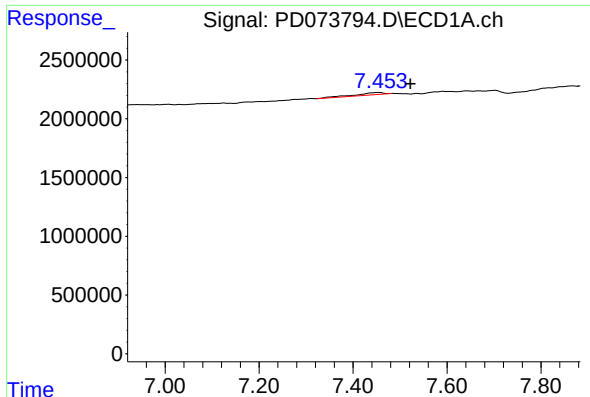

#20 Methoxychlor


R.T.: 7.455 min
Delta R.T.: -0.067 min
Response: 828500
Conc: 0.56 ng/ml

Instrument :
ECD_D
ClientSampleId :

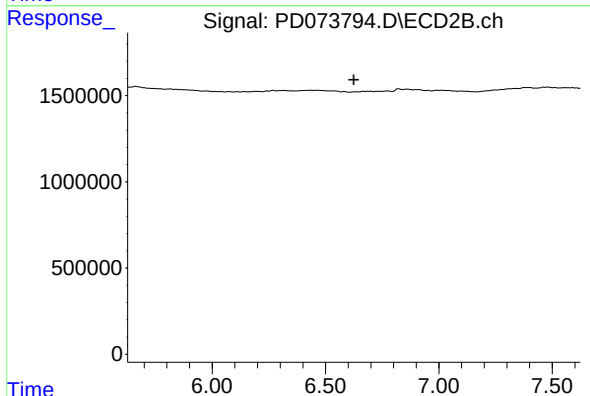


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.625 min
Response: 0
Conc: N.D.

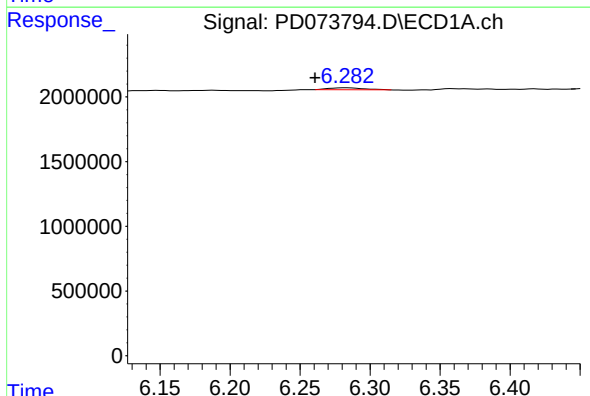


#22 Toxaphene-1

R.T.: 6.283 min
Delta R.T.: 0.022 min
Response: 266204
Conc: 11.83 ng/ml

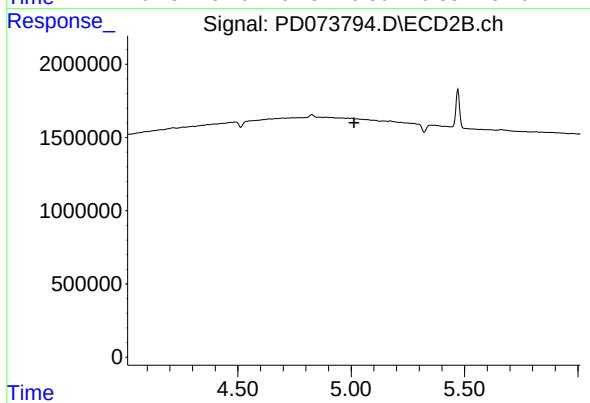

#22 Toxaphene-1


R.T.: 0.000 min
Exp R.T. : 5.013 min
Response: 0
Conc: N.D.

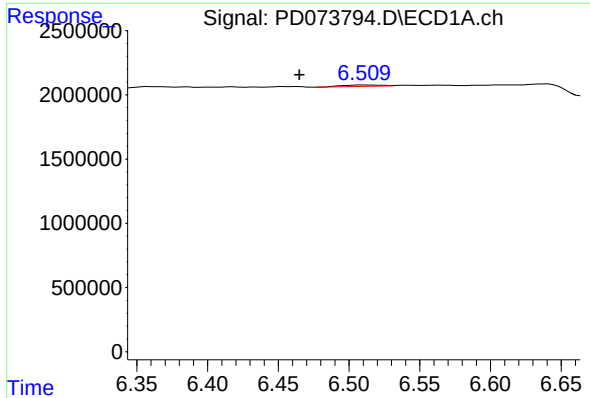

#23 Toxaphene-2


R.T.: 6.510 min
Delta R.T.: 0.045 min
Response: 207655
Conc: 7.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

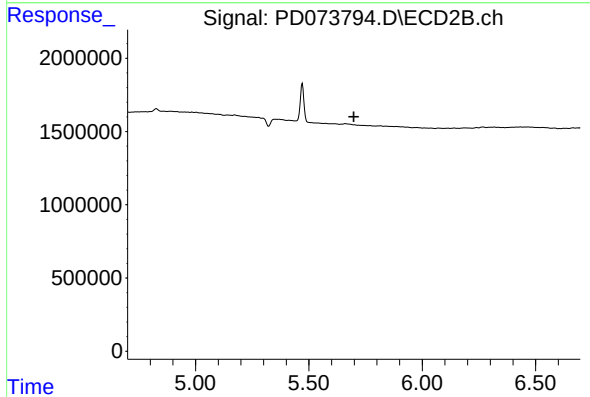


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T. : 5.698 min
Response: 0
Conc: N.D.

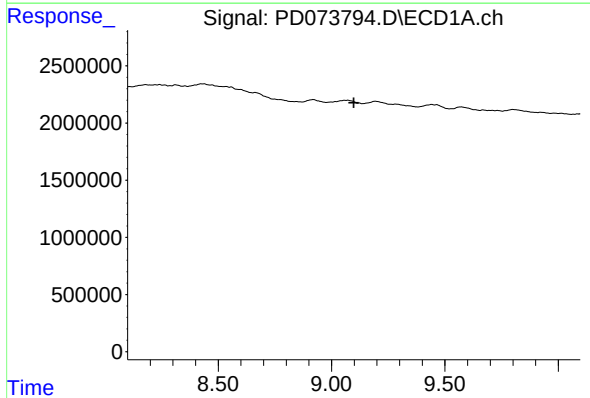

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.098 min
Response: 0
Conc: N.D.

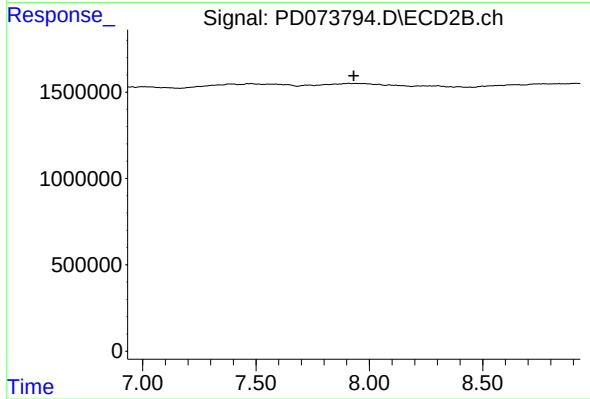

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.932 min
Response: 0
Conc: N.D.