

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD013124\
 Data File : PD080983.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2024 15:08
 Operator : AR\AJ
 Sample : PB158727BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB158727BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 19:09:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.574	2.793	29781251	54021059	20.979	22.583
28)	SA Decachlor...	9.125f	7.935	41105890	58656121	20.426	22.021
Target Compounds							
2)	A alpha-BHC	4.039f	3.309	62428	36840	0.025	0.010 #
3)	MA gamma-BHC...	0.000	3.631	0	150611	N.D.	0.040 #
5)	MB Aldrin	0.000	4.266f	0	54639	N.D.	0.015 #
7)	B delta-BHC	4.803	0.000	1161664	0	0.463	N.D. #
13)	MA Dieldrin	6.398f	0.000	172772	0	0.078	N.D. #
14)	MA Endrin	0.000	5.676f	0	189960	N.D.	0.064 #
18)	B Endrin al...	0.000	6.101f	0	150628	N.D.	0.067 #
24)	Chlordane-2	0.000	4.381	0	13005	N.D.	0.106 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD013124\
Data File : PD080983.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2024 15:08
Operator : AR\AJ
Sample : PB158727BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB158727BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 19:09:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

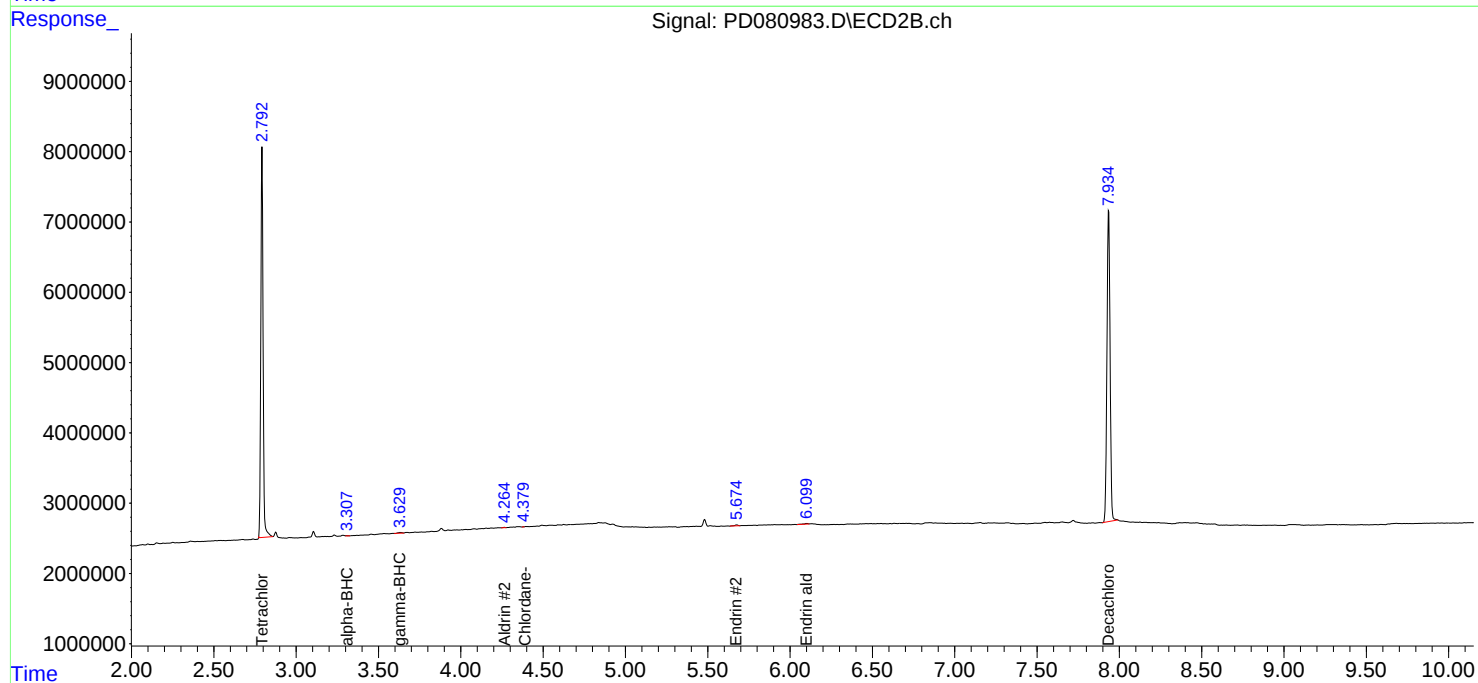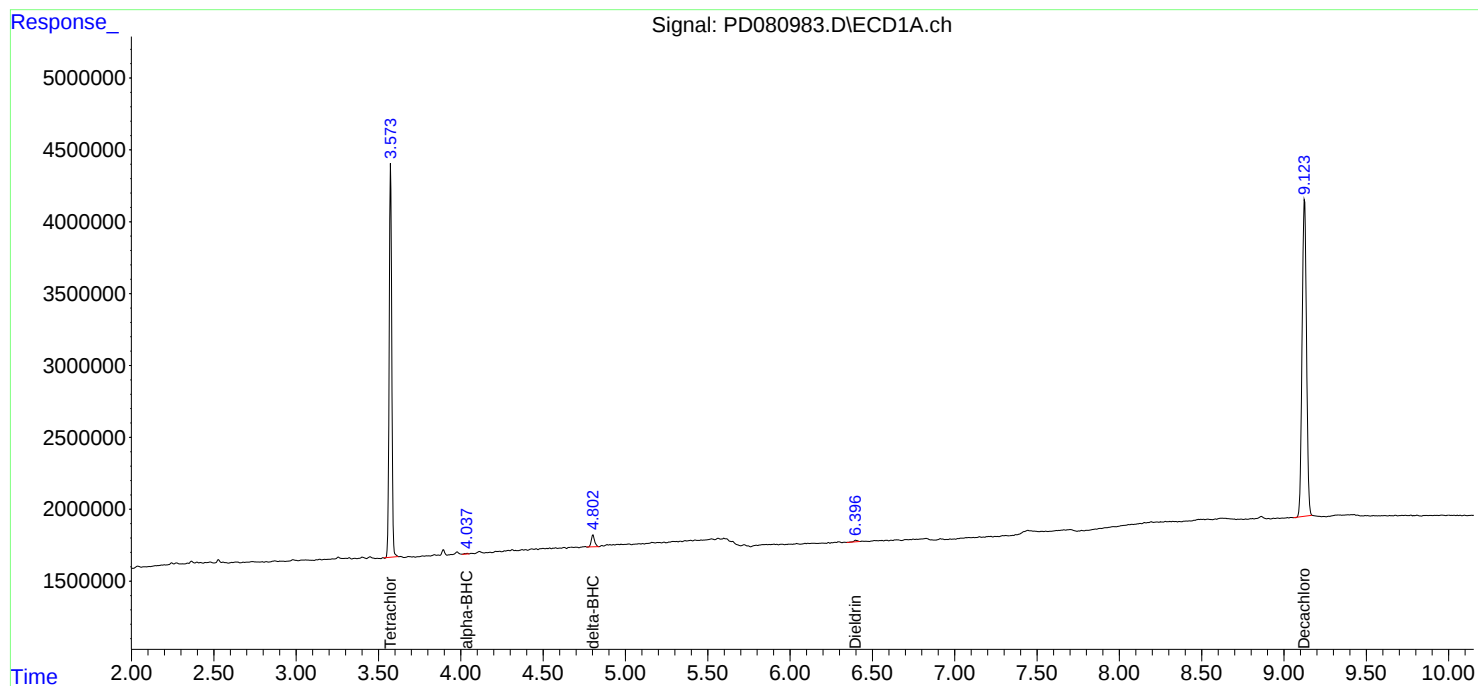


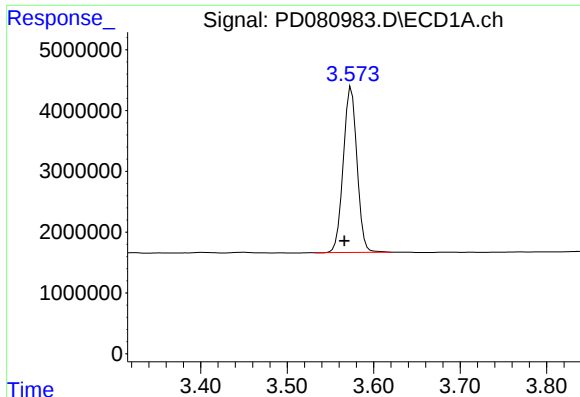

#1 Tetrachloro-m-xylene


R.T.: 3.574 min
Delta R.T.: 0.008 min
Response: 29781251
Conc: 20.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB158727BL

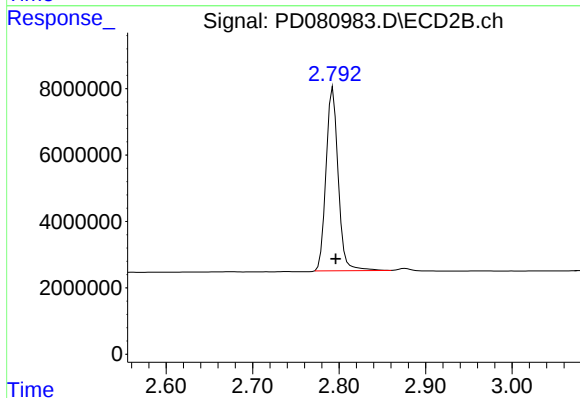


#1 Tetrachloro-m-xylene

R.T.: 2.793 min
Delta R.T.: -0.003 min
Response: 54021059
Conc: 22.58 ng/ml

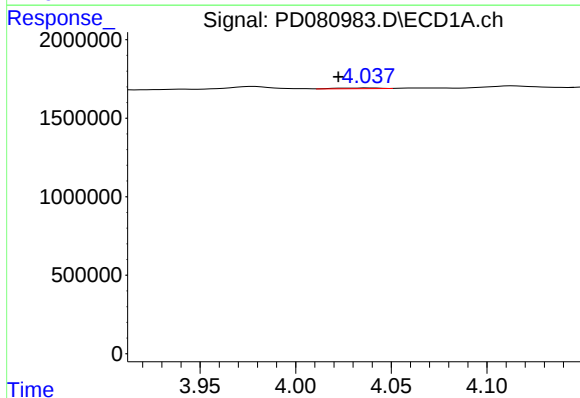


#2 alpha-BHC

R.T.: 4.039 min
Delta R.T.: 0.017 min
Response: 62428
Conc: 0.03 ng/ml

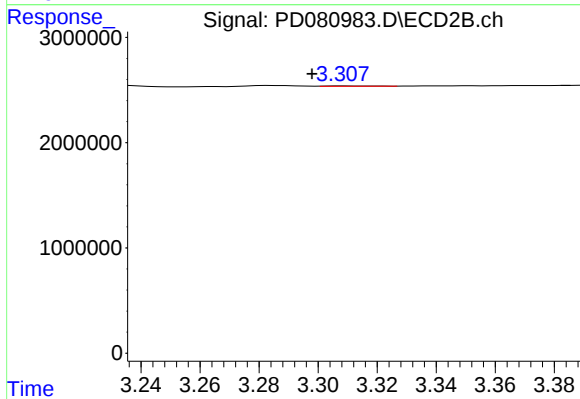

#2 alpha-BHC


R.T.: 3.309 min
Delta R.T.: 0.011 min
Response: 36840
Conc: 0.01 ng/ml

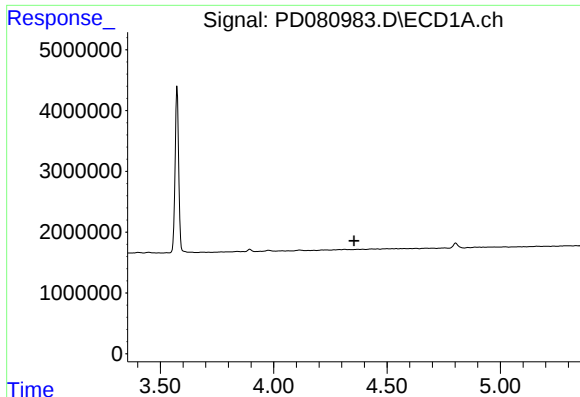

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.355 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB158727BL

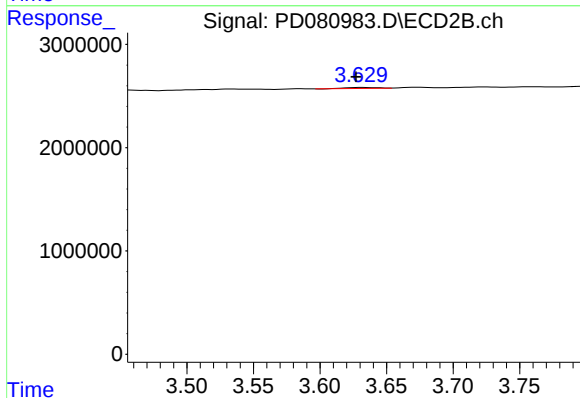


#3 gamma-BHC (Lindane)

R.T.: 3.631 min
Delta R.T.: 0.004 min
Response: 150611
Conc: 0.04 ng/ml

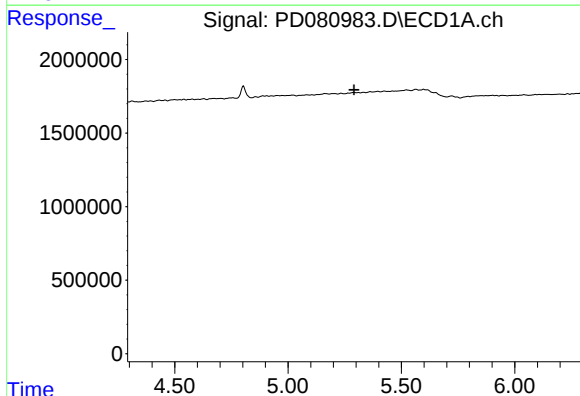


#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 5.292 min
Response: 0
Conc: N.D.

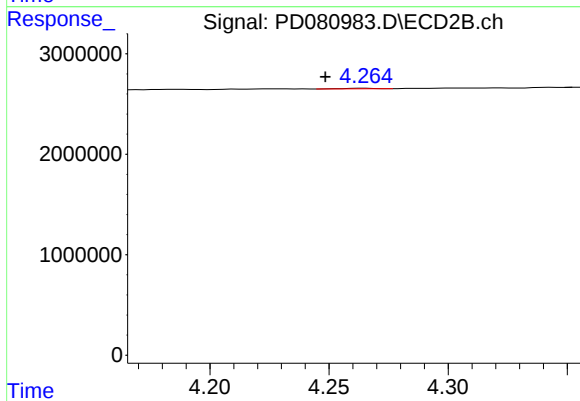

#5 Aldrin


R.T.: 4.266 min
Delta R.T.: 0.017 min
Response: 54639
Conc: 0.02 ng/ml

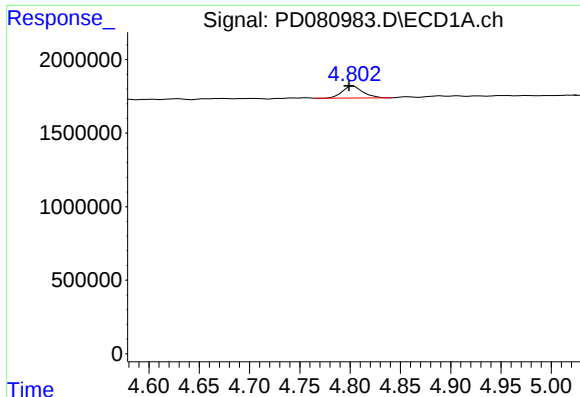

#7 delta-BHC


R.T.: 4.803 min
Delta R.T.: 0.004 min
Response: 1161664
Conc: 0.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB158727BL

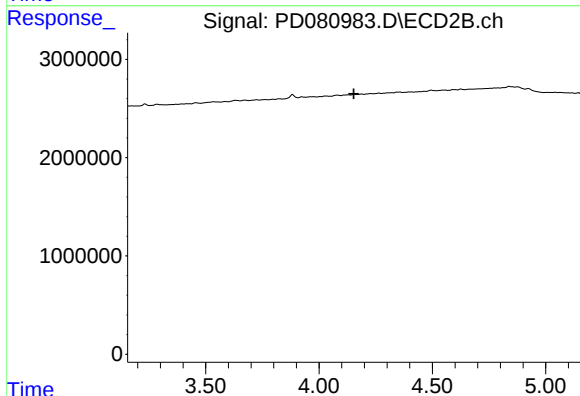


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.153 min
Response: 0
Conc: N.D.

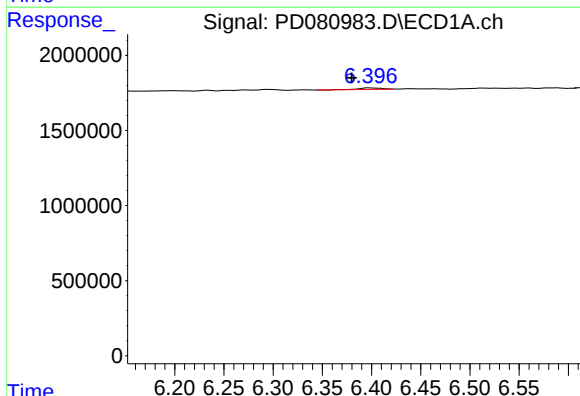


#13 Dieldrin

R.T.: 6.398 min
Delta R.T.: 0.018 min
Response: 172772
Conc: 0.08 ng/ml

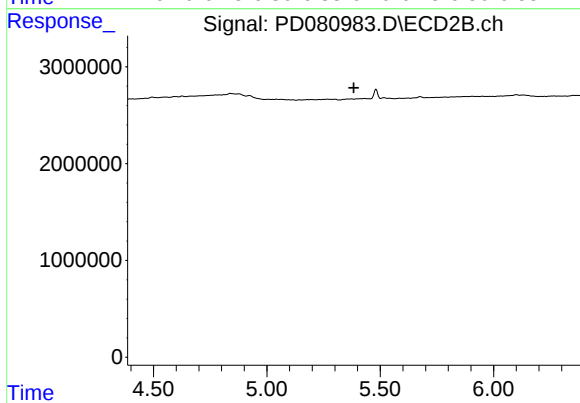

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 5.384 min
Response: 0
Conc: N.D.

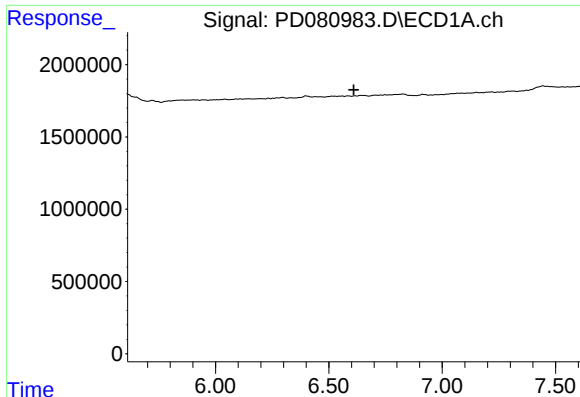

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.610 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB158727BL

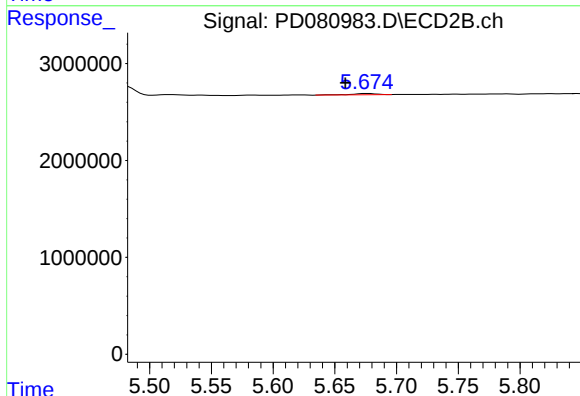


#14 Endrin

R.T.: 5.676 min
Delta R.T.: 0.017 min
Response: 189960
Conc: 0.06 ng/ml

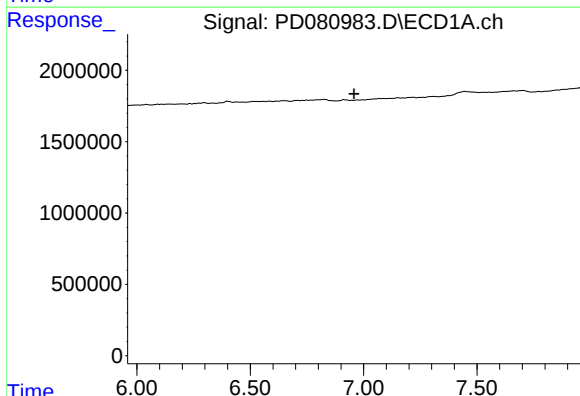


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.958 min
Response: 0
Conc: N.D.

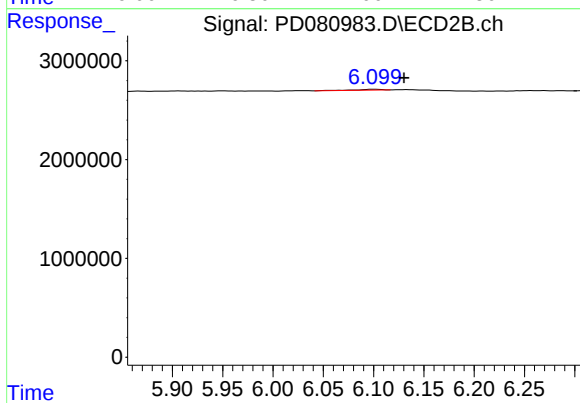

#18 Endrin aldehyde


R.T.: 6.101 min
Delta R.T.: -0.030 min
Response: 150628
Conc: 0.07 ng/ml

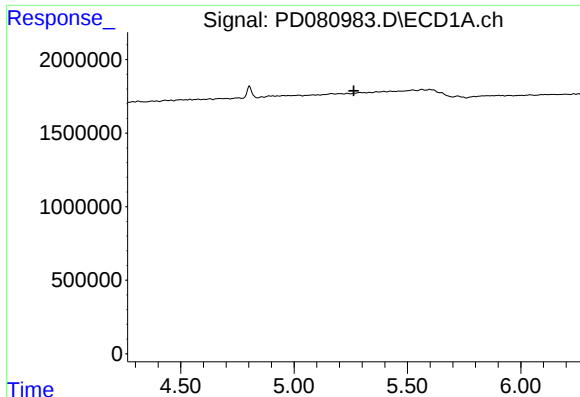

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.263 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB158727BL

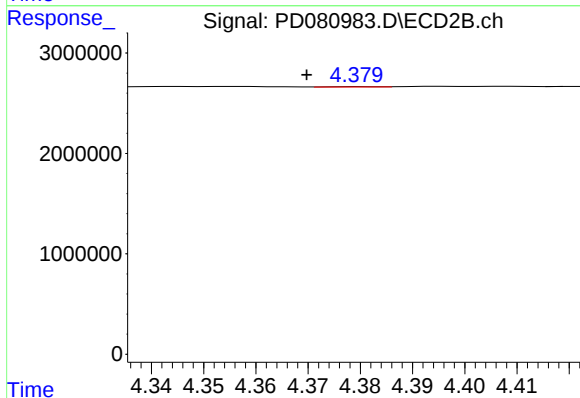


#24 Chlordane-2

R.T.: 4.381 min
Delta R.T.: 0.011 min
Response: 13005
Conc: 0.11 ng/ml

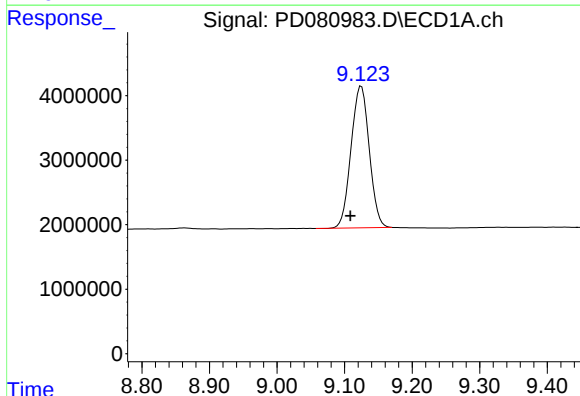

#28 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: 0.016 min
Response: 41105890
Conc: 20.43 ng/ml

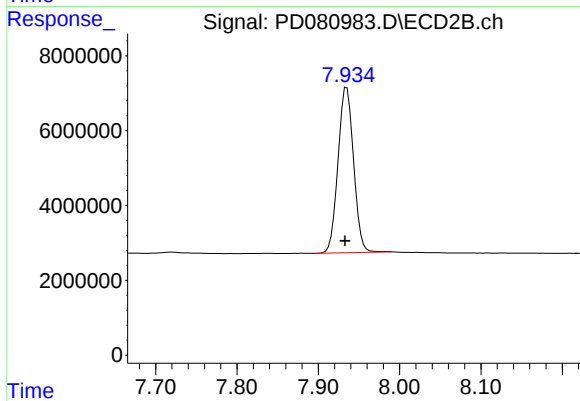

#28 Decachlorobiphenyl

R.T.: 7.935 min
Delta R.T.: 0.002 min
Response: 58656121
Conc: 22.02 ng/ml