

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD013125\
 Data File : PD087626.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2025 13:04
 Operator : AR\AJ
 Sample : Q1197-03MSD
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E2964MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/03/2025
 Supervised By : Ankita Jodhani 02/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 08:07:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 16 13:39:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.554	2.881	29960275	213.4E6	14.701m	17.257m
2) SA Decachlor...	9.083	8.082	37198174	114.6E6	11.126m	7.909m#
Target Compounds						
2) A alpha-BHC	4.005	3.397	182.1E6	926.3E6	43.829m	46.777m
3) MA gamma-BHC...	4.335	3.732	167.3E6	621.5E6	41.585m	33.933m
4) MA Heptachlor	4.936	4.088	165.3E6	821.6E6	40.439m	44.020m
5) MB Aldrin	5.278	4.373	142.4E6	716.1E6	35.555m	39.618m
6) B beta-BHC	4.520	4.027	55743689	239.0E6	31.037m	28.018m
7) B delta-BHC	4.769	4.265	215.9E6	682.6E6	52.246m	36.572m#
8) B Heptachlo...	5.699	4.878	306.7E6	553.7E6	82.089	32.714m#
9) A Endosulfan I	6.082	5.254	261.7E6	610.2E6	75.112m	38.445 #
10) B trans-Chl...	5.954	5.130	165.6E6	738.6E6	44.953m	41.086m
11) B cis-Chlor...	6.032	5.196	175.2E6	715.6E6	47.134m	41.348
12) B 4,4'-DDE	6.202	5.382	286.0E6	845.2E6	81.202m	51.601 #
13) MA Dieldrin	6.356	5.519	343.4E6	1102.4E6	90.079	66.051m#
14) MA Endrin	6.583	5.795	367.8E6	785.6E6	113.310m	52.578m#
15) B Endosulfa...	6.792	6.088	320.1E6	758.2E6	99.438m	51.182 #
16) A 4,4'-DDD	6.712	5.935	209.7E6	944.6E6	76.275m	70.653m
17) MA 4,4'-DDT	7.030	6.190	206.8E6	755.5E6	71.371	54.823m
18) B Endrin al...	6.922	6.266	125.4E6	409.0E6	49.754m	35.479 #
19) B Endosulfa...	7.156	6.490	205.1E6	814.9E6	66.446m	56.059
20) A Methoxychlor	7.502	6.763	652.6E6	2191.0E6	411.888	355.716
21) B Endrin ke...	7.638	6.998	289.0E6	922.7E6	83.941m	58.098m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD013125\
Data File : PD087626.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2025 13:04
Operator : AR\AJ
Sample : Q1197-03MSD
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 08:07:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 16 13:39:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

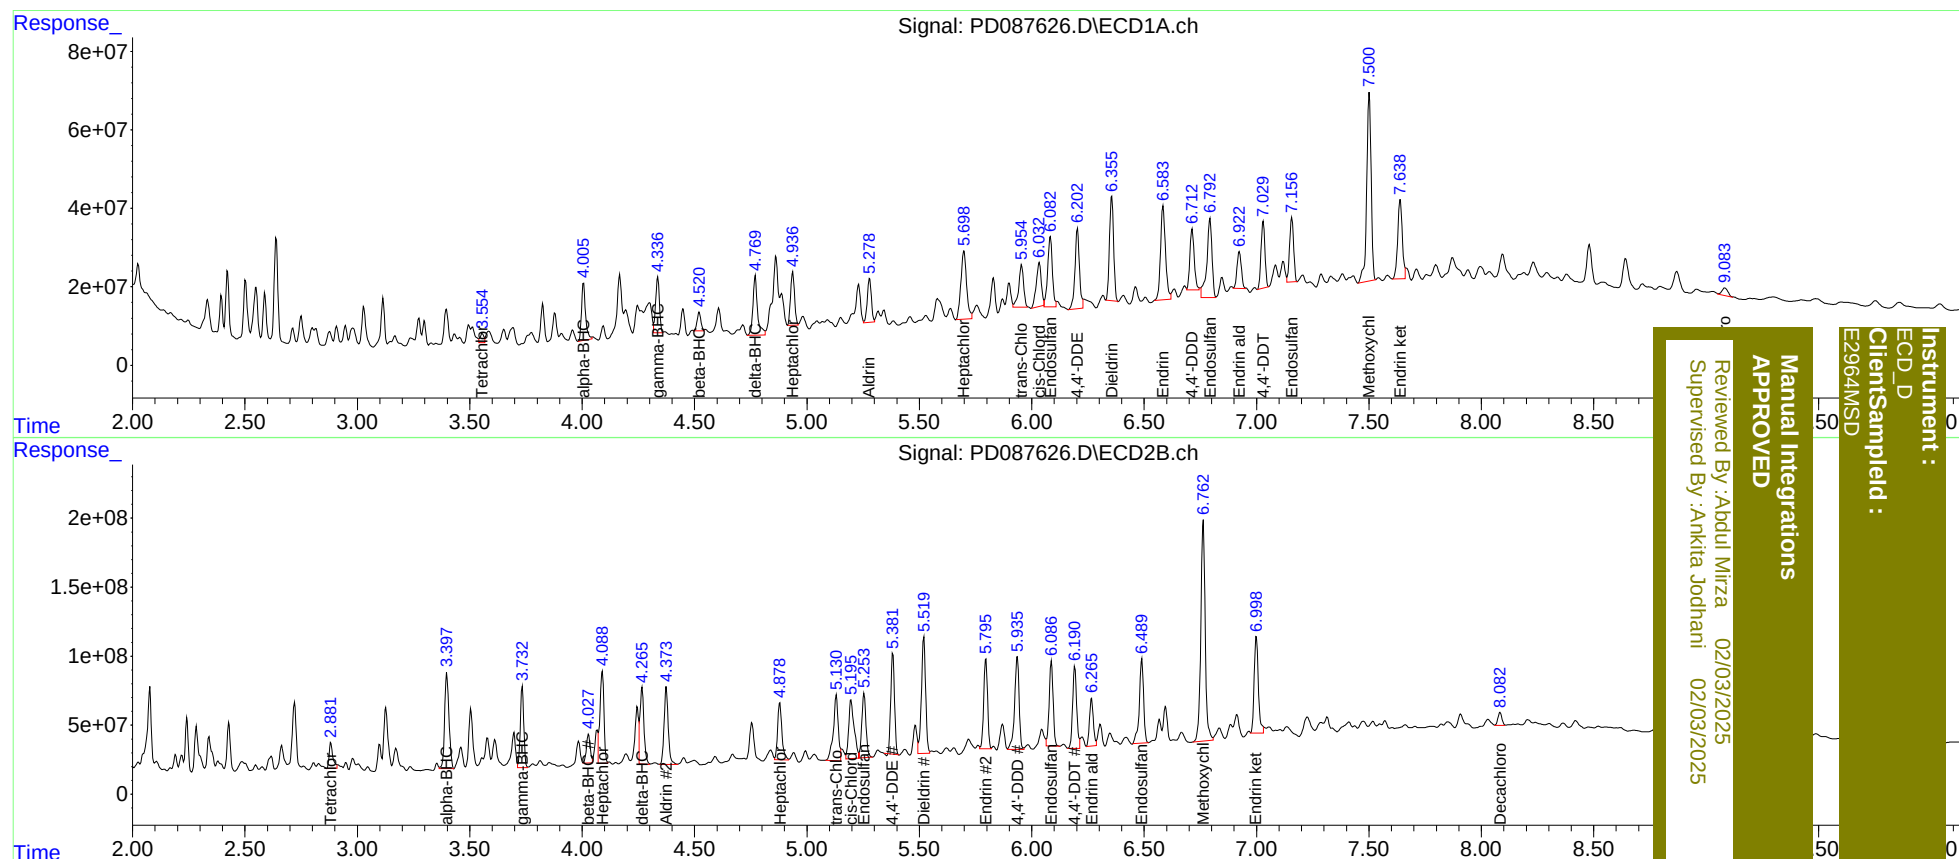

Instrument :
ECD_D
ClientSampled :
E2964MSD

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/03/2025
Supervised By :Ankita Jodhani 02/03/2025