

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020124\
 Data File : PD081015.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2024 16:15
 Operator : AR\AJ
 Sample : P1313-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COMP-1

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/02/2024
 Supervised By : Ankita Jodhani 02/02/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 21:12:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.566	2.796	16086995	27287595	11.332	11.407
2) SA Decachlor...	9.113	7.935	9813891	15818707	4.877	5.939
Target Compounds						
13) MA Dieldrin	6.382	5.384	7844902	15320932	3.550	4.505m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020124\
Data File : PD081015.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2024 16:15
Operator : AR\AJ
Sample : P1313-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
COMP-1


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/02/2024
Supervised By : Ankita Jodhani 02/02/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 21:12:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

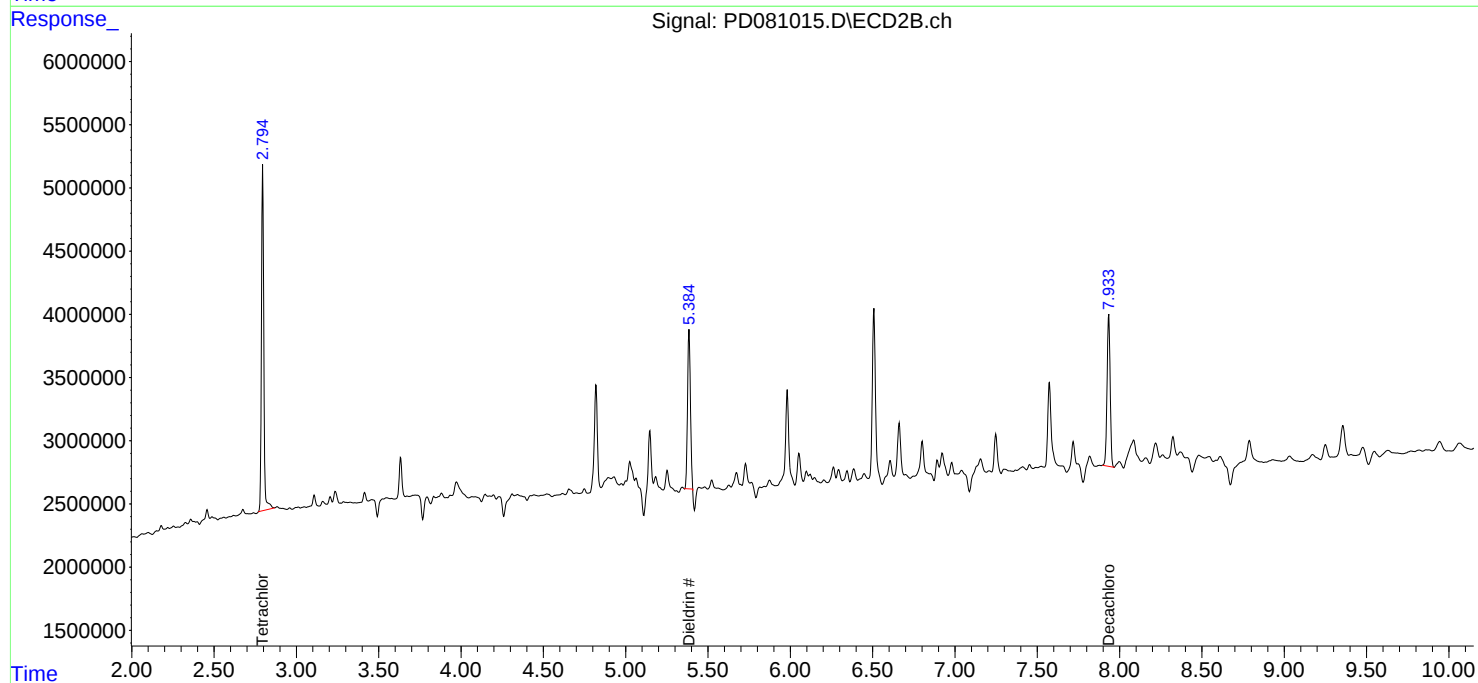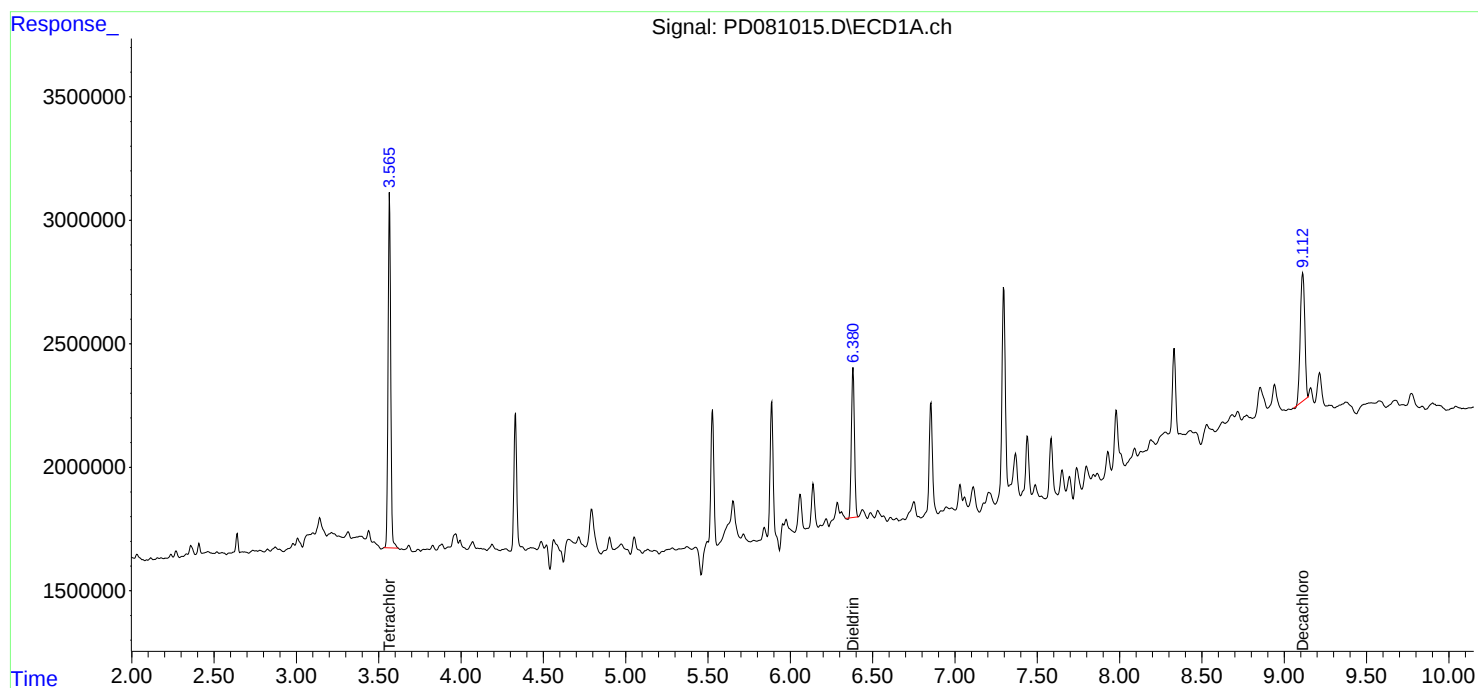

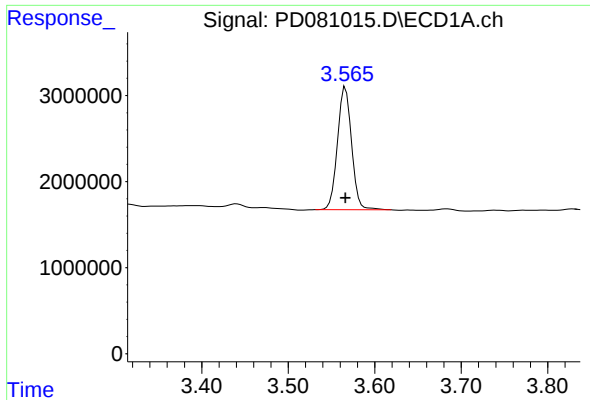


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 16086995
Conc: 11.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-1


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/02/2024
Supervised By :Ankita Jodhani 02/02/2024

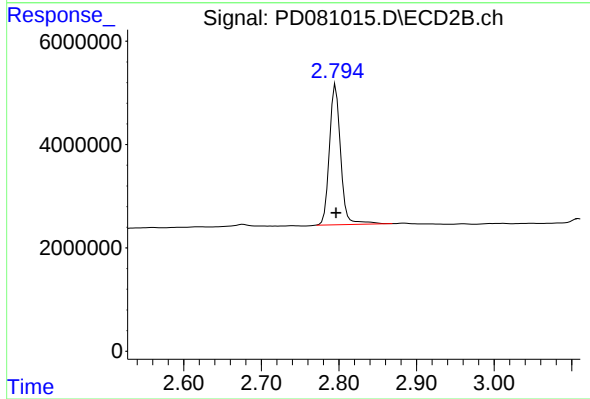


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 27287595
Conc: 11.41 ng/ml

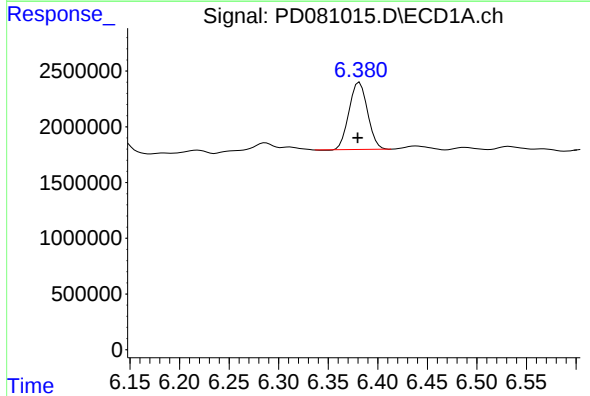


#13 Dieldrin

R.T.: 6.382 min
Delta R.T.: 0.002 min
Response: 7844902
Conc: 3.55 ng/ml

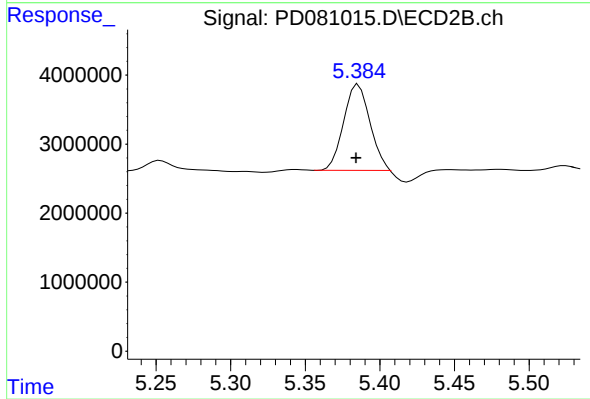

#13 Dieldrin

R.T.: 5.384 min
Delta R.T.: 0.000 min
Response: 15320932
Conc: 4.51 ng/ml m

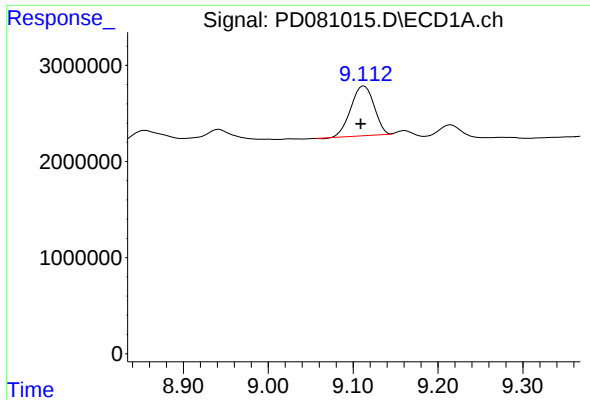


#28 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: 0.004 min
Response: 9813891
Conc: 4.88 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-1

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/02/2024
Supervised By :Ankita Jodhani 02/02/2024

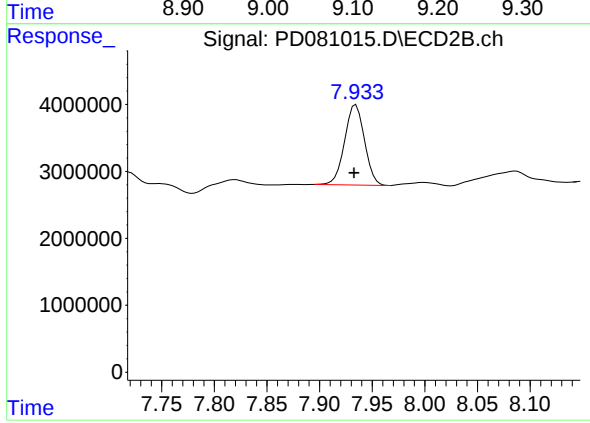

#28 Decachlorobiphenyl

R.T.: 7.935 min
Delta R.T.: 0.002 min
Response: 15818707
Conc: 5.94 ng/ml