

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020124\
 Data File : PD081016.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2024 16:28
 Operator : AR\AJ
 Sample : P1313-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COMP-2

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/02/2024
 Supervised By :Ankita Jodhani 02/02/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 21:13:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.567	2.796	24724669	42792238	17.417	17.889
2) SA Decachlor...	9.113	7.934	14705921	22624645	7.307m	8.494m
Target Compounds						
13) MA Dieldrin	6.381	5.387	3667872	8885203	1.660m	2.613m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020124\
Data File : PD081016.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2024 16:28
Operator : AR\AJ
Sample : P1313-02
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/02/2024
Supervised By : Ankita Jodhani 02/02/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 21:13:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

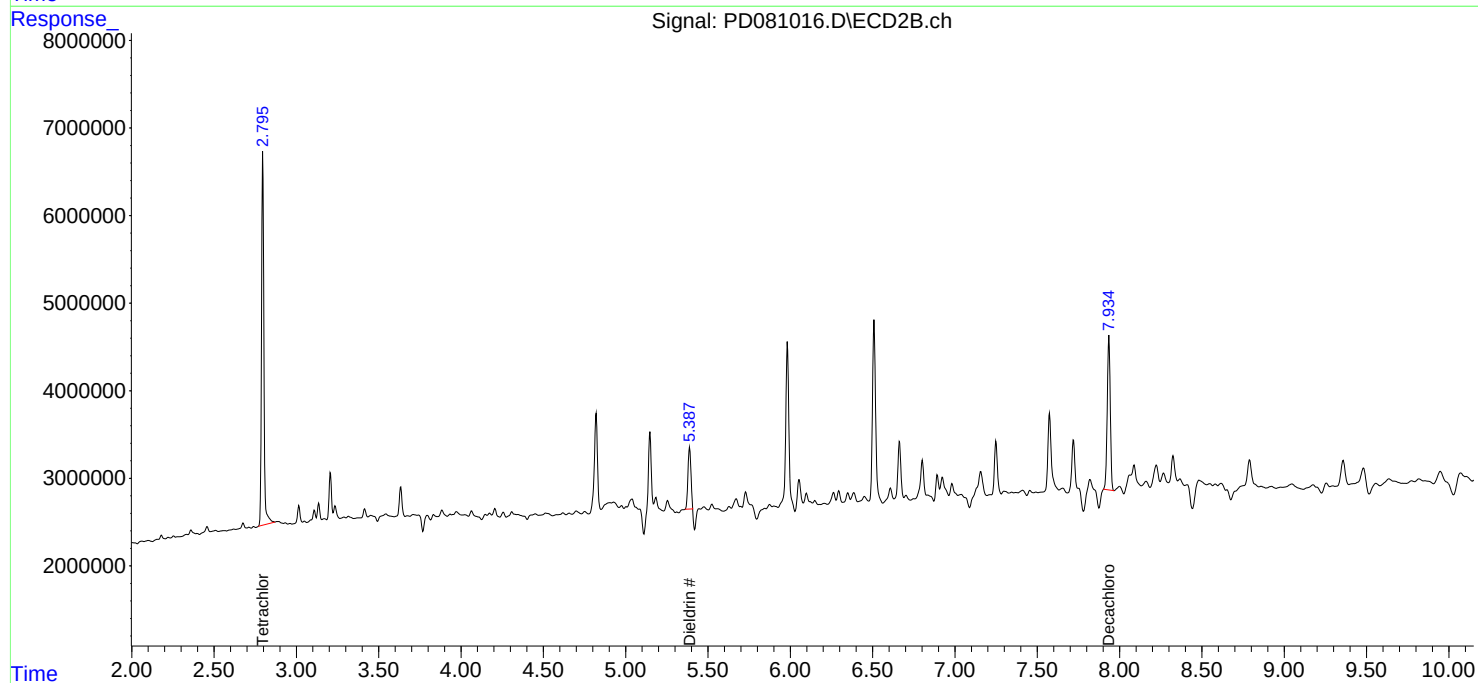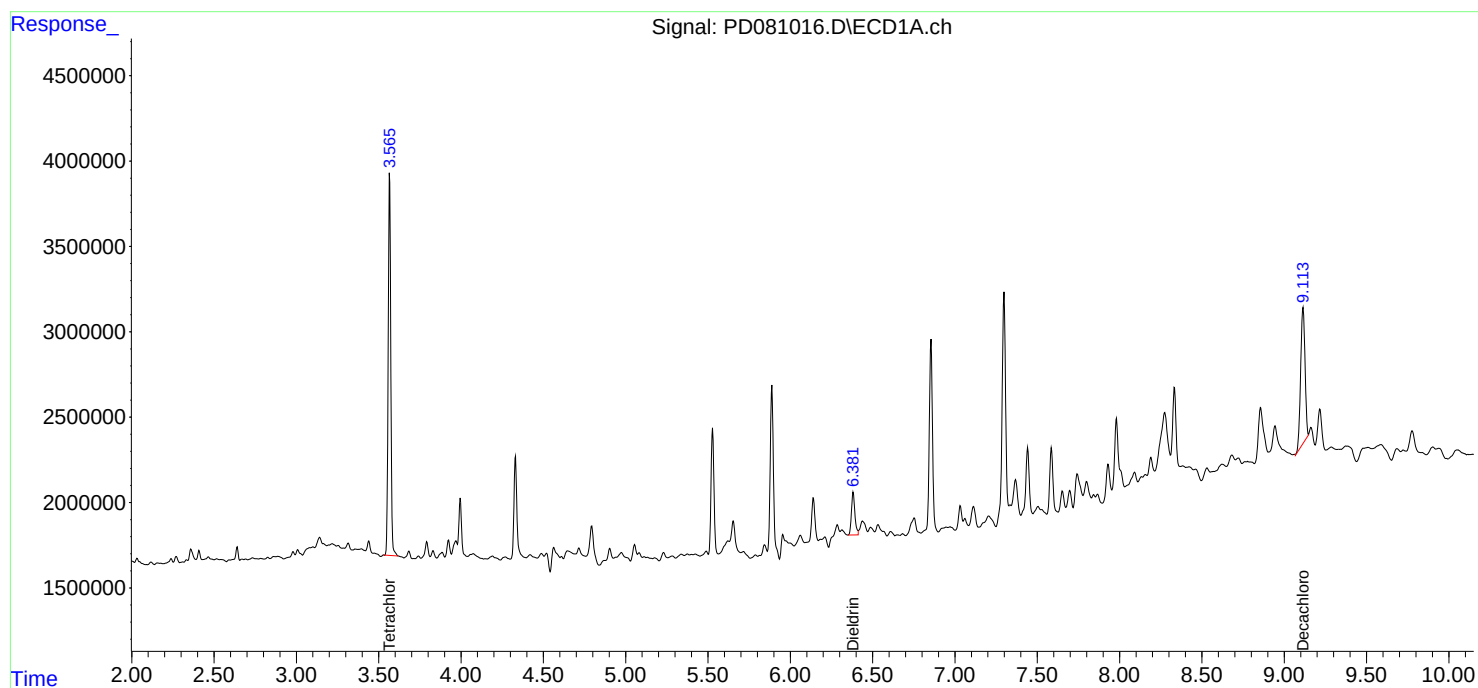

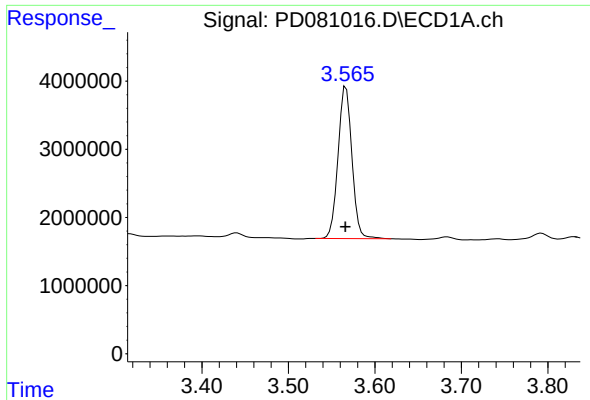


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: 0.000 min
Response: 24724669
Conc: 17.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/02/2024
Supervised By :Ankita Jodhani 02/02/2024

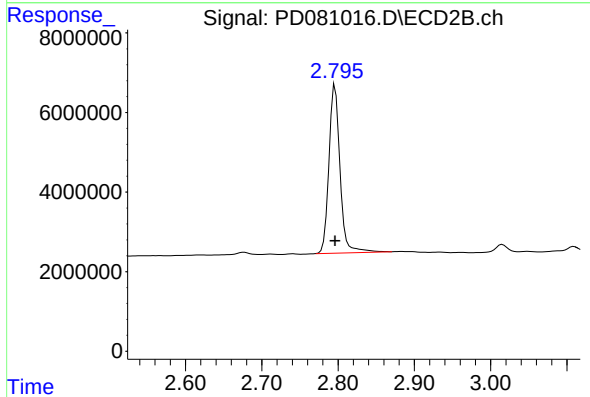


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 42792238
Conc: 17.89 ng/ml

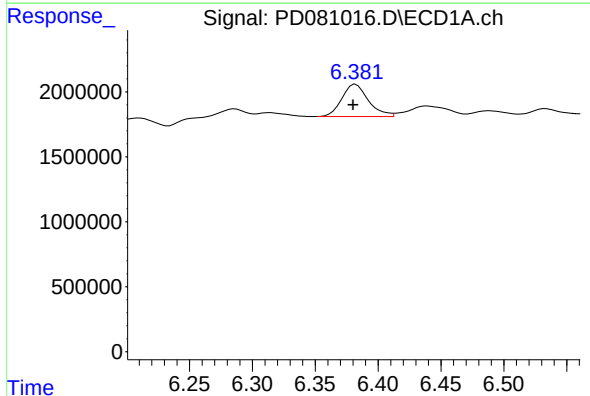


#13 Dieldrin

R.T.: 6.381 min
Delta R.T.: 0.000 min
Response: 3667872
Conc: 1.66 ng/ml m

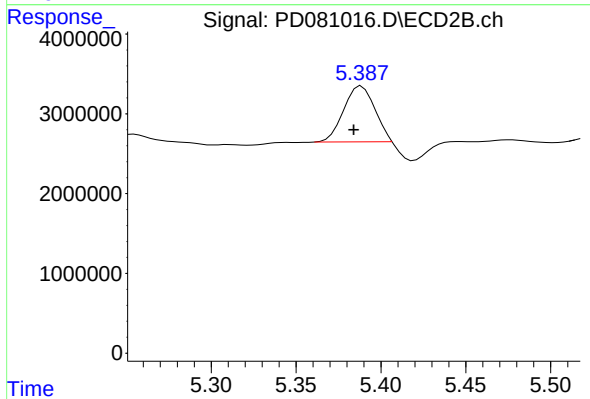

#13 Dieldrin

R.T.: 5.387 min
Delta R.T.: 0.003 min
Response: 8885203
Conc: 2.61 ng/ml m

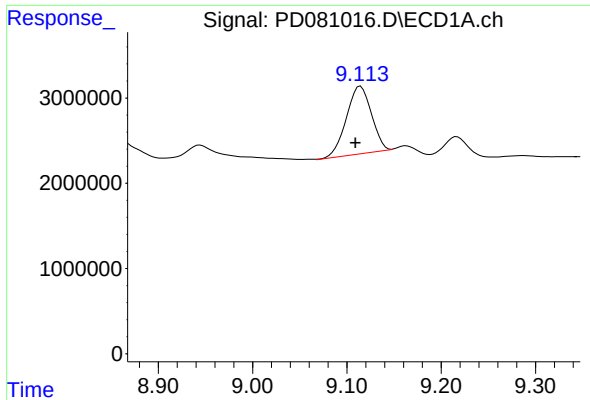


#28 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: 0.004 min
Response: 14705921
Conc: 7.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/02/2024
Supervised By :Ankita Jodhani 02/02/2024

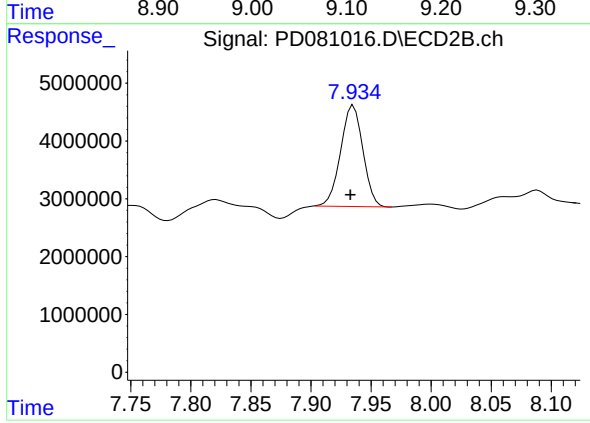

#28 Decachlorobiphenyl

R.T.: 7.934 min
Delta R.T.: 0.001 min
Response: 22624645
Conc: 8.49 ng/ml m