

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020124\
 Data File : PD081017.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2024 16:42
 Operator : AR\AJ
 Sample : P1316-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COMP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 21:15:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.796	14202808	24623751	10.005	10.294
28)	SA Decachlor...	9.115	7.935	20851075	30669836	10.361	11.514
Target Compounds							
12)	B 4,4'-DDE	6.225	5.253	2284962	1787333	1.123	0.583 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020124\
Data File : PD081017.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2024 16:42
Operator : AR\AJ
Sample : P1316-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 21:15:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

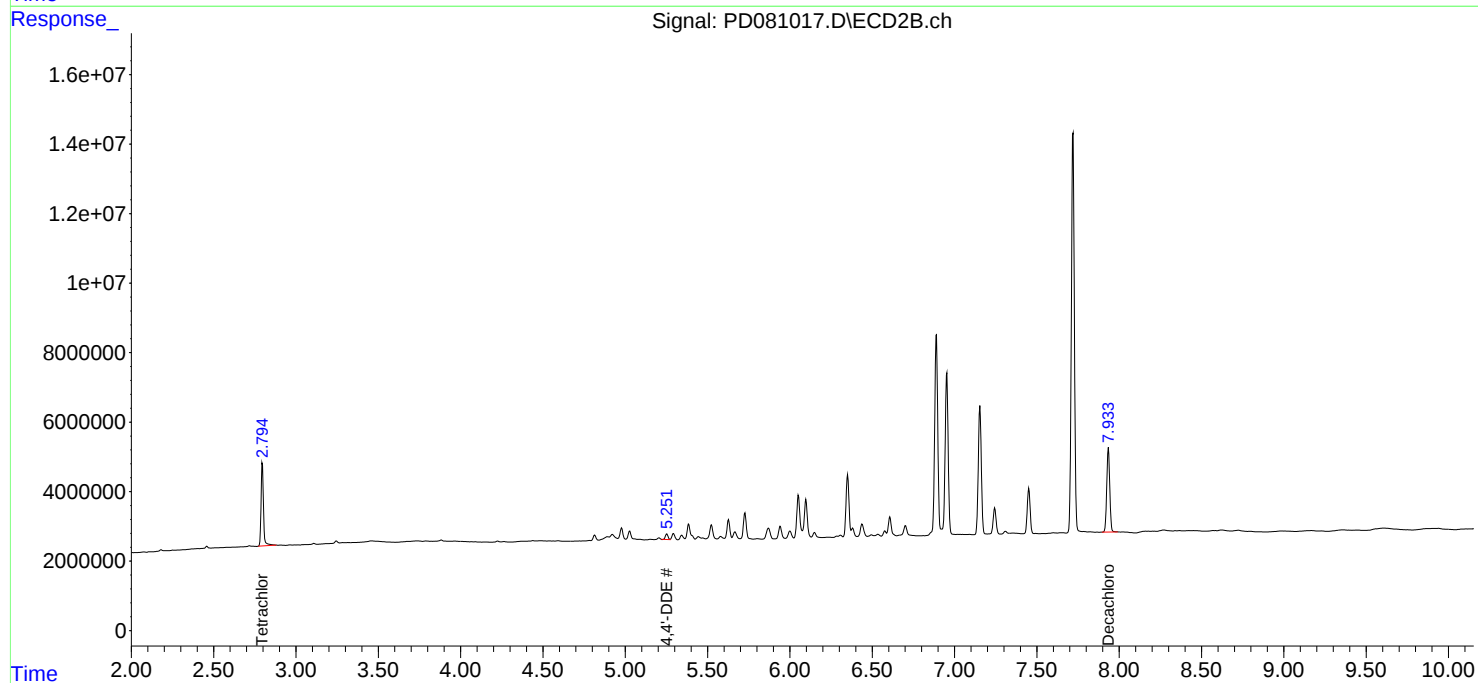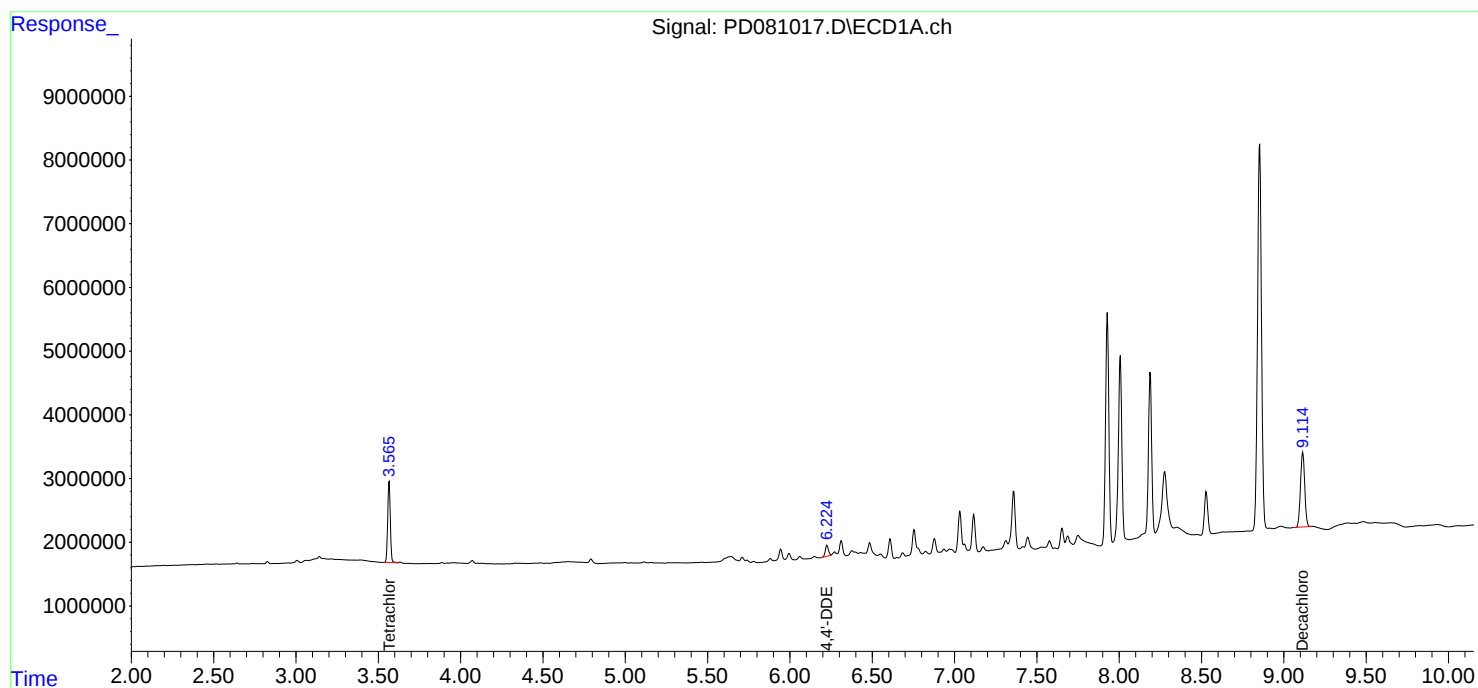


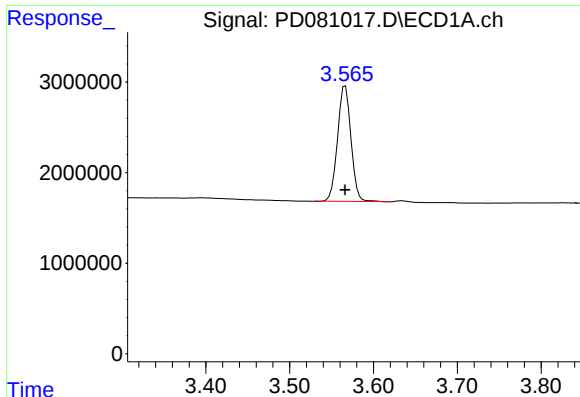

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 14202808
Conc: 10.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-1

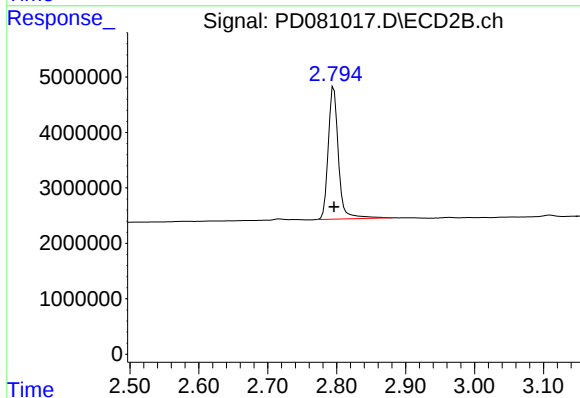


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 24623751
Conc: 10.29 ng/ml

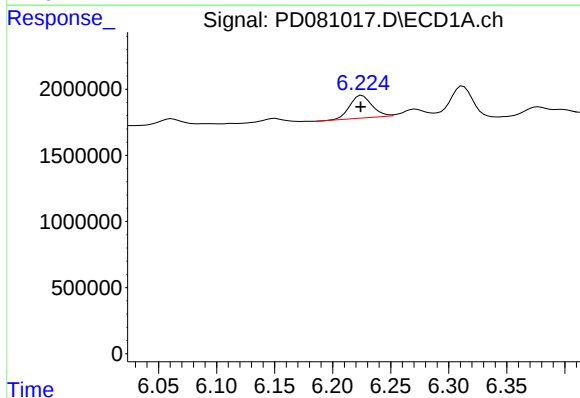


#12 4,4'-DDE

R.T.: 6.225 min
Delta R.T.: 0.001 min
Response: 2284962
Conc: 1.12 ng/ml

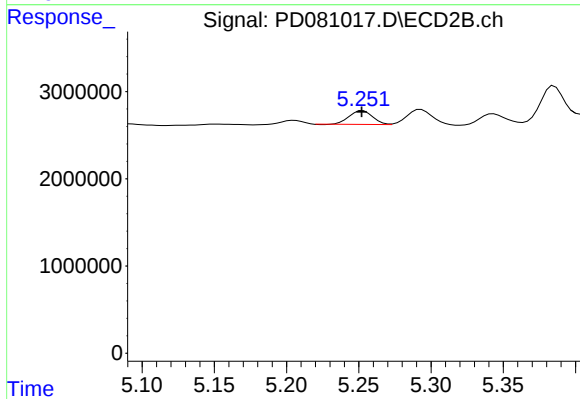

#12 4,4'-DDE

R.T.: 5.253 min
Delta R.T.: 0.000 min
Response: 1787333
Conc: 0.58 ng/ml

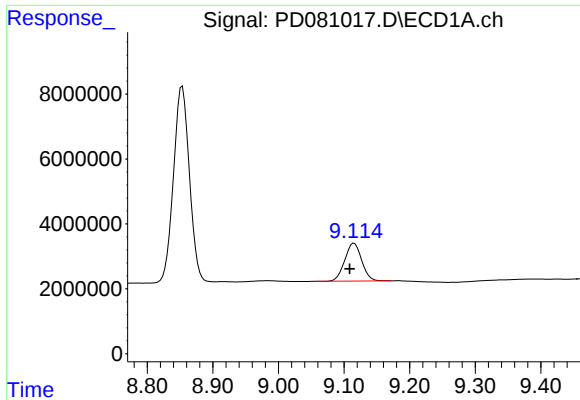

#28 Decachlorobiphenyl


R.T.: 9.115 min

Delta R.T.: 0.006 min

Response: 20851075

Conc: 10.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-1

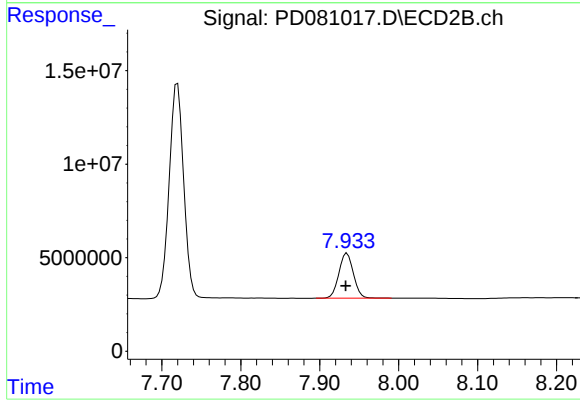

#28 Decachlorobiphenyl

R.T.: 7.935 min

Delta R.T.: 0.002 min

Response: 30669836

Conc: 11.51 ng/ml