

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020224\
 Data File : PD081021.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Feb 2024 09:34
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 01:25:30 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	0.000	2.788	0	208161	N.D.	0.087 #
Target Compounds						
2) A alpha-BHC	0.000	3.313f	0	44386	N.D.	0.012 #
8) B Heptachlo...	5.715	0.000	1278910	0	0.571	N.D. #
10) B gamma-Chl...	5.942f	0.000	76227	0	0.035	N.D. #
14) MA Endrin	0.000	5.677f	0	1297759	N.D.	0.438 #
15) B Endosulfa...	6.833	0.000	255788	0	0.132	N.D. #
18) B Endrin al...	6.971	6.151f	177031	228482	0.116	0.101
24) Chlordane-2	0.000	4.375	0	366238	N.D.	2.988 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020224\
Data File : PD081021.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Feb 2024 09:34
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 01:25:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

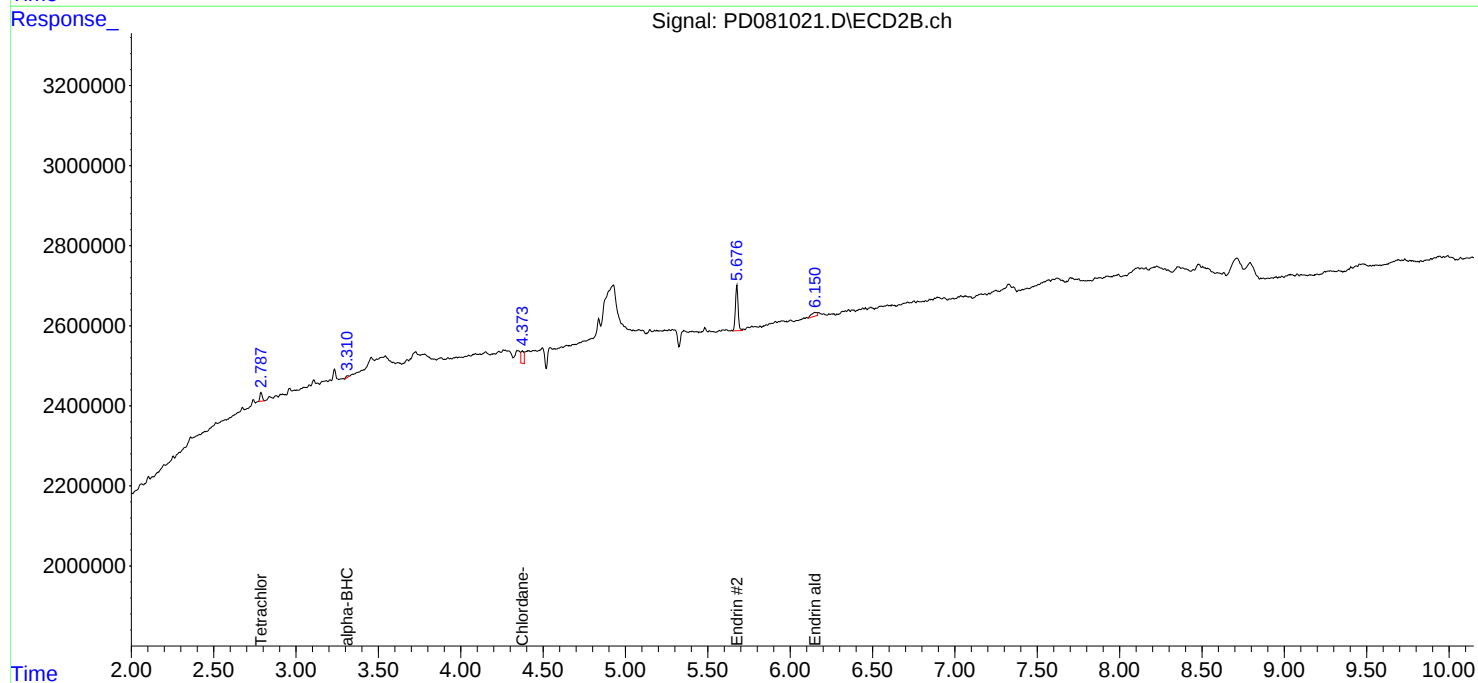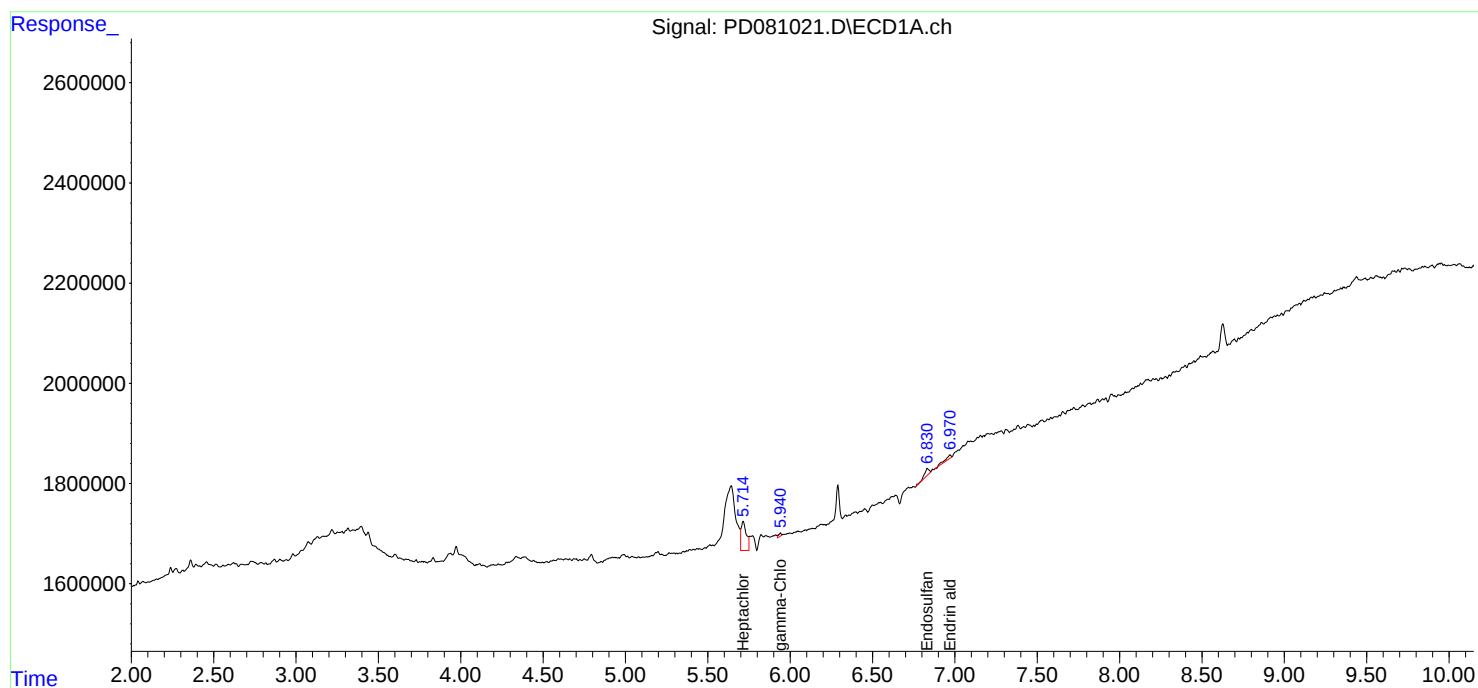


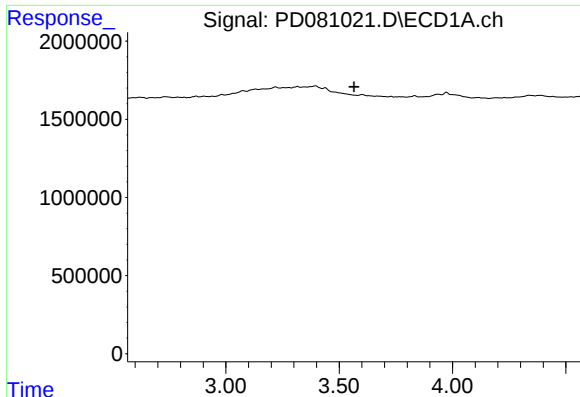

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.566 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

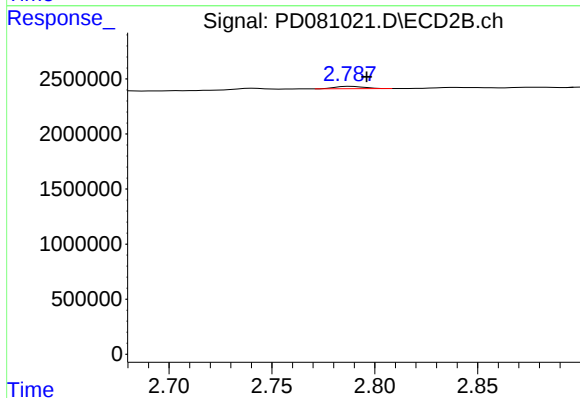


#1 Tetrachloro-m-xylene

R.T.: 2.788 min
Delta R.T.: -0.008 min
Response: 208161
Conc: 0.09 ng/ml

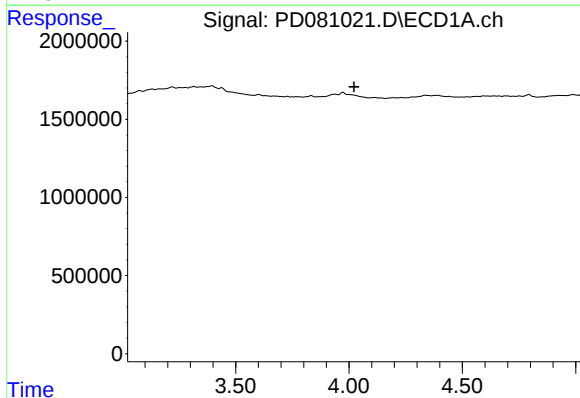


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T.: 4.022 min
Response: 0
Conc: N.D.

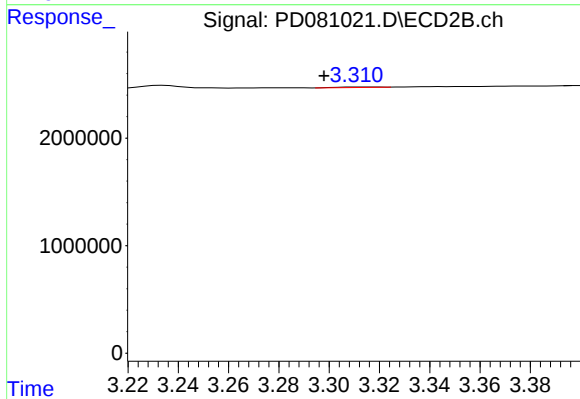

#2 alpha-BHC


R.T.: 3.313 min
Delta R.T.: 0.015 min
Response: 44386
Conc: 0.01 ng/ml

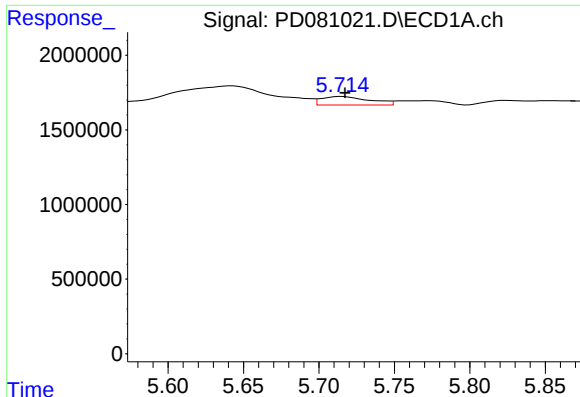

#8 Heptachlor epoxide


R.T.: 5.715 min
Delta R.T.: -0.002 min
Response: 1278910
Conc: 0.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

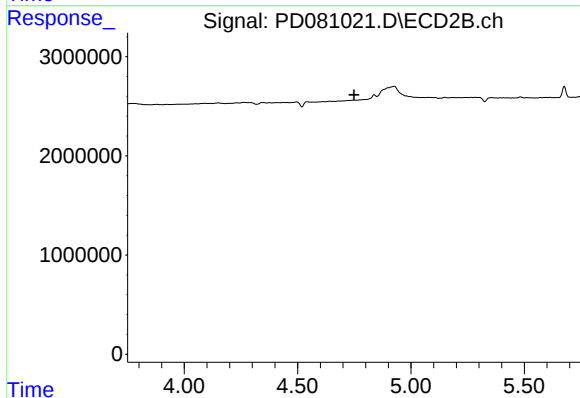


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.750 min
Response: 0
Conc: N.D.

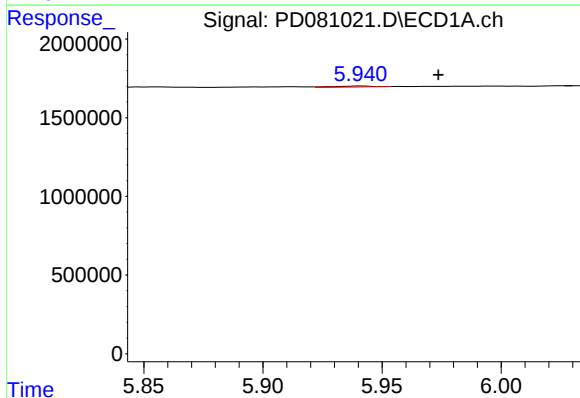


#10 gamma-Chlordane

R.T.: 5.942 min
Delta R.T.: -0.032 min
Response: 76227
Conc: 0.03 ng/ml

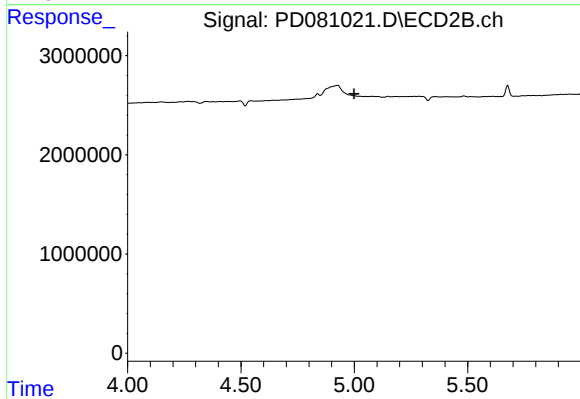

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.000 min
Response: 0
Conc: N.D.

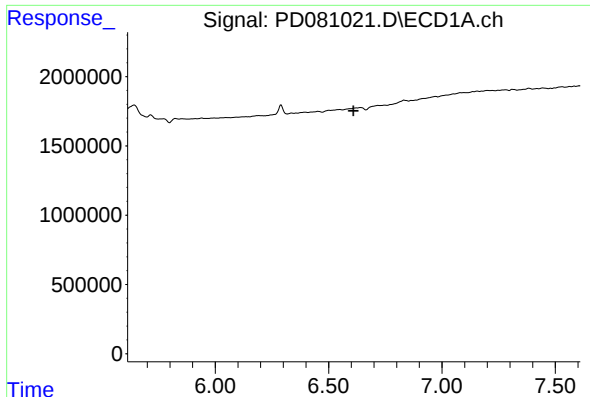

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.610 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

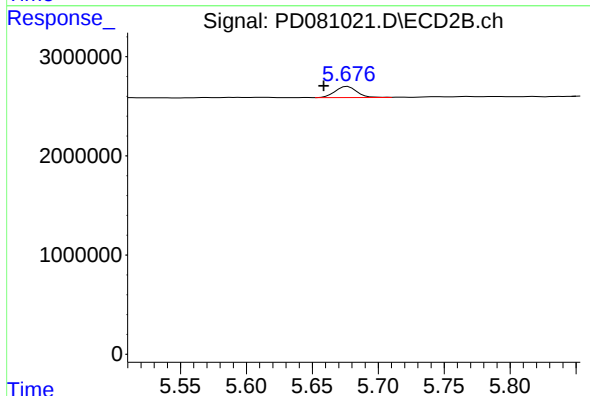


#14 Endrin

R.T.: 5.677 min
Delta R.T.: 0.018 min
Response: 1297759
Conc: 0.44 ng/ml

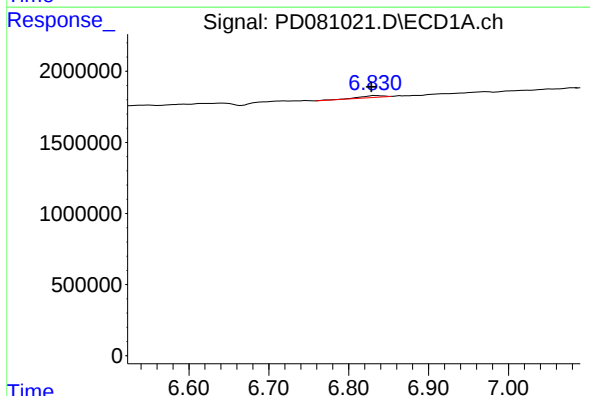


#15 Endosulfan II

R.T.: 6.833 min
Delta R.T.: 0.004 min
Response: 255788
Conc: 0.13 ng/ml

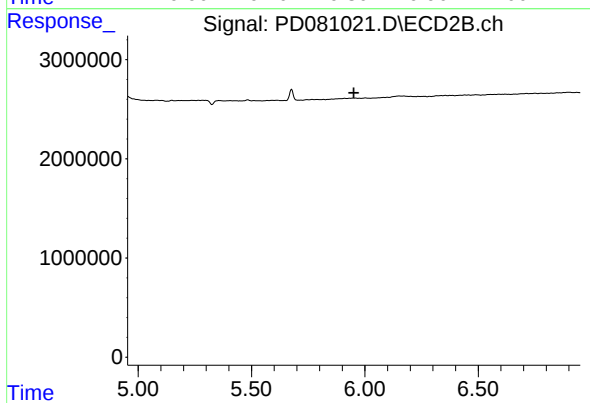

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.951 min
Response: 0
Conc: N.D.

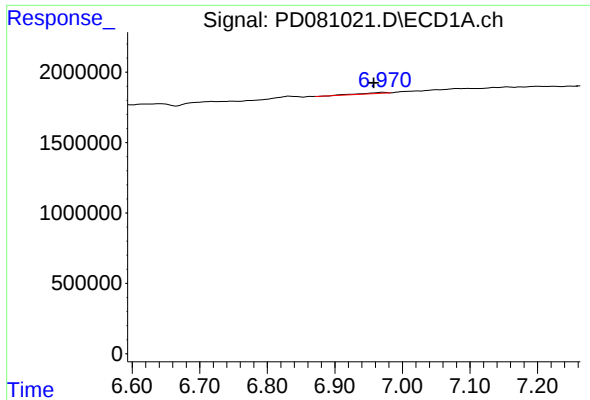

#18 Endrin aldehyde


R.T.: 6.971 min
Delta R.T.: 0.013 min
Response: 177031
Conc: 0.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

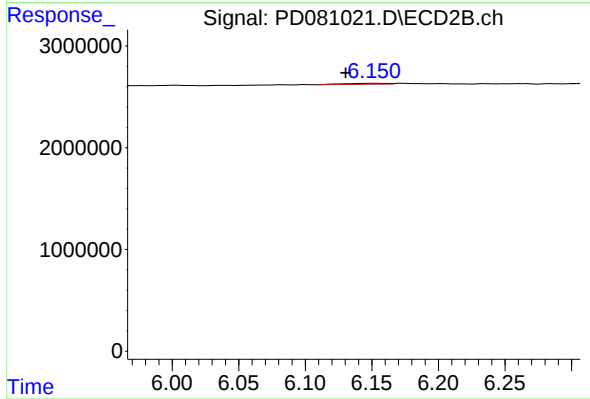


#18 Endrin aldehyde

R.T.: 6.151 min
Delta R.T.: 0.021 min
Response: 228482
Conc: 0.10 ng/ml

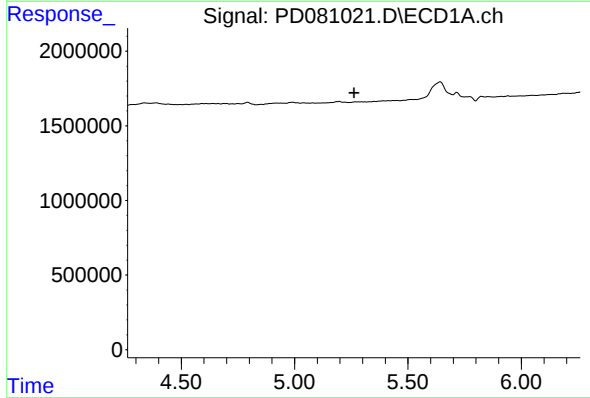


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.263 min
Response: 0
Conc: N.D.

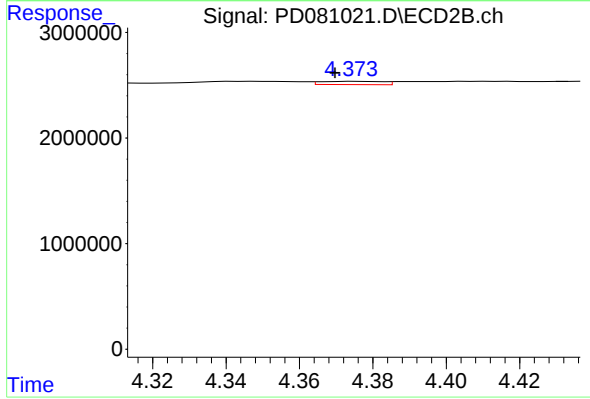

#24 Chlordane-2


R.T.: 4.375 min
Delta R.T.: 0.005 min
Response: 366238
Conc: 2.99 ng/ml

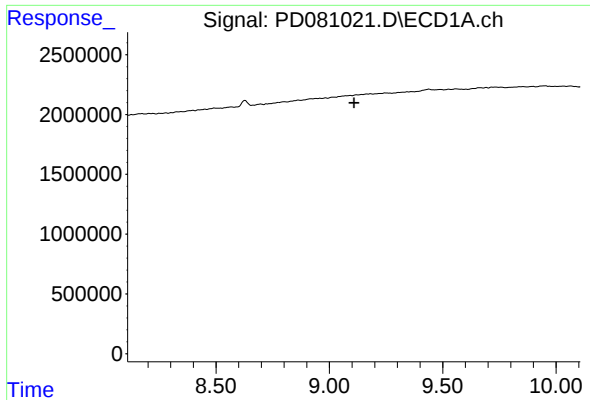

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.109 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

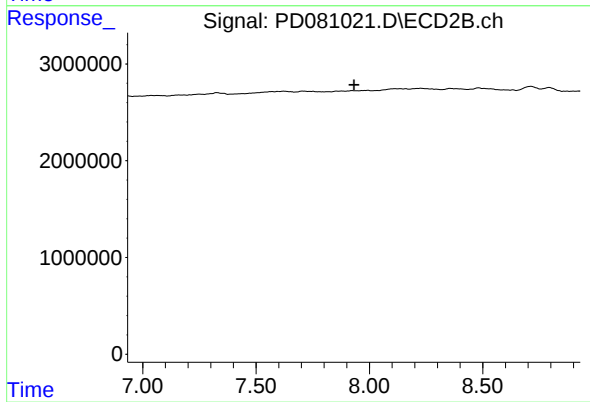

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.933 min
Response: 0
Conc: N.D.