

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020224\
 Data File : PD081037.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Feb 2024 17:55
 Operator : AR\AJ
 Sample : P1341-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COMP-2

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/05/2024
 Supervised By :Ankita Jodhani 02/05/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 01:39:14 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.796	19288248	33331362	13.587	13.934
28)	SA Decachlor...	9.113	7.934	26317015	36926795	13.077	13.863
Target Compounds							
12)	B 4,4'-DDE	6.224	5.251	8038052	4285417	3.950	1.399m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020224\
Data File : PD081037.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Feb 2024 17:55
Operator : AR\AJ
Sample : P1341-02
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/05/2024
Supervised By : Ankita Jodhani 02/05/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 01:39:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

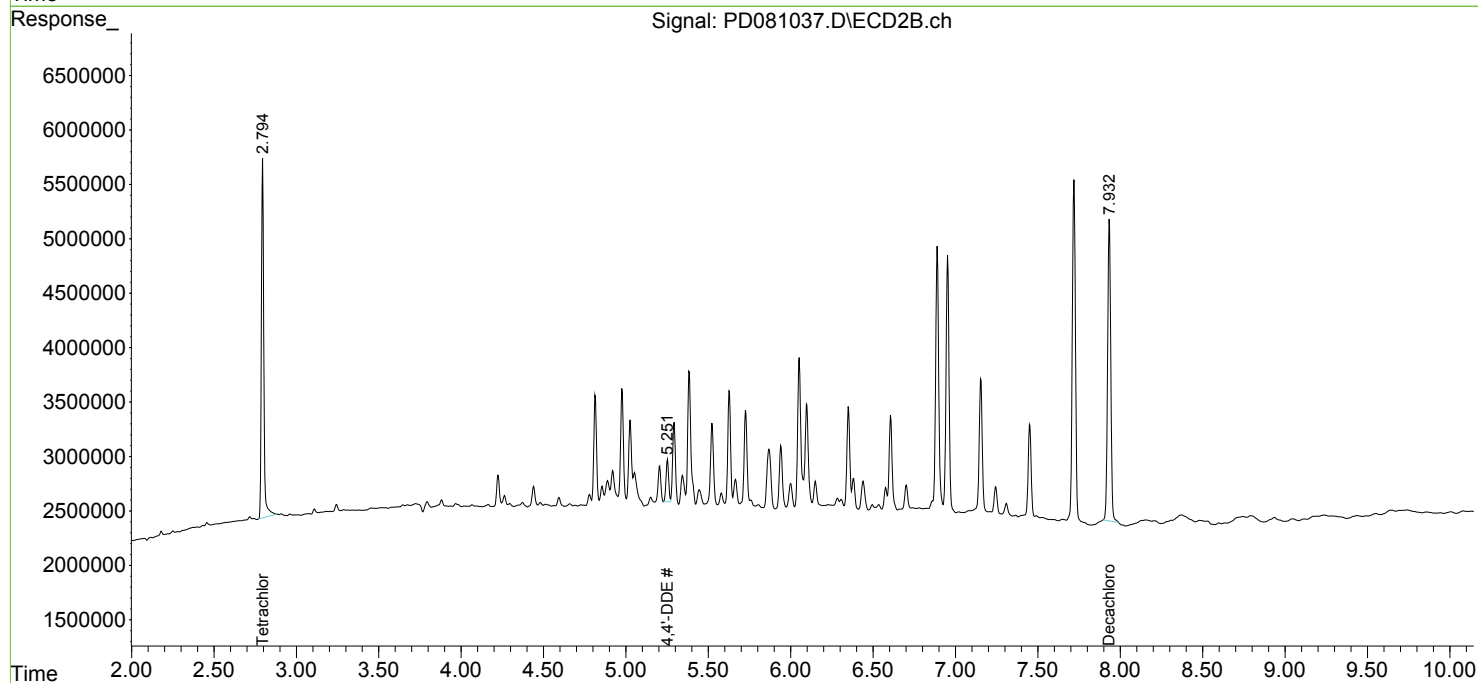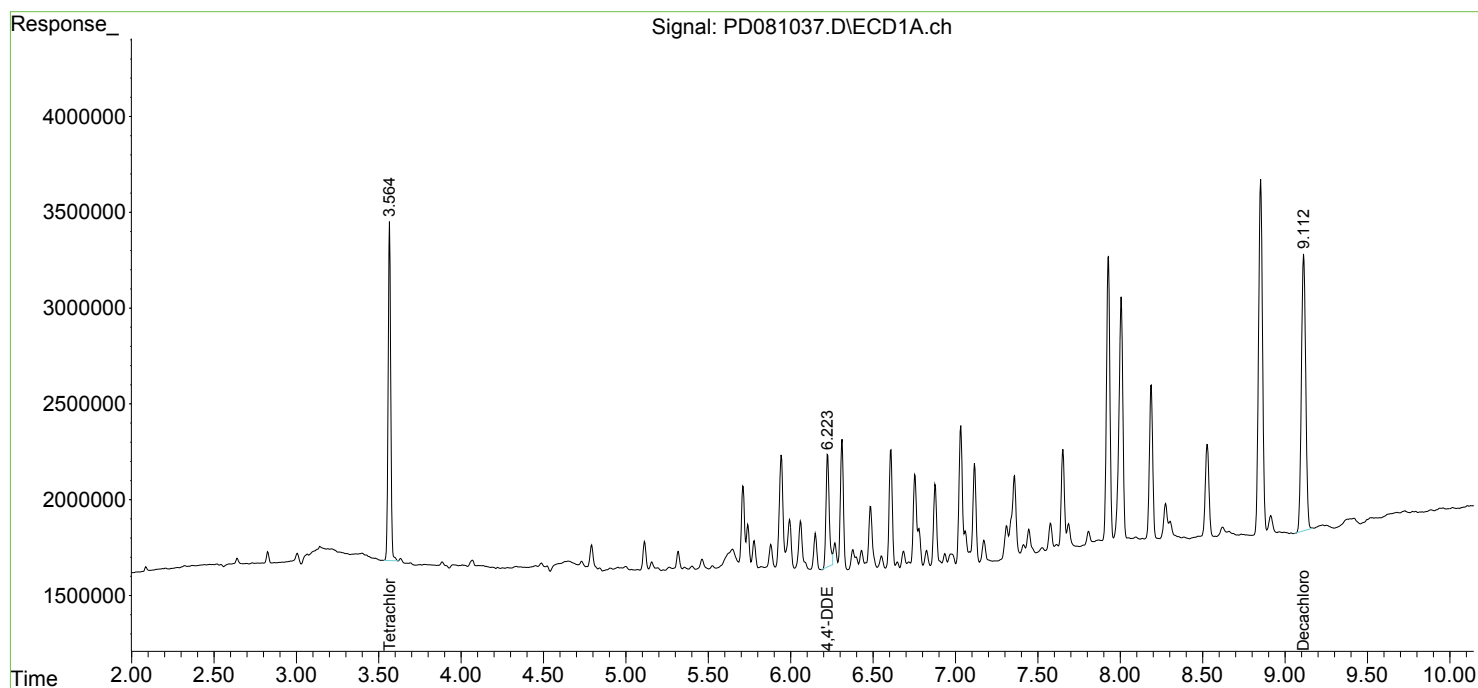

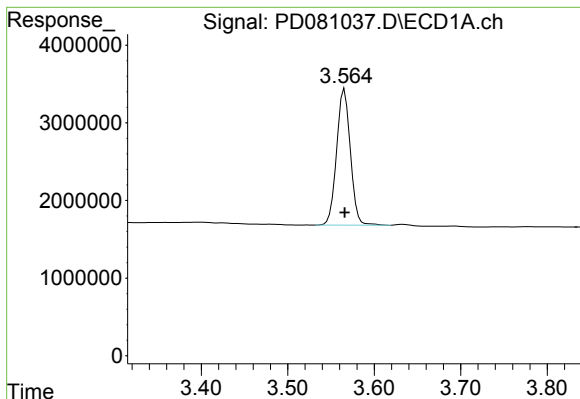


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 19288248
Conc: 13.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/05/2024
Supervised By :Ankita Jodhani 02/05/2024

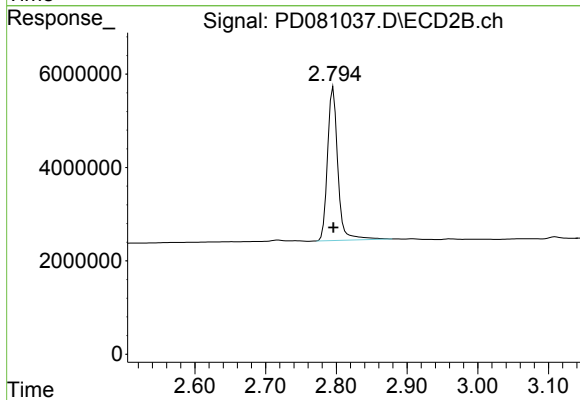


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 33331362
Conc: 13.93 ng/ml

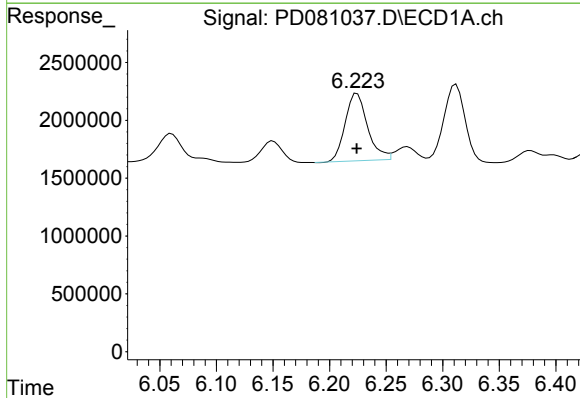


#12 4,4'-DDE

R.T.: 6.224 min
Delta R.T.: 0.000 min
Response: 8038052
Conc: 3.95 ng/ml

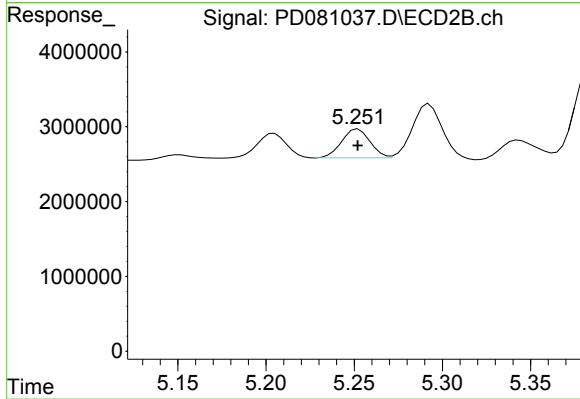

#12 4,4'-DDE

R.T.: 5.251 min
Delta R.T.: -0.001 min
Response: 4285417
Conc: 1.40 ng/ml m

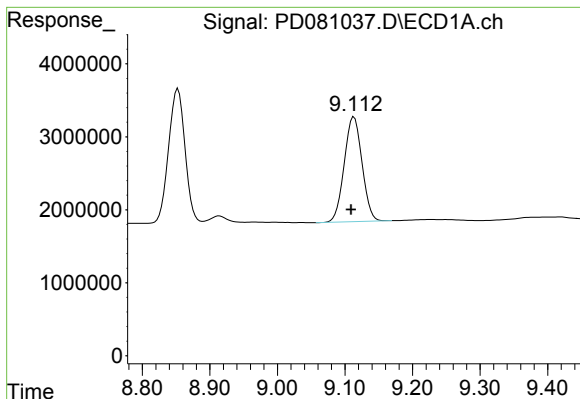


#28 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: 0.004 min
Response: 26317015
Conc: 13.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/05/2024
Supervised By :Ankita Jodhani 02/05/2024

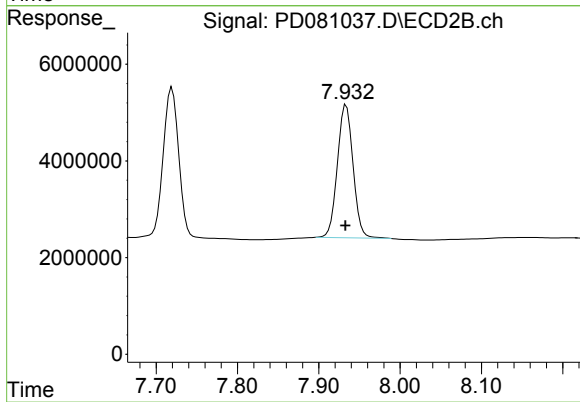

#28 Decachlorobiphenyl

R.T.: 7.934 min
Delta R.T.: 0.000 min
Response: 36926795
Conc: 13.86 ng/ml