

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020322\
 Data File : PD067890.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2022 09:52
 Operator : AR\AJ
 Sample : TOXAPH201
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 00:58:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020322CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 04 00:54:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.429	3.959	20977494	85797304	10.430	11.240
27)	SA Decachlor...	8.148	9.008	19913121	105.2E6	22.441	22.386
Target Compounds							
22)	Toxaphene-1	5.663	6.341	15739893	35926083	1010.736	1108.360
23)	Toxaphene-2	6.144	6.634	16348002	37620781	1036.456	1085.321
24)	Toxaphene-3	6.263	7.117	36686513	101.4E6	996.367	1071.547
25)	Toxaphene-4	6.508	7.202	36412067	101.2E6	988.884	1063.905
26)	Toxaphene-5	6.992	7.620	35988562	76859669	1003.896	1076.940

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020322\
Data File : PD067890.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2022 09:52
Operator : AR\AJ
Sample : TOXAPH201
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 00:58:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020322CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 04 00:54:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

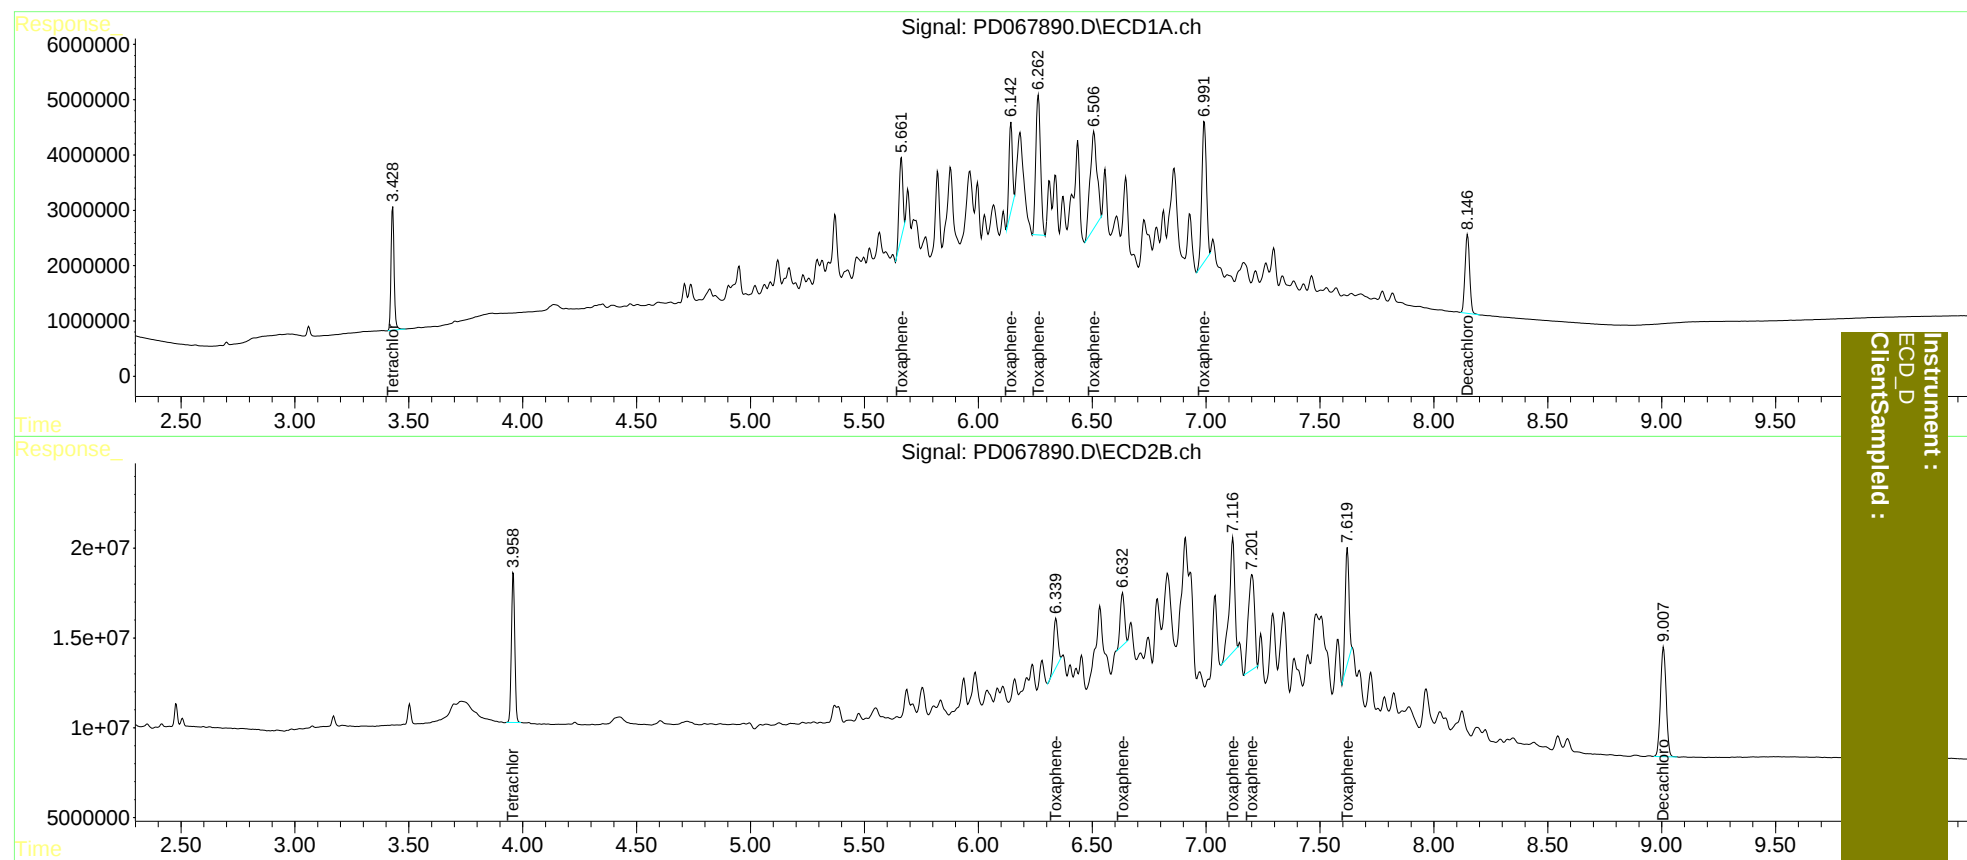

Instrument :
ECD_D
ClientSampled :