

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020322\
 Data File : PD067887.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2022 09:11
 Operator : AR\AJ
 Sample : RESC009
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC018

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/04/2022
 Supervised By : Ankita Jodhani 02/08/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 02:18:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020322CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 04 02:10:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.430	3.959	44956735	173.5E6	22.228	22.108
27)	SA Decachlor...	8.148	9.008	40133027	211.7E6	43.921	43.236
Target Compounds							
2)	A alpha-BHC	3.866	4.353	32643797	117.2E6	10.944	11.699
3)	MA gamma-BHC...	4.147	4.637	31587041	112.1E6	10.973	11.789
4)	MA Heptachlor	4.440	5.136	32115748	98536893	10.942	11.565
5)	MB Aldrin	4.684	5.440	31011246	91090194	10.532	11.125
6)	B beta-BHC	4.396	4.816	14029280	52080201	10.537	11.567
7)	B delta-BHC	4.598	5.030	28764807	96670798	10.222	11.821
8)	B Heptachlo...	5.125	5.827	27739262	105.3E6	10.407	15.523m#
9)	A Endosulfan I	5.460	6.185	27134985	81812201	11.056	11.744
10)	B trans-Chl...	5.348	6.062	28260694	80848608	10.387	11.094
11)	B cis-Chlor...	5.406	6.133	27631628	81430491	10.261	11.133
12)	B 4,4'-DDE	5.570	6.294	54090266	145.5E6	22.119	21.457
13)	MA Dieldrin	5.702	6.443	57034096	164.1E6	21.456	22.856
14)	MA Endrin	5.959	6.658	50101930	109.6E6	23.273	18.413m
15)	B Endosulfa...	6.232	6.876	45017447	133.4E6	21.154	21.609
16)	A 4,4'-DDD	6.084	6.789	43159279	129.7E6	21.908	22.403
17)	MA 4,4'-DDT	6.322	7.085	40606066	128.7E6	21.203	22.366
18)	B Endrin al...	6.400	7.001	33965739	104.8E6	21.775	21.842
19)	B Endosulfa...	6.612	7.224	37964628	128.3E6	20.994	21.839
20)	A Methoxychlor	6.869	7.546	97038050	330.9E6	110.484	118.234m
21)	B Endrin ke...	7.101	7.695	42748339	148.4E6	22.608m	22.189

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020322\
Data File : PD067887.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2022 09:11
Operator : AR\AJ
Sample : RESC009
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 02:18:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020322CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 04 02:10:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

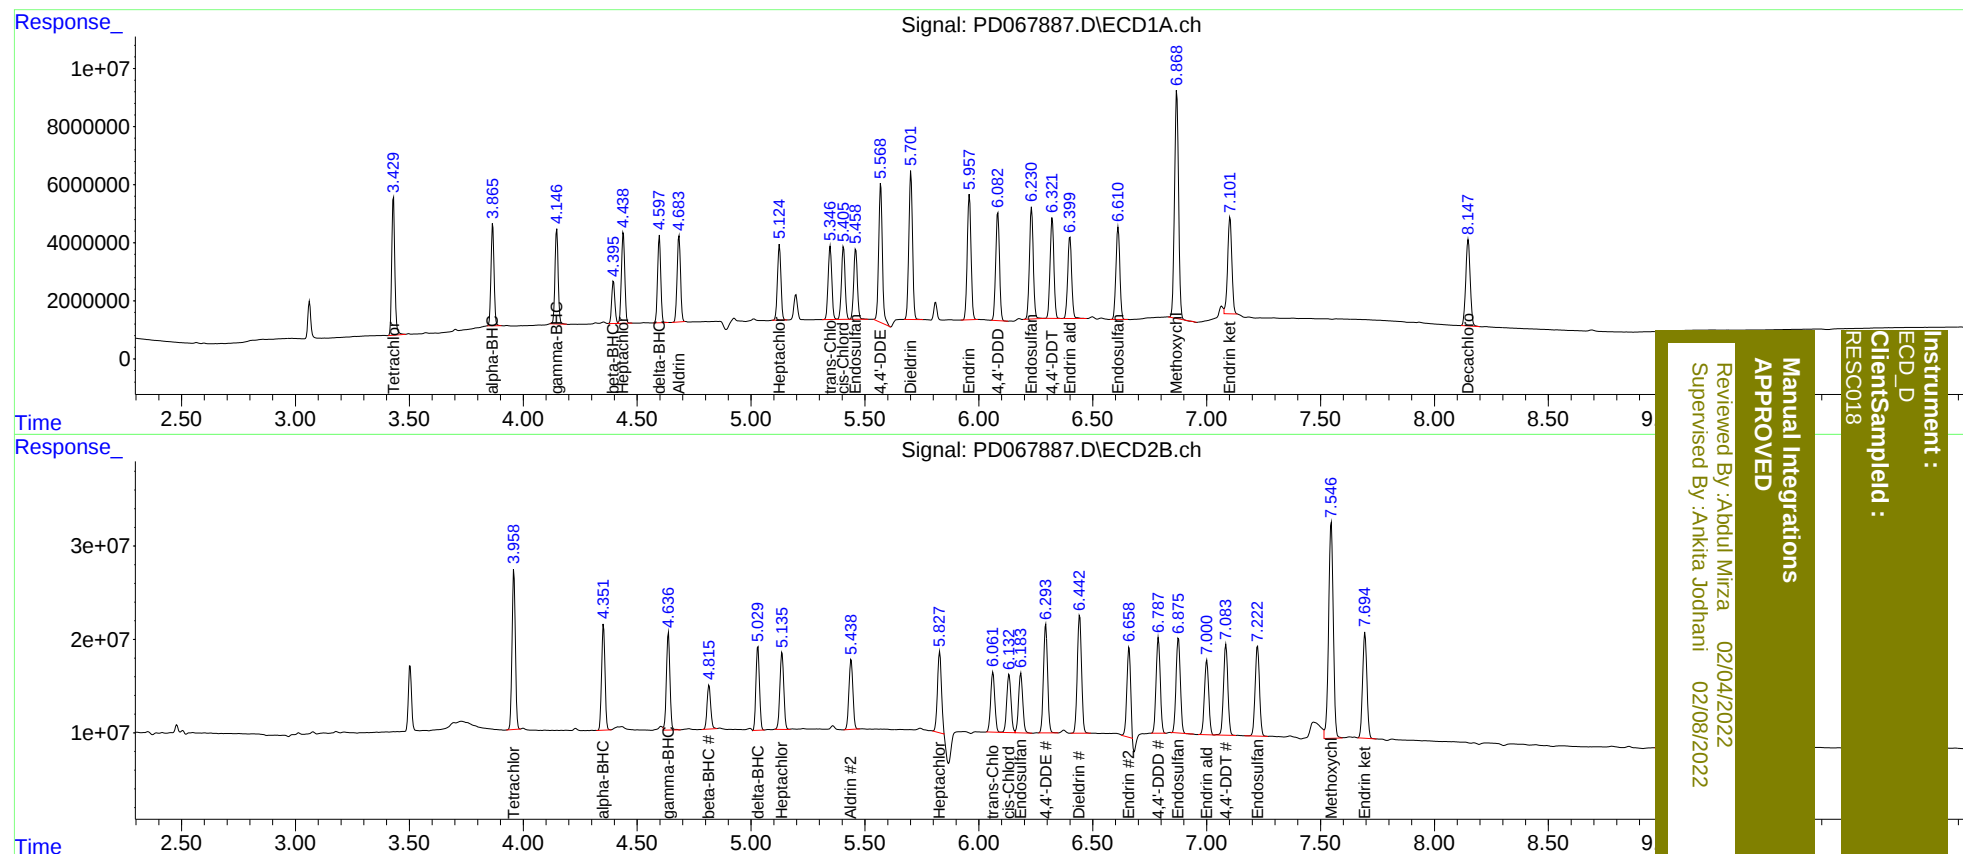

Reviewed By: Abdul Mirza 02/04/2022
Supervised By: Ankita Jodhani 02/08/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
RESC018