

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020322\
 Data File : PD067921.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2022 17:53
 Operator : AR\AJ
 Sample : N1307-09
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0Q50

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/04/2022
 Supervised By :Ankita Jodhani 02/08/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 05:59:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020322CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 04 02:10:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.453	3.938	7525.1E6	30731.3E6	3720.652	3915.295m
2) SA Decachlor...	8.150	9.010	24829826	145.3E6	27.173	29.668
Target Compounds						
13) MA Dieldrin	5.704	6.443	10868635	20130395	4.089	2.805 #
21) B Endrin ke...	7.106	7.673	1418949	13057031	0.750m	1.953 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020322\
Data File : PD067921.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2022 17:53
Operator : AR\AJ
Sample : N1307-09
Misc :
ALS Vial : 34 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 05:59:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020322CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 04 02:10:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

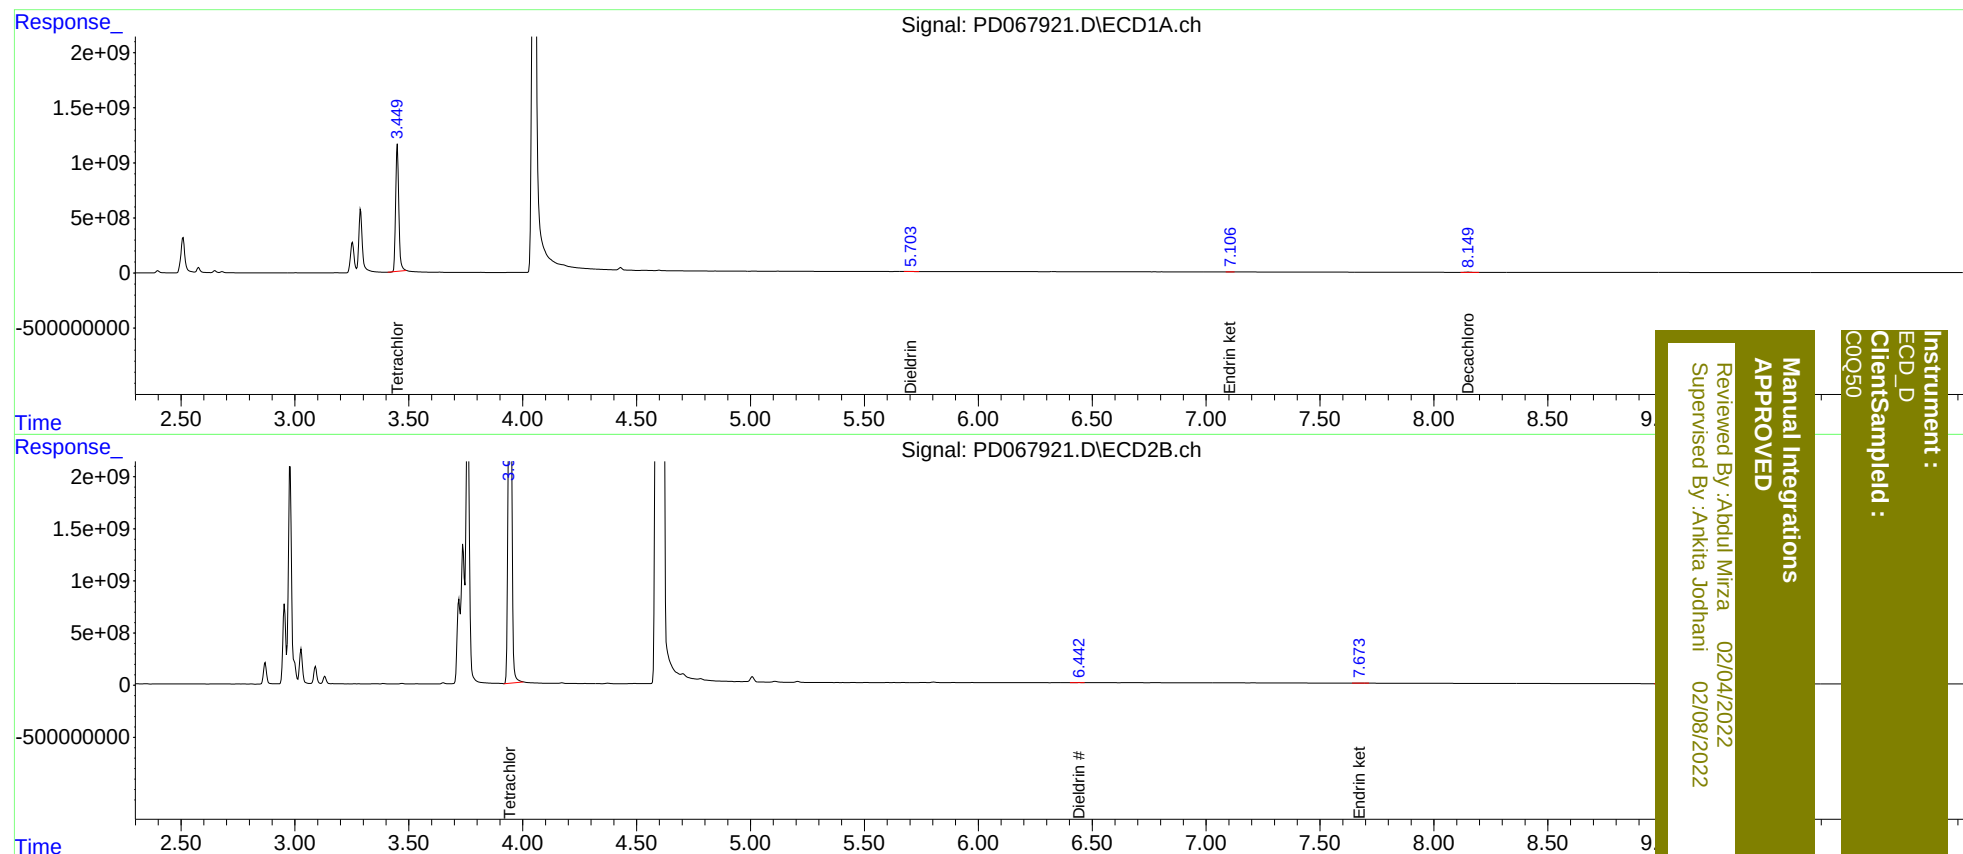

Reviewed By: Abdul Mirza 02/04/2022
Supervised By: Ankita Jodhani 02/08/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
C0050