

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020322\
 Data File : PD067900.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2022 12:11
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA4025

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/04/2022
 Supervised By : Ankita Jodhani 02/08/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 12:28:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020322CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 03 12:07:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.430	3.959	78023142	286.1E6	38.162	36.135
27)	SA Decachlor...	8.147	9.009	67458613	366.9E6	73.662	73.992
Target Compounds							
2)	A alpha-BHC	3.866	4.352	120.7E6	381.0E6	40.054	37.567
3)	MA gamma-BHC...	4.147	4.636	113.5E6	357.5E6	39.424	37.375m
4)	MA Heptachlor	4.440	5.136	116.6E6	320.4E6	39.503	37.141
9)	A Endosulfan I	5.459	6.185	95995340	262.2E6	38.932	37.182
13)	MA Dieldrin	5.701	6.442	213.9E6	549.3E6	79.511	75.729
14)	MA Endrin	5.958	6.661	171.4E6	451.7E6	78.357	74.622
16)	A 4,4'-DDD	6.083	6.788	157.4E6	445.3E6	78.826	75.700
17)	MA 4,4'-DDT	6.321	7.085	156.4E6	447.0E6	80.304	76.365
20)	A Methoxychlor	6.868	7.547	337.3E6	1036.1E6	379.690	364.894

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020322\
Data File : PD067900.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2022 12:11
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 12:28:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020322CLP.M
Quant Title : GC Extractables
QLast Update : Thu Feb 03 12:07:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

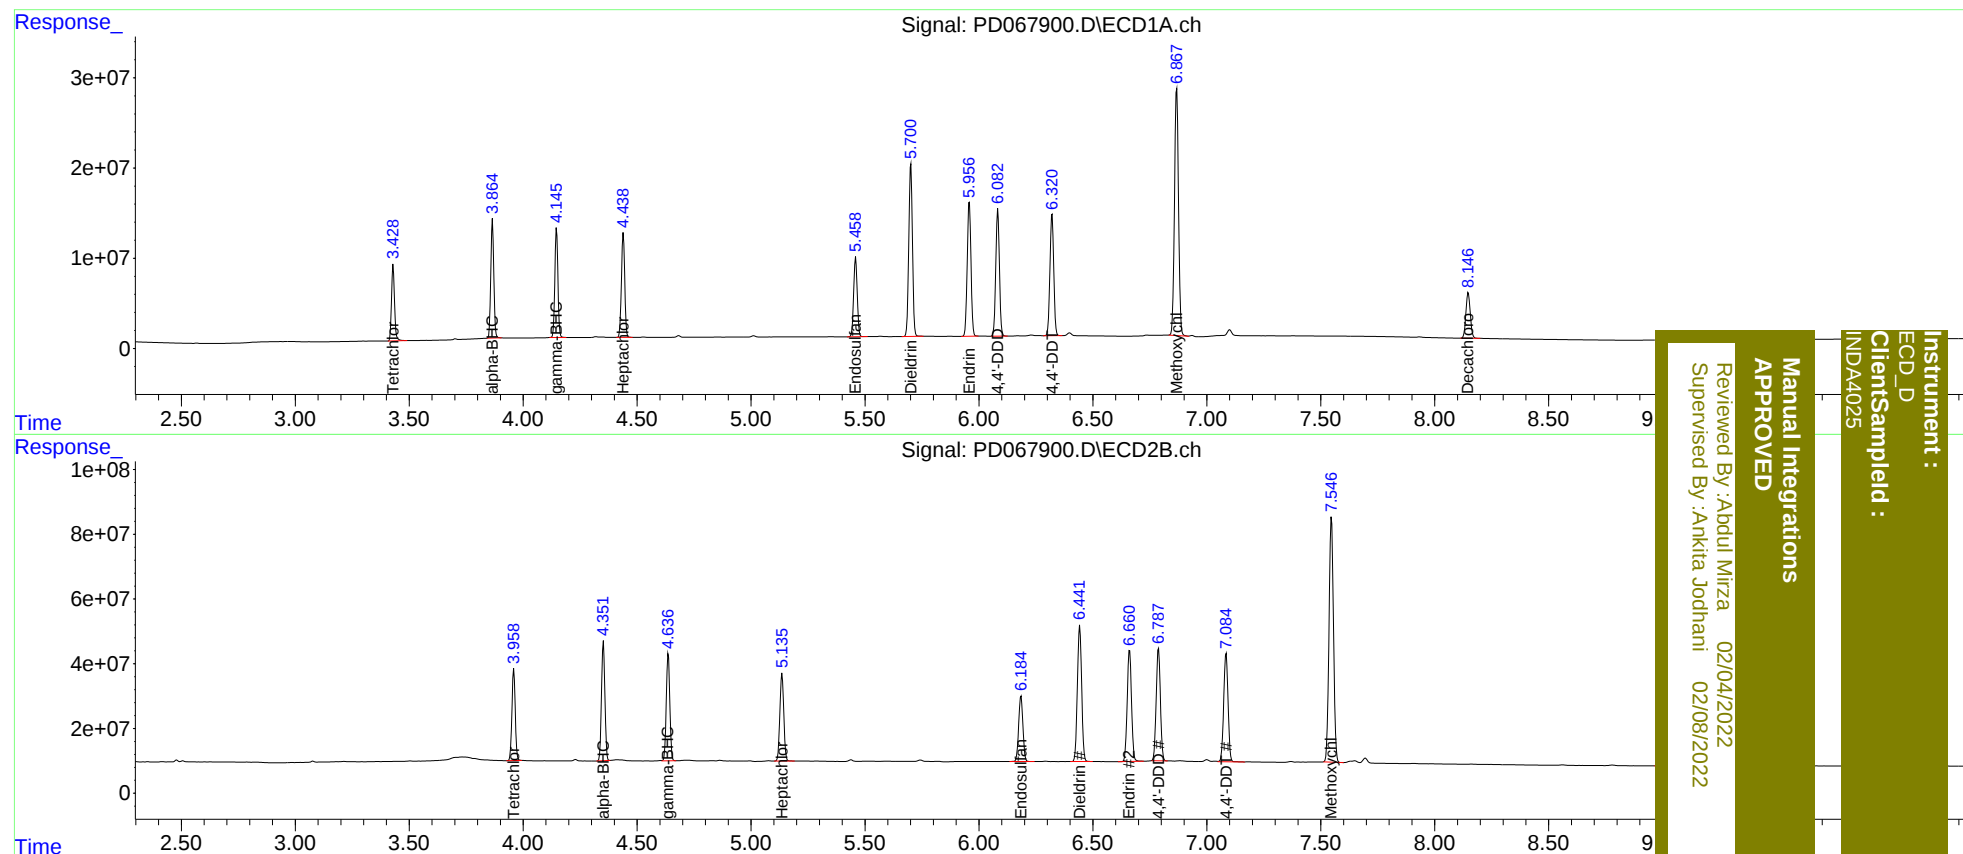

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 02/04/2022
Supervised By: Ankita Jodhani 02/08/2022

Instrument :
ECD_D
ClientSampled :
INDA4025