

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020322\
 Data File : PD067910.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2022 14:47
 Operator : AR\AJ
 Sample : N1307-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0Q00

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/09/2022
 Supervised By : Ankita Jodhani 02/09/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 08:16:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020322CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 04 02:10:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.433	3.944	16985432	2408.4E6	8.398m	306.841m#
2) SA Decachlor...	8.152	9.011	27621288	159.9E6	30.228	32.657
Target Compounds						
8) B Heptachlo...	5.125	5.825	3681483	10307224	1.381m	1.519m
9) A Endosulfan I	5.442	6.170	2993175	7262173	1.220m	1.042
13) MA Dieldrin	5.705	6.445	37669992	114.1E6	14.171m	15.899
21) B Endrin ke...	7.105	7.692	2752639	28745717	1.456m	4.299m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020322\
Data File : PD067910.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2022 14:47
Operator : AR\AJ
Sample : N1307-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 08:16:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020322CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 04 02:10:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

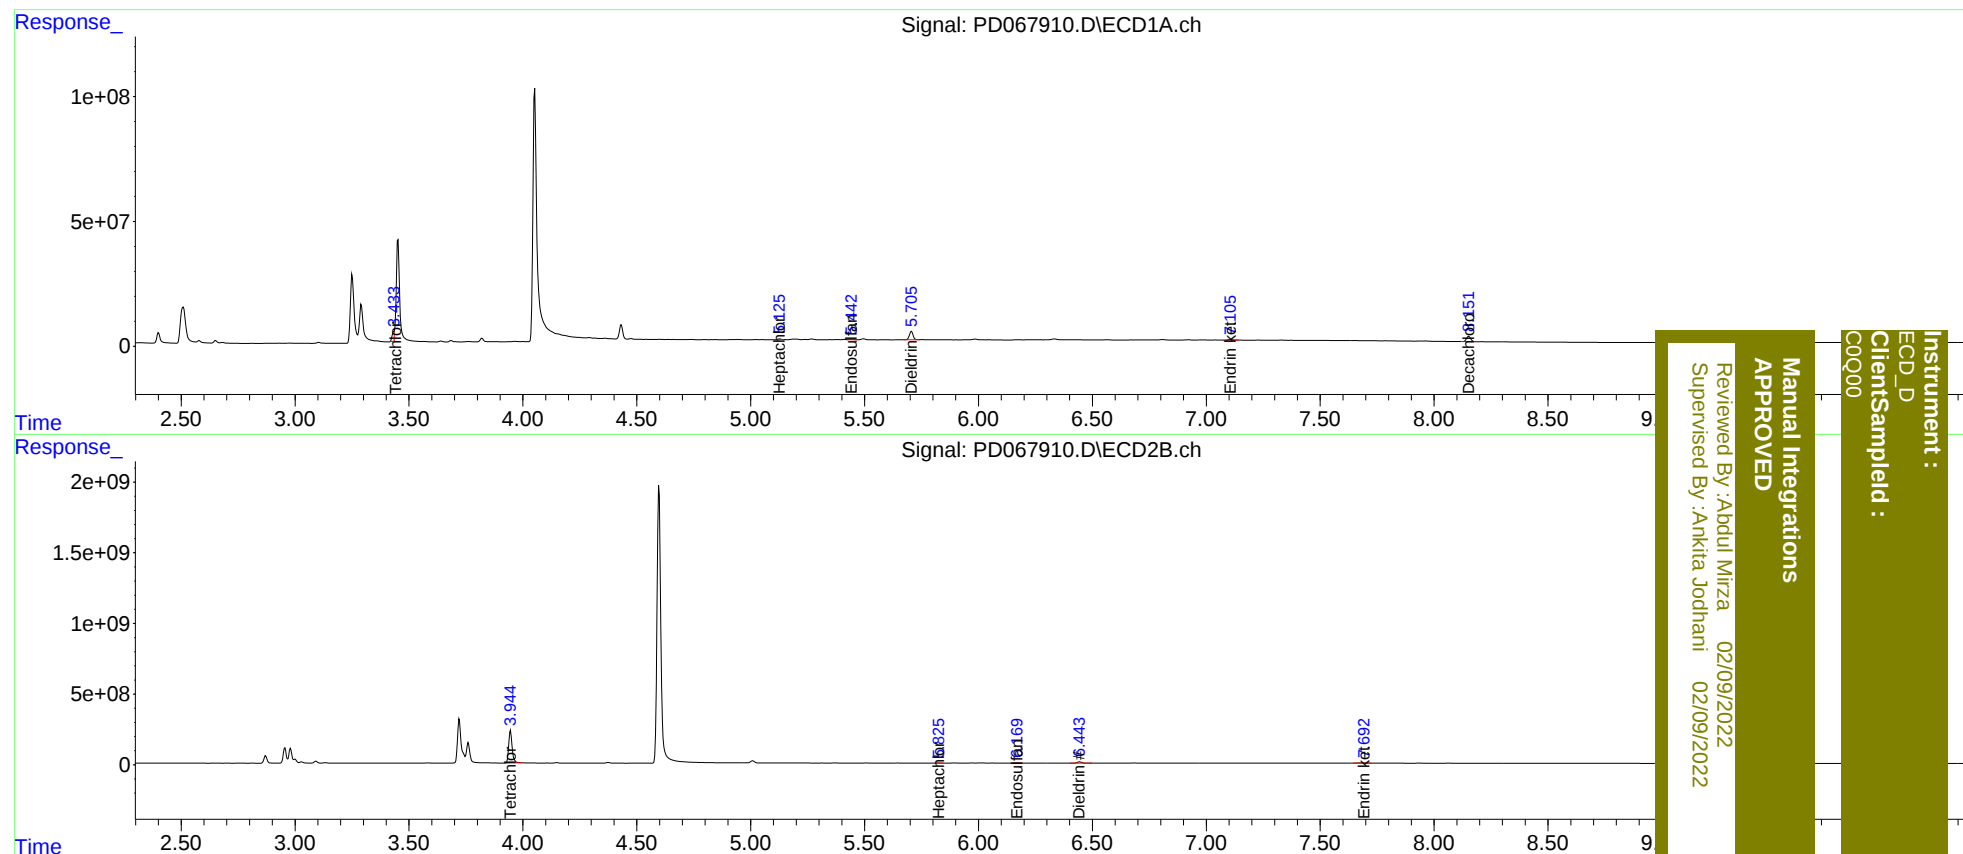

Instrument :
ECD_D
ClientSampled :
C0000

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/09/2022
Supervised By :Ankita Jodhani 02/09/2022