

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020322\
 Data File : PD067916.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2022 16:10
 Operator : AR\AJ
 Sample : N1307-07
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0Q47

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/09/2022
 Supervised By :Ankita Jodhani 02/09/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 08:40:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020322CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 04 02:10:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.429	3.945	21640441	942.2E6	10.700m	120.042m#
2) SA Decachlor...	8.149	9.009	27899504	158.8E6	30.533	32.431
Target Compounds						
13) MA Dieldrin	5.700	6.444	3756242	9402864	1.413m	1.310m
14) MA Endrin	5.981	6.684	17368537	43359028	8.068m	7.284

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020322\
Data File : PD067916.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2022 16:10
Operator : AR\AJ
Sample : N1307-07
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 08:40:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020322CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 04 02:10:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

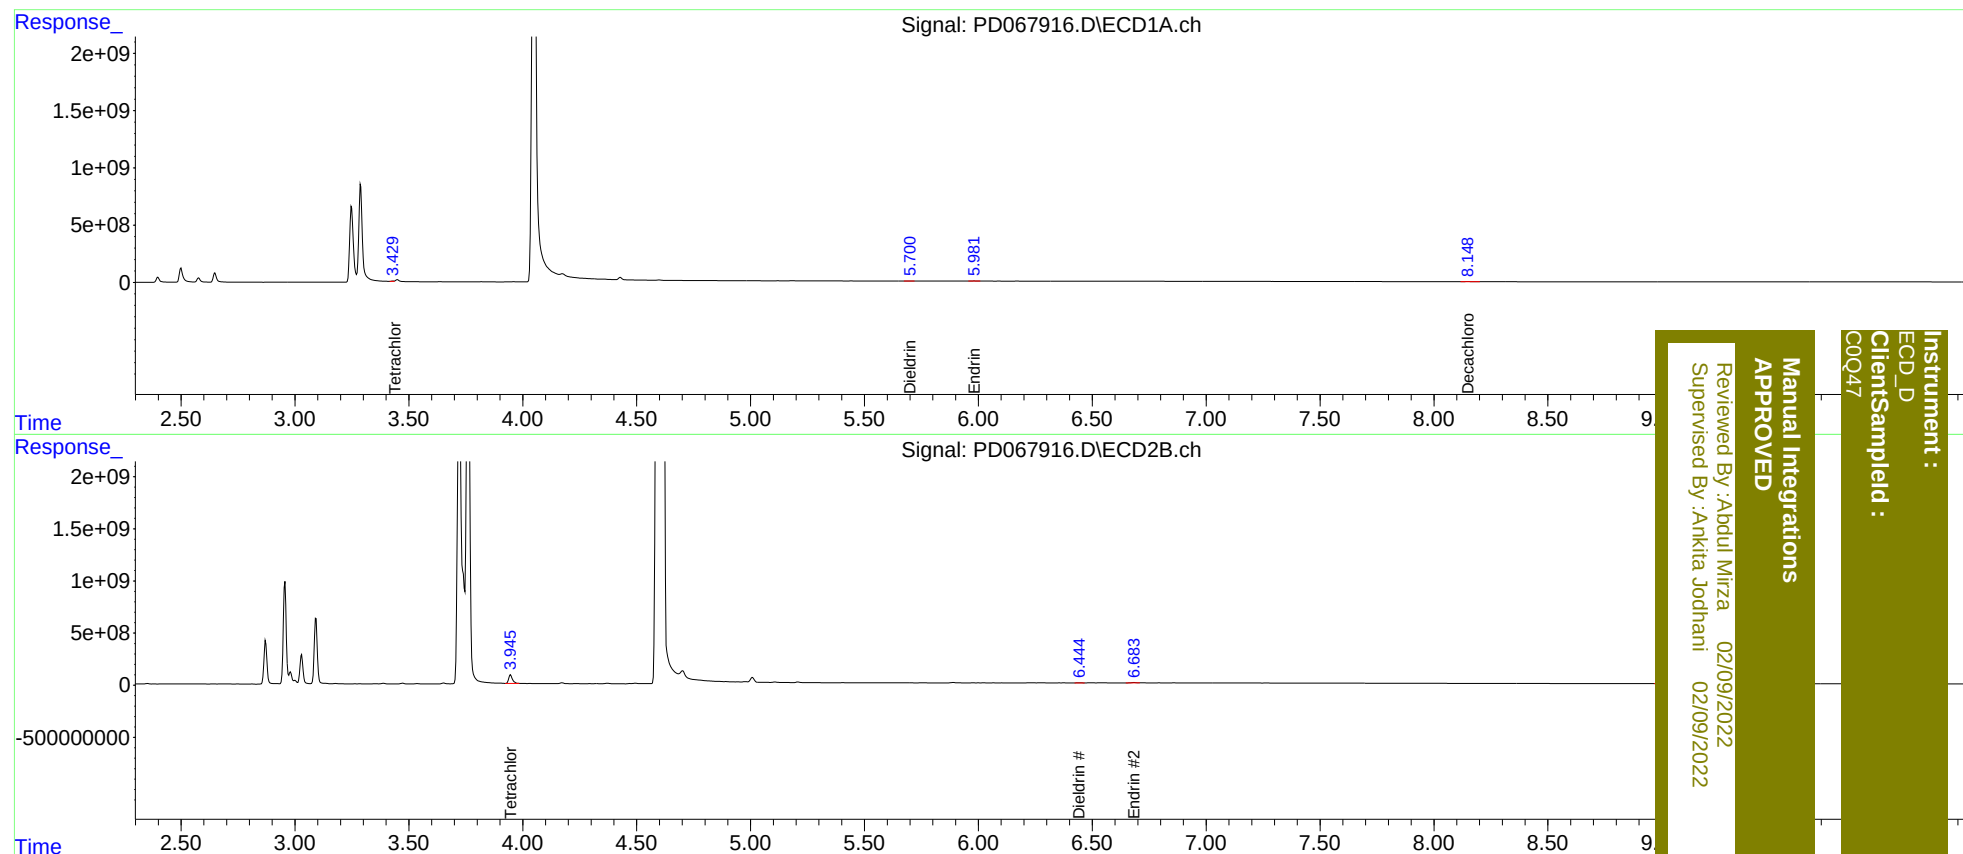

Instrument :
ECD_D
ClientSampled :
C0047

Manual Integrations
APPROVED


Reviewed By :Abdul Mirza 02/09/2022
Supervised By :Ankita Jodhani 02/09/2022

File : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020322\PD067916.D
Operator : AR\AJ
Acquired : 03 Feb 2022 16:10 using AcqMethod ECD_D.M
Instrument : ECD_D
Sample Name: N1307-07
Misc Info :
Vial Number: 30

Instrument :
ECD_D
ClientSampleId :
C0Q47

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/09/2022
Supervised By : Ankita Jodhani 02/09/2022

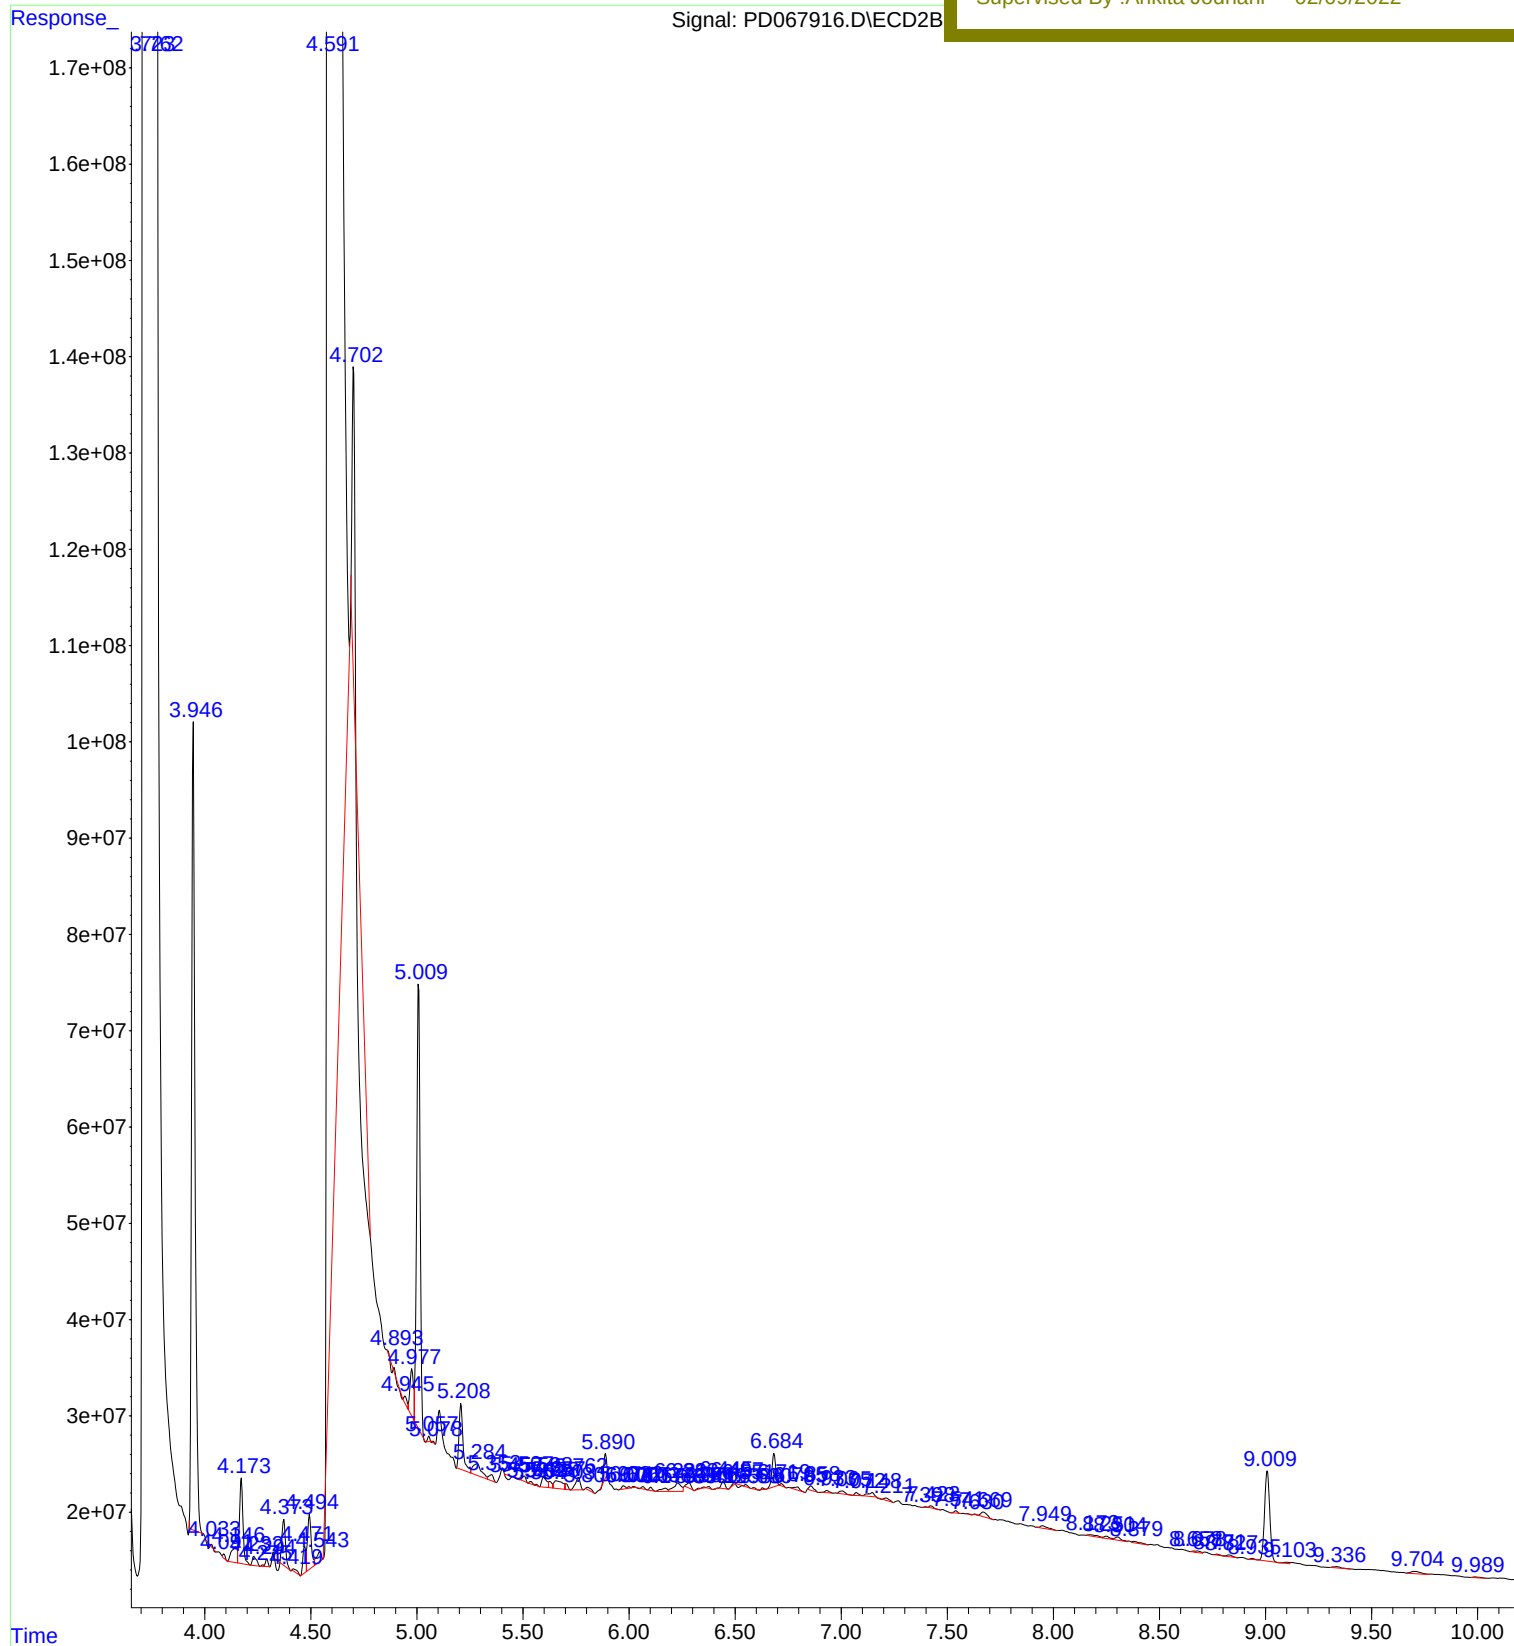

File :Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020322\PD067916.D
Operator : AR\AJ
Acquired : 03 Feb 2022 16:10 using AcqMethod ECD_D.M
Instrument : ECD_D
Sample Name: N1307-07
Misc Info :
Vial Number: 30

Instrument :
ECD_D
ClientSampleId :
C0Q47

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/09/2022
Supervised By :Ankita Jodhani 02/09/2022

