

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020325\
 Data File : PD087667.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2025 15:02
 Operator : AR\AJ
 Sample : 1202-11
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E29A2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 08:19:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 16 13:39:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.883	41641689	222.0E6	20.433	17.953
27)	SA Decachlor...	9.084	8.083	73039109	317.7E6	21.846	21.934
Target Compounds							
5)	MB Aldrin	0.000	4.345f	0	1896.4E6	N.D.	104.922
6)	B beta-BHC	0.000	3.984f	0	184.2E6	N.D.	21.594
7)	B delta-BHC	4.794	0.000	21176451	0	5.125	N.D. #
9)	A Endosulfan I	6.063	0.000	1657815	0	0.476	N.D. #
10)	B trans-Chl...	0.000	5.083f	0	2248.2E6	N.D.	125.052
11)	B cis-Chlor...	6.063	0.000	1657815	0	0.446	N.D. #
20)	A Methoxychlor	0.000	6.766	0	1134205	N.D.	0.184
24)	Toxaphene-3	0.000	6.766	0	1134205	N.D.	3.811
25)	Toxaphene-4	0.000	7.191	0	3388069	N.D.	15.993
26)	Toxaphene-5	7.905	7.296f	660688	5494306	13.596	35.429 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020325\
Data File : PD087667.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2025 15:02
Operator : AR\AJ
Sample : 1202-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 08:19:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 16 13:39:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

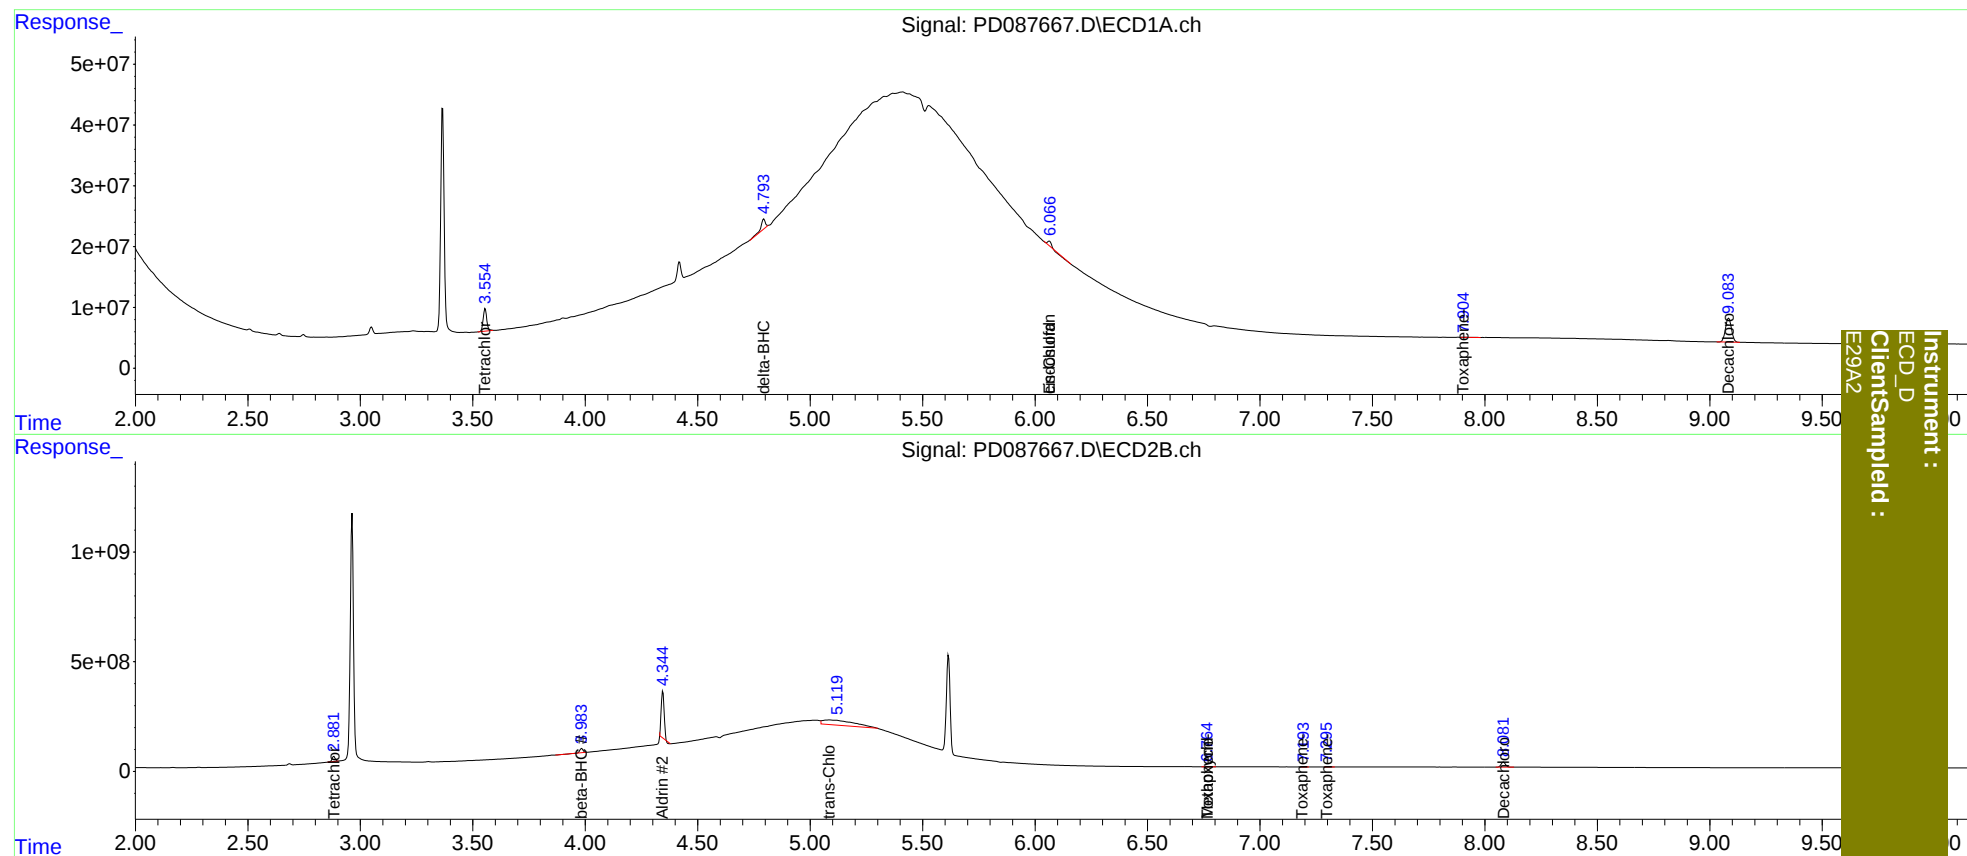


Instrument :
ECD_D
ClientSampled :
E29A2

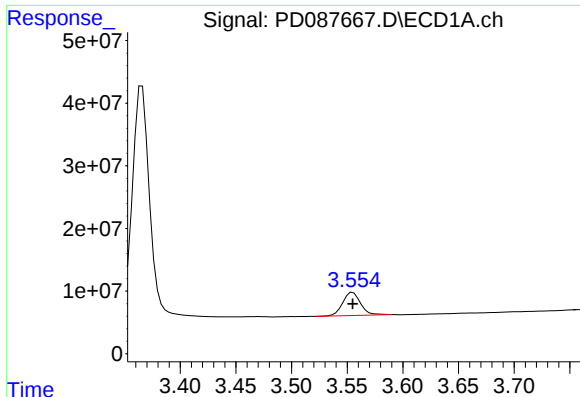

#1 Tetrachloro-m-xylene


R.T.: 3.555 min
Delta R.T.: 0.000 min
Response: 41641689
Conc: 20.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
E29A2

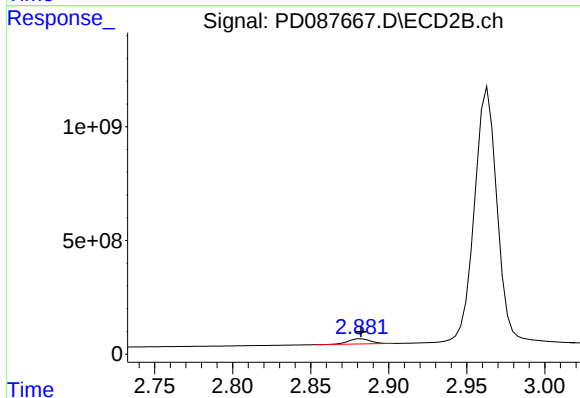


#1 Tetrachloro-m-xylene

R.T.: 2.883 min
Delta R.T.: 0.000 min
Response: 222040366
Conc: 17.95 ng/ml

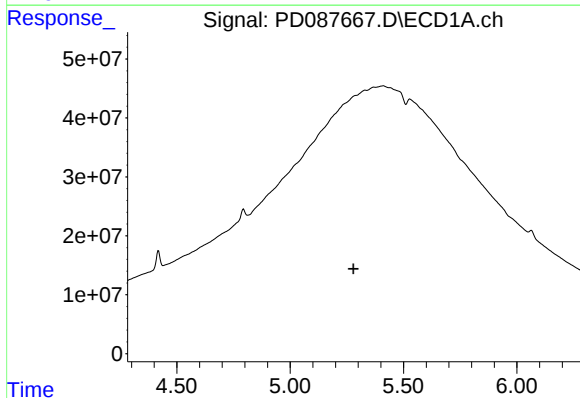


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.279 min
Response: 0
Conc: N.D.

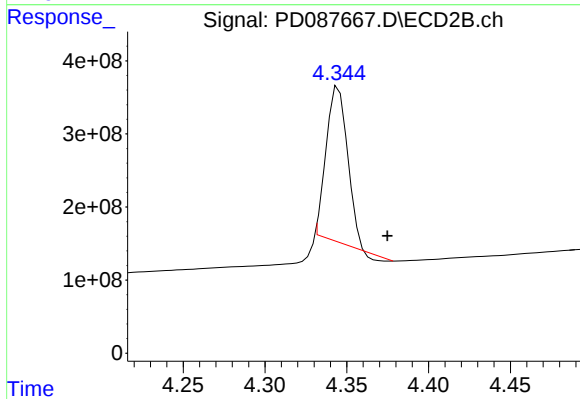

#5 Aldrin


R.T.: 4.345 min
Delta R.T.: -0.030 min
Response: 1896366499
Conc: 104.92 ng/ml

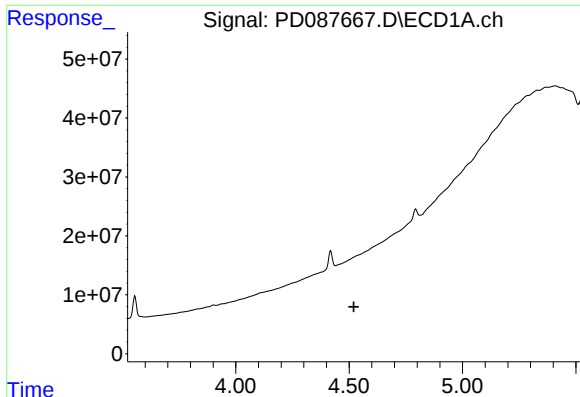

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.520 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
E29A2

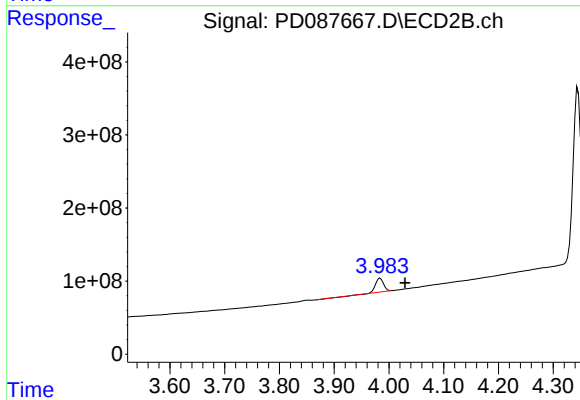


#6 beta-BHC

R.T.: 3.984 min
Delta R.T.: -0.045 min
Response: 184210348
Conc: 21.59 ng/ml

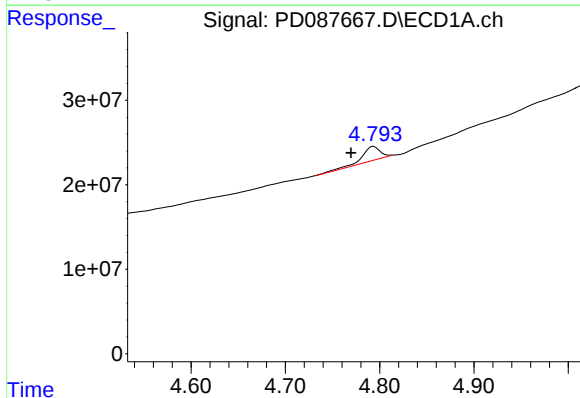


#7 delta-BHC

R.T.: 4.794 min
Delta R.T.: 0.024 min
Response: 21176451
Conc: 5.12 ng/ml

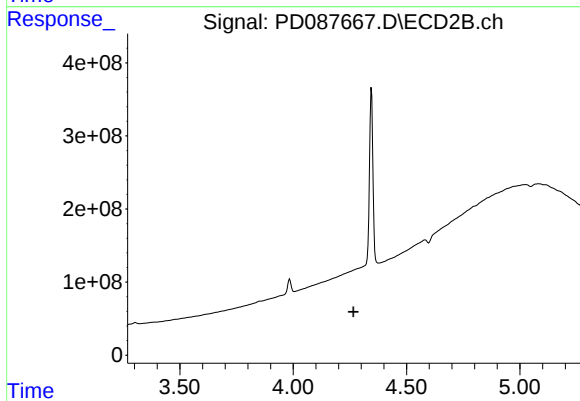

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.266 min
Response: 0
Conc: N.D.

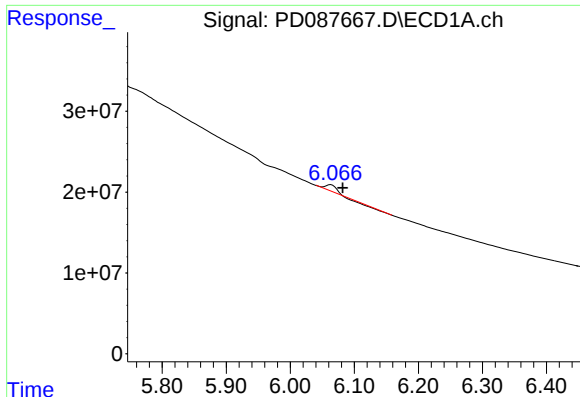

#9 Endosulfan I


R.T.: 6.063 min
Delta R.T.: -0.019 min
Response: 1657815
Conc: 0.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
E29A2

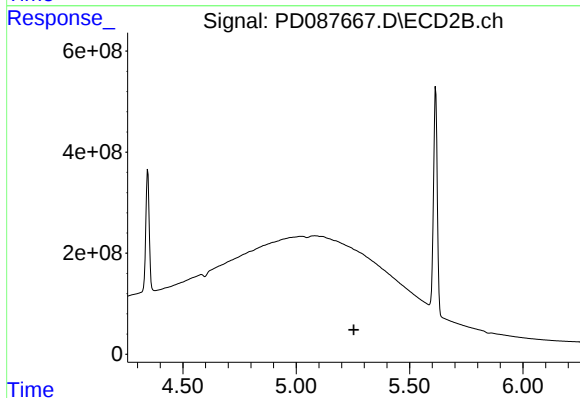


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.255 min
Response: 0
Conc: N.D.

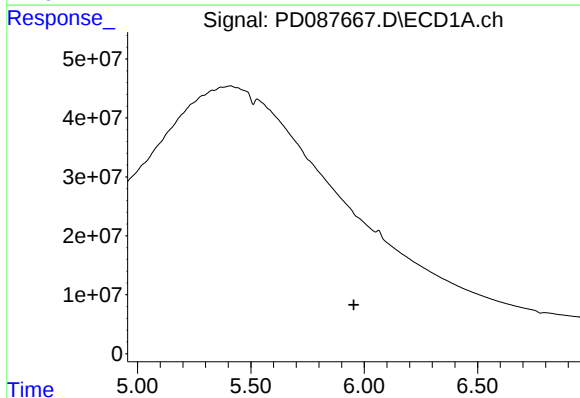


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.954 min
Response: 0
Conc: N.D.

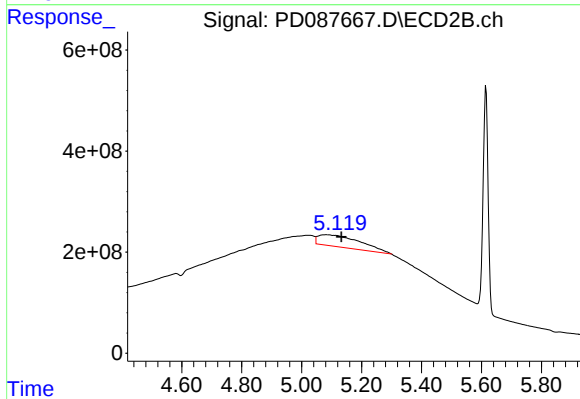

#10 trans-Chlordane


R.T.: 5.083 min
Delta R.T.: -0.050 min
Response: 2248165586
Conc: 125.05 ng/ml

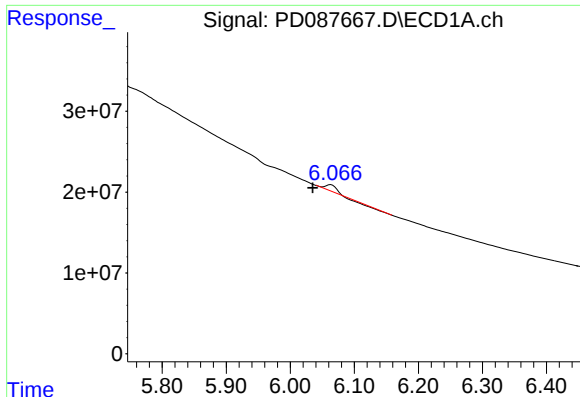

#11 cis-Chlordane


R.T.: 6.063 min
Delta R.T.: 0.028 min
Response: 1657815
Conc: 0.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
E29A2

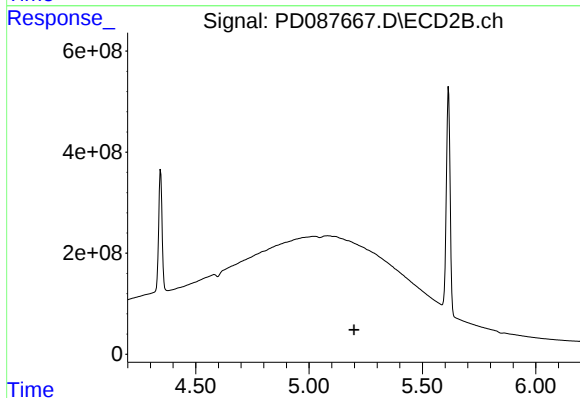


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.198 min
Response: 0
Conc: N.D.

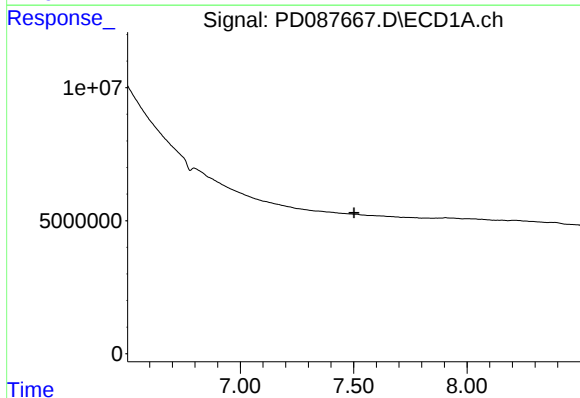


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.502 min
Response: 0
Conc: N.D.

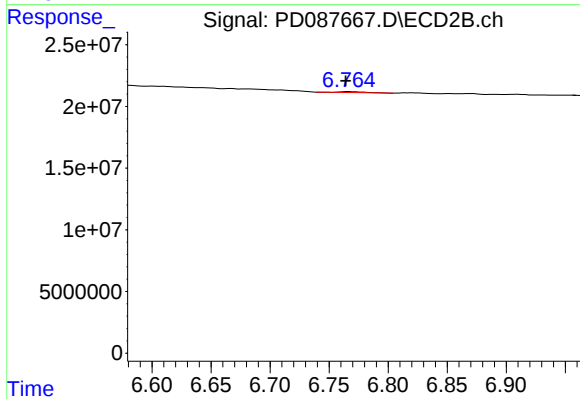

#20 Methoxychlor


R.T.: 6.766 min
Delta R.T.: 0.002 min
Response: 1134205
Conc: 0.18 ng/ml

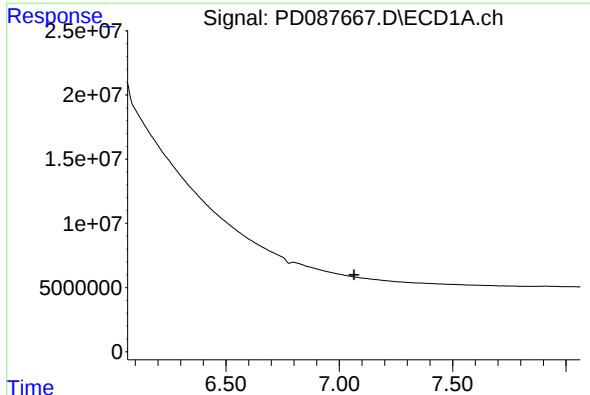

#24 Toxaphene-3


R.T.: 0.000 min
Exp R.T.: 7.065 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
E29A2

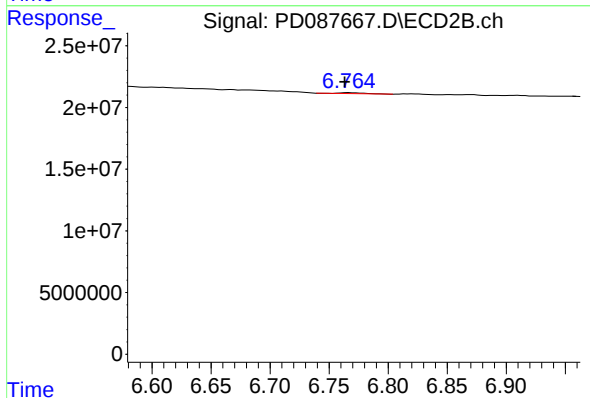


#24 Toxaphene-3

R.T.: 6.766 min
Delta R.T.: 0.003 min
Response: 1134205
Conc: 3.81 ng/ml

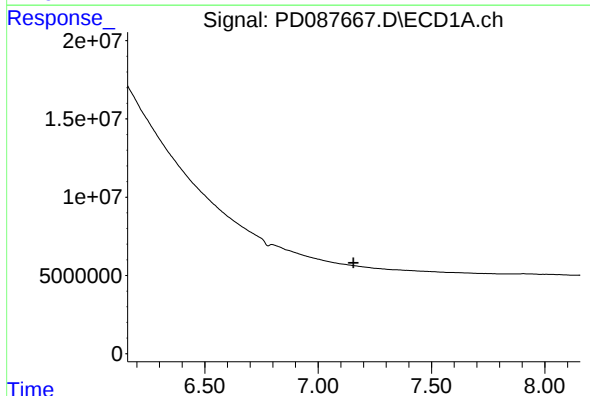


#25 Toxaphene-4

R.T.: 0.000 min
Exp R.T.: 7.156 min
Response: 0
Conc: N.D.

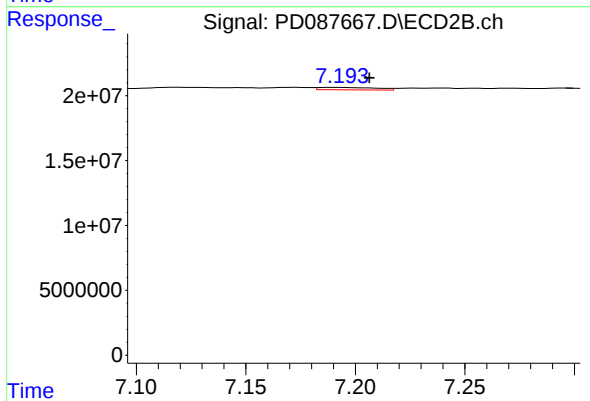

#25 Toxaphene-4


R.T.: 7.191 min
Delta R.T.: -0.016 min
Response: 3388069
Conc: 15.99 ng/ml

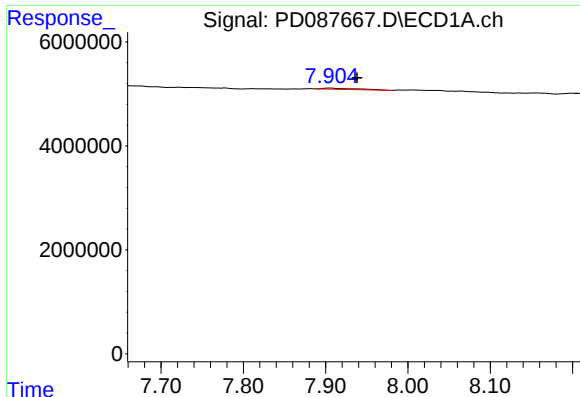

#26 Toxaphene-5


R.T.: 7.905 min
Delta R.T.: -0.033 min
Response: 660688
Conc: 13.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
E29A2

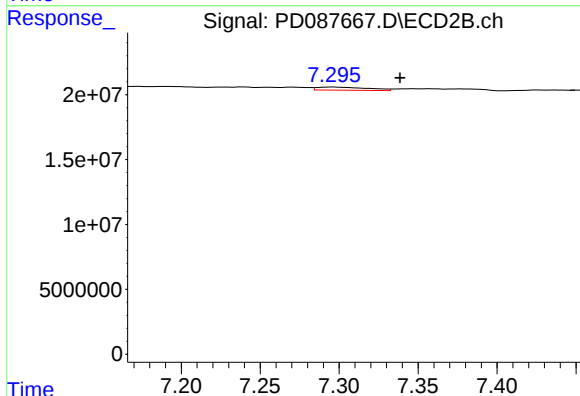


#26 Toxaphene-5

R.T.: 7.296 min
Delta R.T.: -0.043 min
Response: 5494306
Conc: 35.43 ng/ml

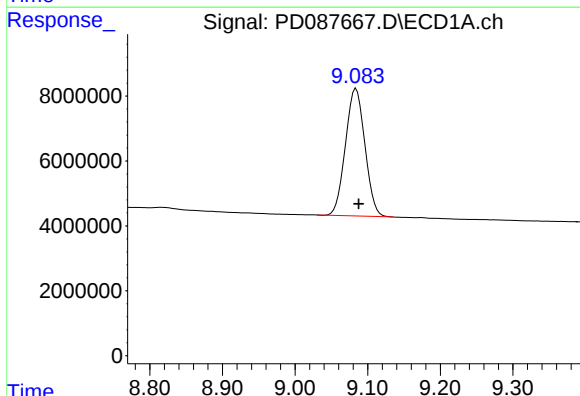

#27 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: -0.003 min
Response: 73039109
Conc: 21.85 ng/ml

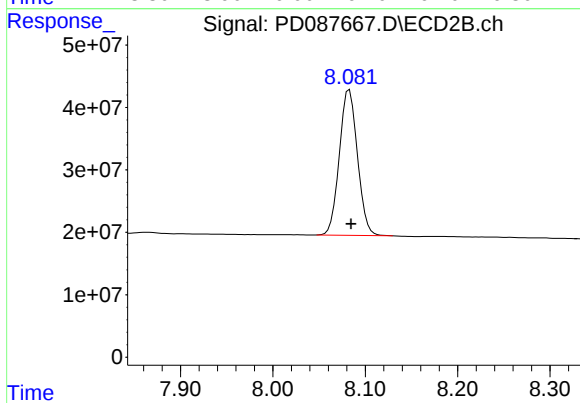

#27 Decachlorobiphenyl

R.T.: 8.083 min
Delta R.T.: -0.002 min
Response: 317702031
Conc: 21.93 ng/ml