

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020325\
 Data File : PD087689.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2025 20:15
 Operator : AR\AJ
 Sample : Q1226-18MS
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCZN8MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/04/2025
 Supervised By : Ankita Jodhani 02/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 08:28:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 16 13:39:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.553	2.898	52631202	2453.8E6	25.825m	198.399m#
27)	SA Decachlor...	9.086	8.083	67939898	306.4E6	20.321	21.157
Target Compounds							
2)	A alpha-BHC	4.006	3.396	248.5E6	1096.1E6	59.816	55.352
3)	MA gamma-BHC...	4.334	3.734	393.1E6	1005.4E6	97.711m	54.889 #
4)	MA Heptachlor	4.938	4.087	212.5E6	955.7E6	51.977	51.203m
5)	MB Aldrin	5.280	4.374	233.4E6	924.2E6	58.267	51.132
6)	B beta-BHC	4.520	4.030	101.0E6	397.8E6	56.225m	46.636
7)	B delta-BHC	4.771	4.267	249.5E6	1023.0E6	60.387	54.811
8)	B Heptachlo...	5.699	4.879	184.1E6	845.9E6	49.287	49.979
9)	A Endosulfan I	6.082	5.254	172.6E6	779.4E6	49.550m	49.106
10)	B trans-Chl...	5.954	5.133	180.4E6	875.1E6	48.957	48.679
11)	B cis-Chlor...	6.034	5.197	187.1E6	859.1E6	50.327m	49.639
12)	B 4,4'-DDE	6.203	5.383	353.8E6	1620.2E6	100.448m	98.920
13)	MA Dieldrin	6.354	5.520	392.2E6	1685.1E6	102.888m	100.963
14)	MA Endrin	6.583	5.796	323.5E6	1511.7E6	99.667	101.168
15)	B Endosulfa...	6.794	6.088	307.4E6	1435.7E6	95.476	96.914
16)	A 4,4'-DDD	6.713	5.937	278.6E6	1348.1E6	101.314	100.833
17)	MA 4,4'-DDT	7.028	6.192	286.9E6	1370.1E6	98.991m	99.423
18)	B Endrin al...	6.923	6.266	228.5E6	1064.0E6	90.701	92.292
19)	B Endosulfa...	7.157	6.490	299.7E6	1409.3E6	97.077	96.943
20)	A Methoxychlor	7.502	6.764	719.4E6	2774.6E6	454.046	450.469
21)	B Endrin ke...	7.637	7.000	328.5E6	1513.0E6	95.420m	95.263

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020325\
Data File : PD087689.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2025 20:15
Operator : AR\AJ
Sample : Q1226-18MS
Misc :
ALS Vial : 41 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 08:28:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 16 13:39:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

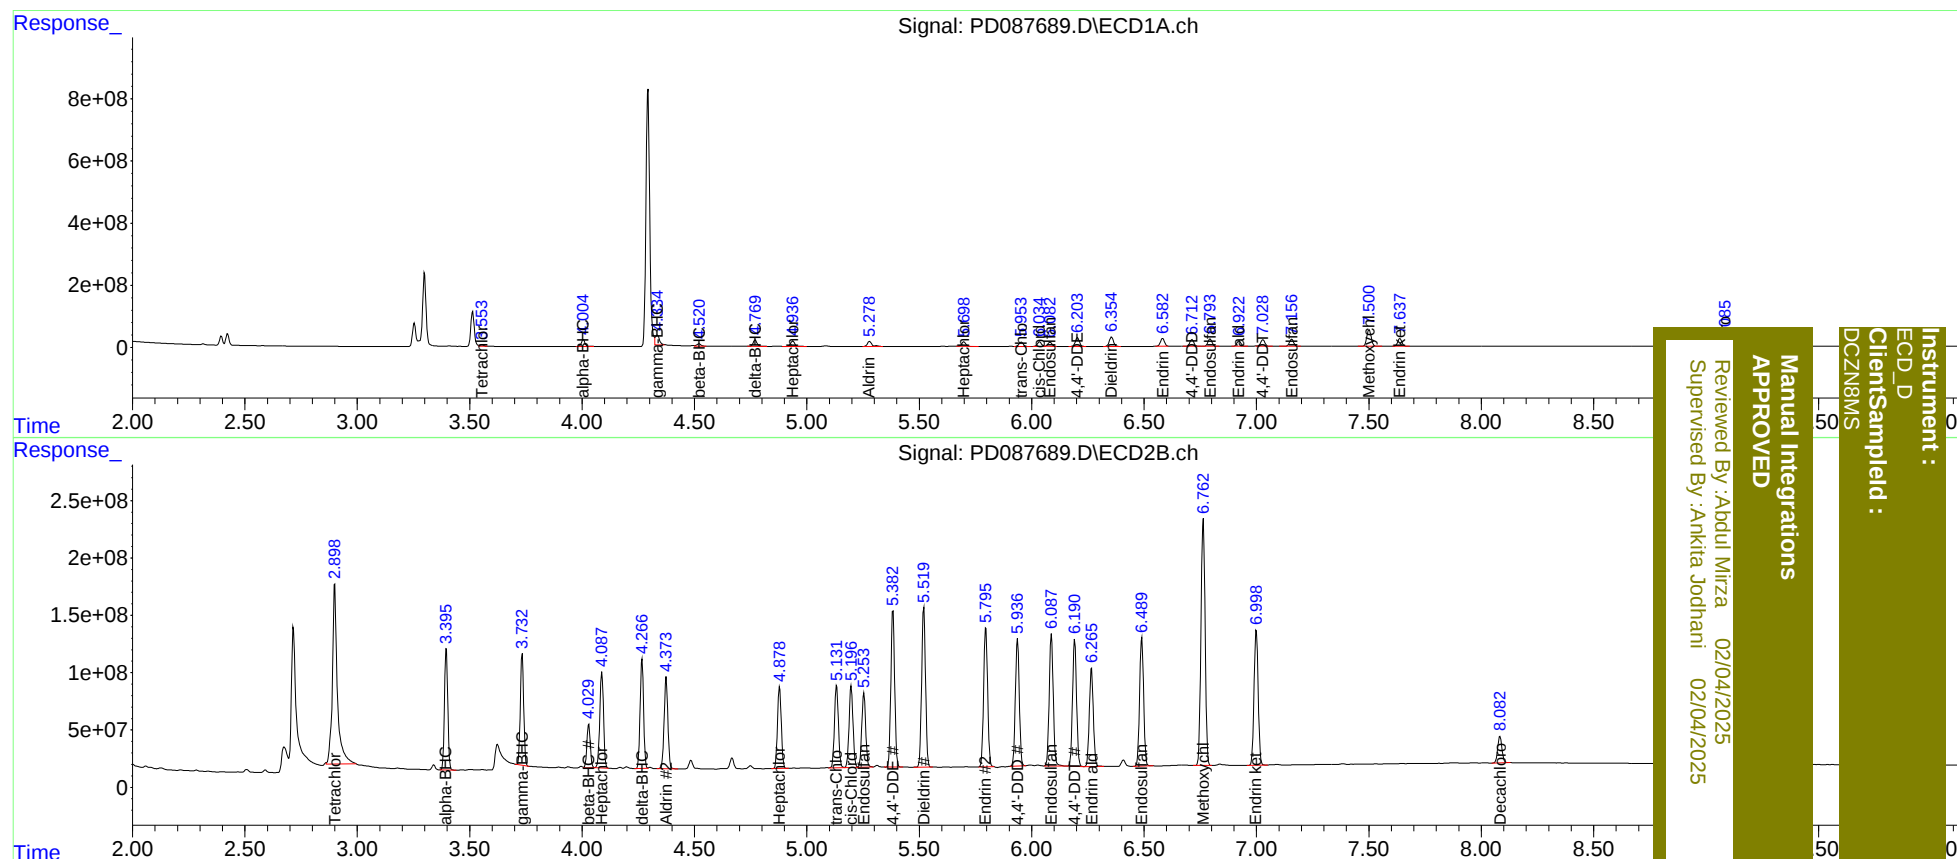

Instrument :
ECD_D
Client Sampled :
DCZN8MS

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 02/04/2025
Supervised By: Ankita Jodhani 02/04/2025