

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020325\
 Data File : PD087659.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2025 13:10
 Operator : AR\AJ
 Sample : Q1202-02MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E2975MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/04/2025
 Supervised By :Ankita Jodhani 02/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 08:16:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 16 13:39:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.555	2.882	34395621	234.4E6	16.877	18.955
27) SA Decachlor...	9.084	8.083	56743406	257.5E6	16.972	17.778
Target Compounds						
2) A alpha-BHC	4.005	3.396	218.7E6	1000.6E6	52.635	50.529
3) MA gamma-BHC...	4.336	3.733	208.9E6	914.2E6	51.936	49.912
4) MA Heptachlor	4.936	4.088	195.7E6	861.2E6	47.868	46.144
5) MB Aldrin	5.278	4.374	187.4E6	851.3E6	46.785	47.098
6) B beta-BHC	4.521	4.029	78706590	385.1E6	43.822	45.138
7) B delta-BHC	4.770	4.266	213.8E6	929.5E6	51.749	49.802
8) B Heptachlo...	5.698	4.879	175.7E6	795.2E6	47.022	46.980
9) A Endosulfan I	6.080	5.253	162.2E6	748.6E6	46.560m	47.161
10) B trans-Chl...	5.953	5.132	168.0E6	826.8E6	45.597	45.992
11) B cis-Chlor...	6.033	5.197	173.6E6	816.9E6	46.699m	47.200
12) B 4,4'-DDE	6.202	5.382	327.1E6	1517.0E6	92.884m	92.618
13) MA Dieldrin	6.355	5.519	364.2E6	1562.2E6	95.537	93.597
14) MA Endrin	6.582	5.796	300.4E6	1384.7E6	92.561	92.670
15) B Endosulfa...	6.793	6.087	289.0E6	1341.8E6	89.771	90.570
16) A 4,4'-DDD	6.712	5.936	254.9E6	1228.1E6	92.704	91.857
17) MA 4,4'-DDT	7.028	6.191	258.9E6	1237.2E6	89.336m	89.774
18) B Endrin al...	6.922	6.266	210.8E6	986.0E6	83.652	85.524
19) B Endosulfa...	7.156	6.490	278.1E6	1314.4E6	90.063	90.419
20) A Methoxychlor	7.500	6.763	666.0E6	2452.7E6	420.347	398.218
21) B Endrin ke...	7.638	6.999	299.9E6	1396.3E6	87.097	87.919

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020325\
Data File : PD087659.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2025 13:10
Operator : AR\AJ
Sample : Q1202-02MS
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 08:16:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 16 13:39:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

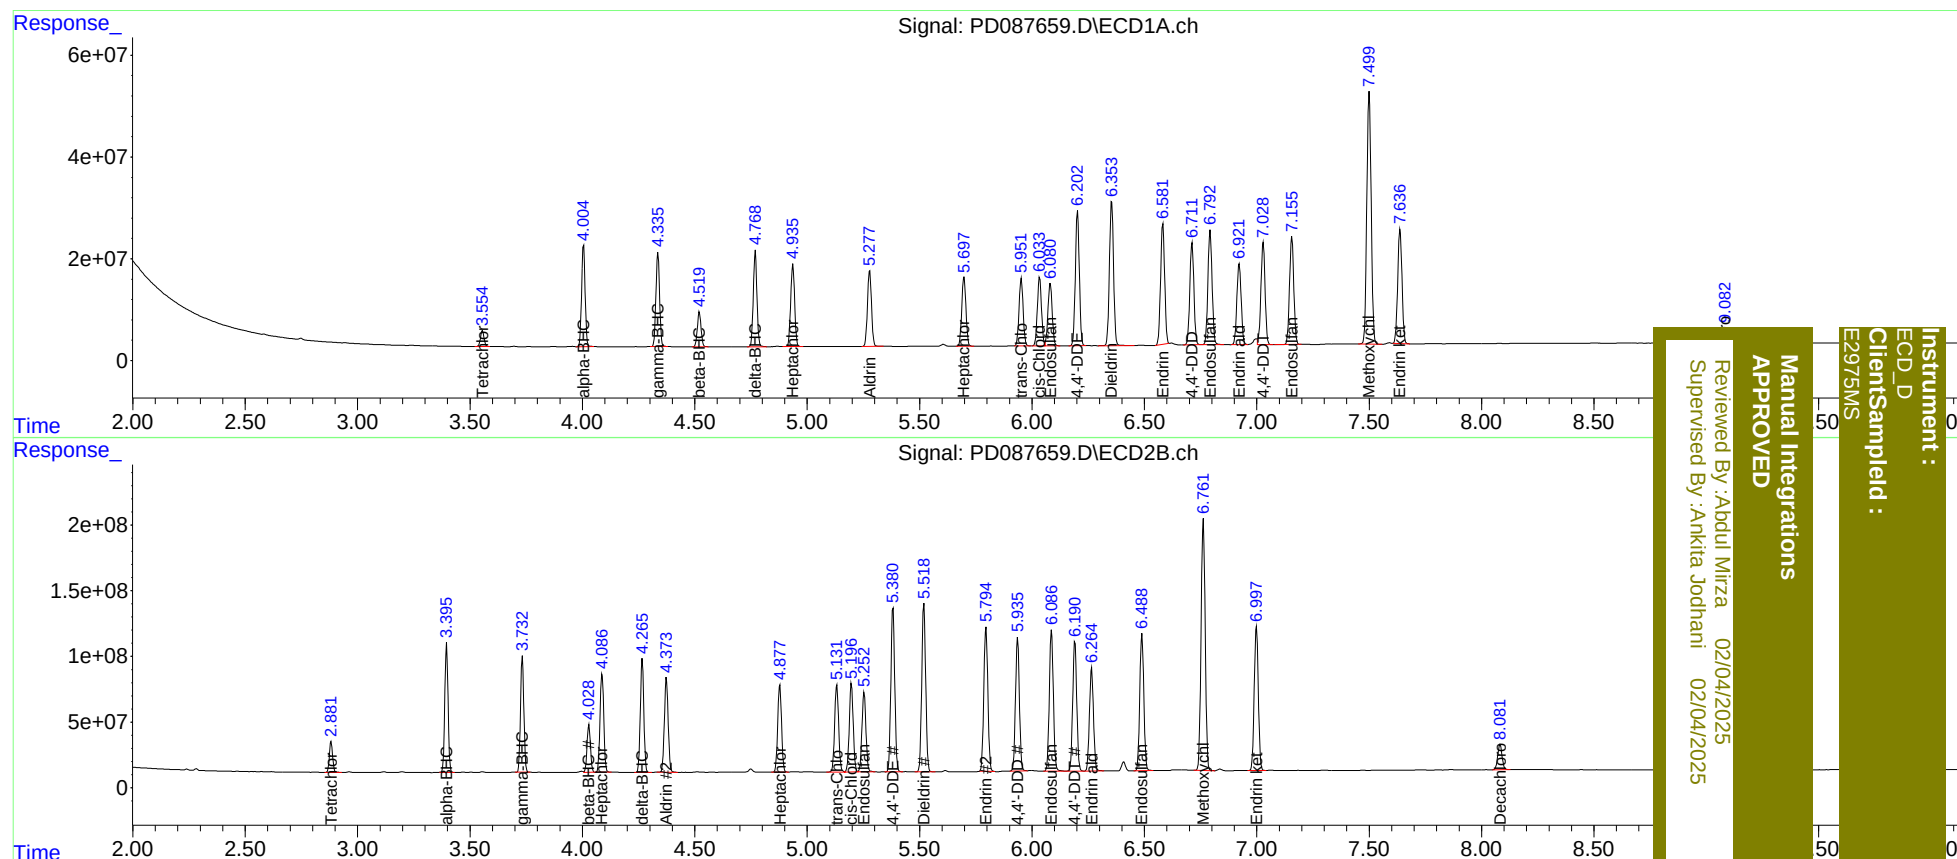

280.0

Reviewed By: Abdul Mirza 02/04/2025
Supervised By: Ankita Jodhani 02/04/2025

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
EZ975MS