

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020325\
 Data File : PD087664.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2025 14:20
 Operator : AR\AJ
 Sample : Q1202-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E2980

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/04/2025
 Supervised By : Ankita Jodhani 02/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 08:18:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 16 13:39:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.556	2.882	32330673	277.7E6	15.864	22.457 #
27) SA Decachlor...	9.084	8.083	49965167	212.6E6	14.945	14.679
Target Compounds						
3) MA gamma-BHC...	4.349	3.746	1947338	12752100	0.484m	0.696m#
4) MA Heptachlor	4.948	4.091	2405434	7895084	0.588	0.423 #
9) A Endosulfan I	6.071	5.262	5164588	14329231	1.482m	0.903 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020325\
Data File : PD087664.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2025 14:20
Operator : AR\AJ
Sample : Q1202-08
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 08:18:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 16 13:39:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

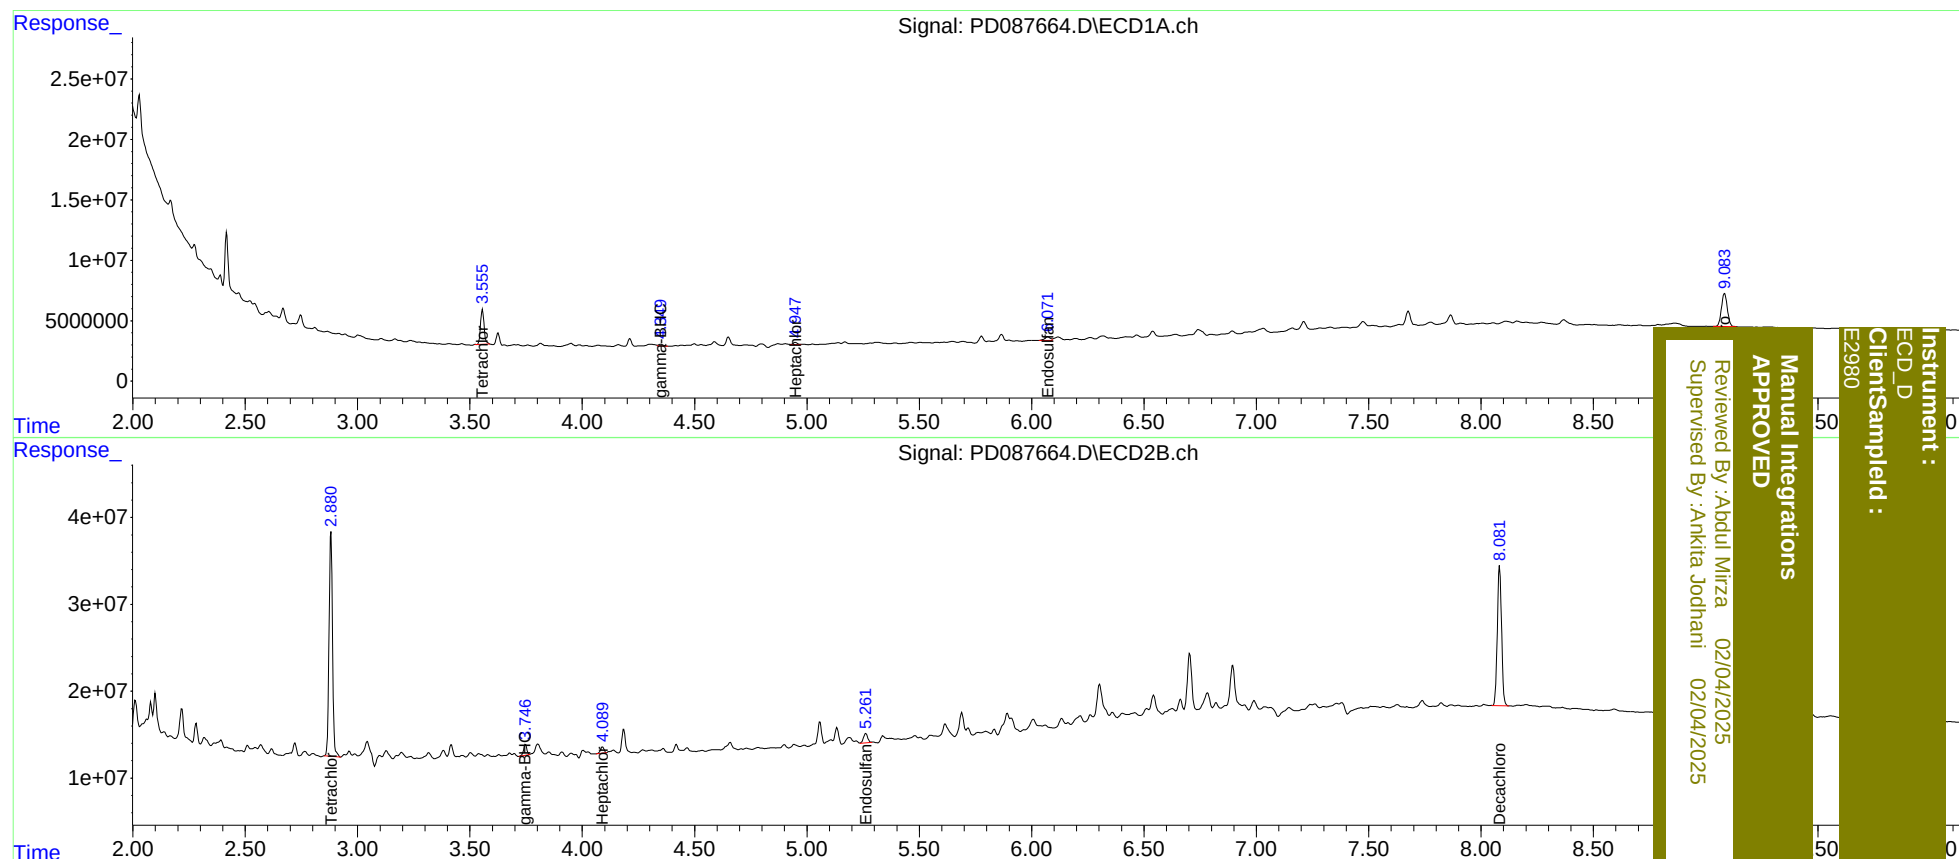

Instrument :
ECD_D
ClientSampled :
E2980

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/04/2025
Supervised By :Ankita Jodhani 02/04/2025