

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020325\
 Data File : PD087682.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2025 18:36
 Operator : AR\AJ
 Sample : Q1226-08
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCZP0

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/04/2025
 Supervised By : Ankita Jodhani 02/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 08:25:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 16 13:39:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.554	2.883	48002689	169.6E6	23.554m	13.717m#
27) SA Decachlor...	9.085	8.084	67947208	314.1E6	20.323	21.687
Target Compounds						
2) A alpha-BHC	4.006	3.396	60272397	333.9E6	14.508	16.860
3) MA gamma-BHC...	4.326	3.733	24580144	56988895	6.111m	3.111 #
6) B beta-BHC	4.521	4.030	12674010	64800024	7.057	7.596
7) B delta-BHC	4.770	4.267	726.3E6	2757.7E6	175.770	147.757

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD087682\
Data File : PD087682.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2025 18:36
Operator : AR\AJ
Sample : Q1226-08
Misc :
ALS Vial : 34 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 08:25:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 16 13:39:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

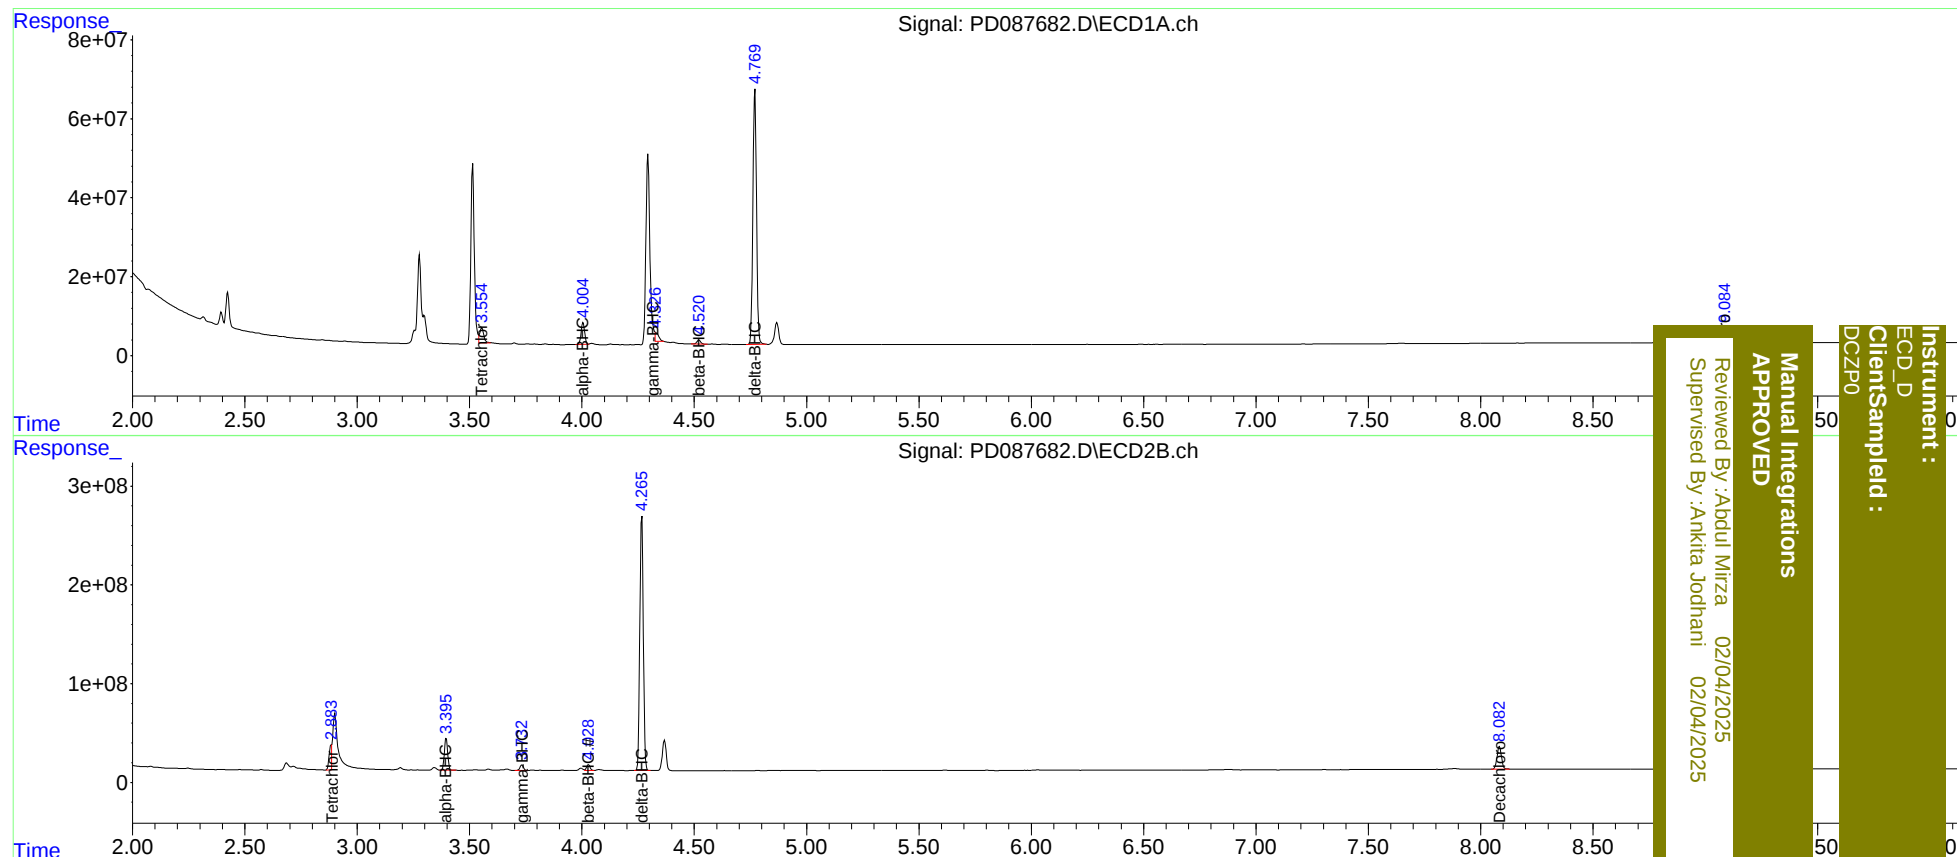

Instrument :
ECD_D
ClientSampled :
DCZP0

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/04/2025
Supervised By : Ankita Jodhani 02/04/2025