

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020421\
 Data File : PD061105.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2021 08:36
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 00:46:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 26 00:33:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
Target Compounds							
6) B	beta-BHC	4.435f	4.909f	660193	600138	1.059	0.140 #
7) B	delta-BHC	0.000	5.060	0	2960558	N.D.	0.290
8) B	Heptachlo...	5.293f	5.894	1343584	31798928	0.987	3.670 #
9) A	Endosulfan I	0.000	6.229	0	1317160	N.D.	0.153
11) B	cis-Chlor...	0.000	6.229	0	1317160	N.D.	0.148
18) B	Endrin al...	0.000	7.050	0	6250833	N.D.	1.054
20) A	Methoxychlor	7.046f	0.000	2327822	0	3.729	N.D. #
21) B	Endrin ke...	7.176f	0.000	295649	0	0.229	N.D. #
22)	Toxaphene-1	0.000	6.434	0	6439650	N.D.	118.149
23)	Toxaphene-2	5.910	0.000	1689104	0	136.495	N.D. #
24)	Toxaphene-3	0.000	7.050	0	6250833	N.D.	65.247
26)	Toxaphene-5	7.125	0.000	990935	0	28.521	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020421\
Data File : PD061105.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2021 08:36
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 00:46:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jan 26 00:33:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

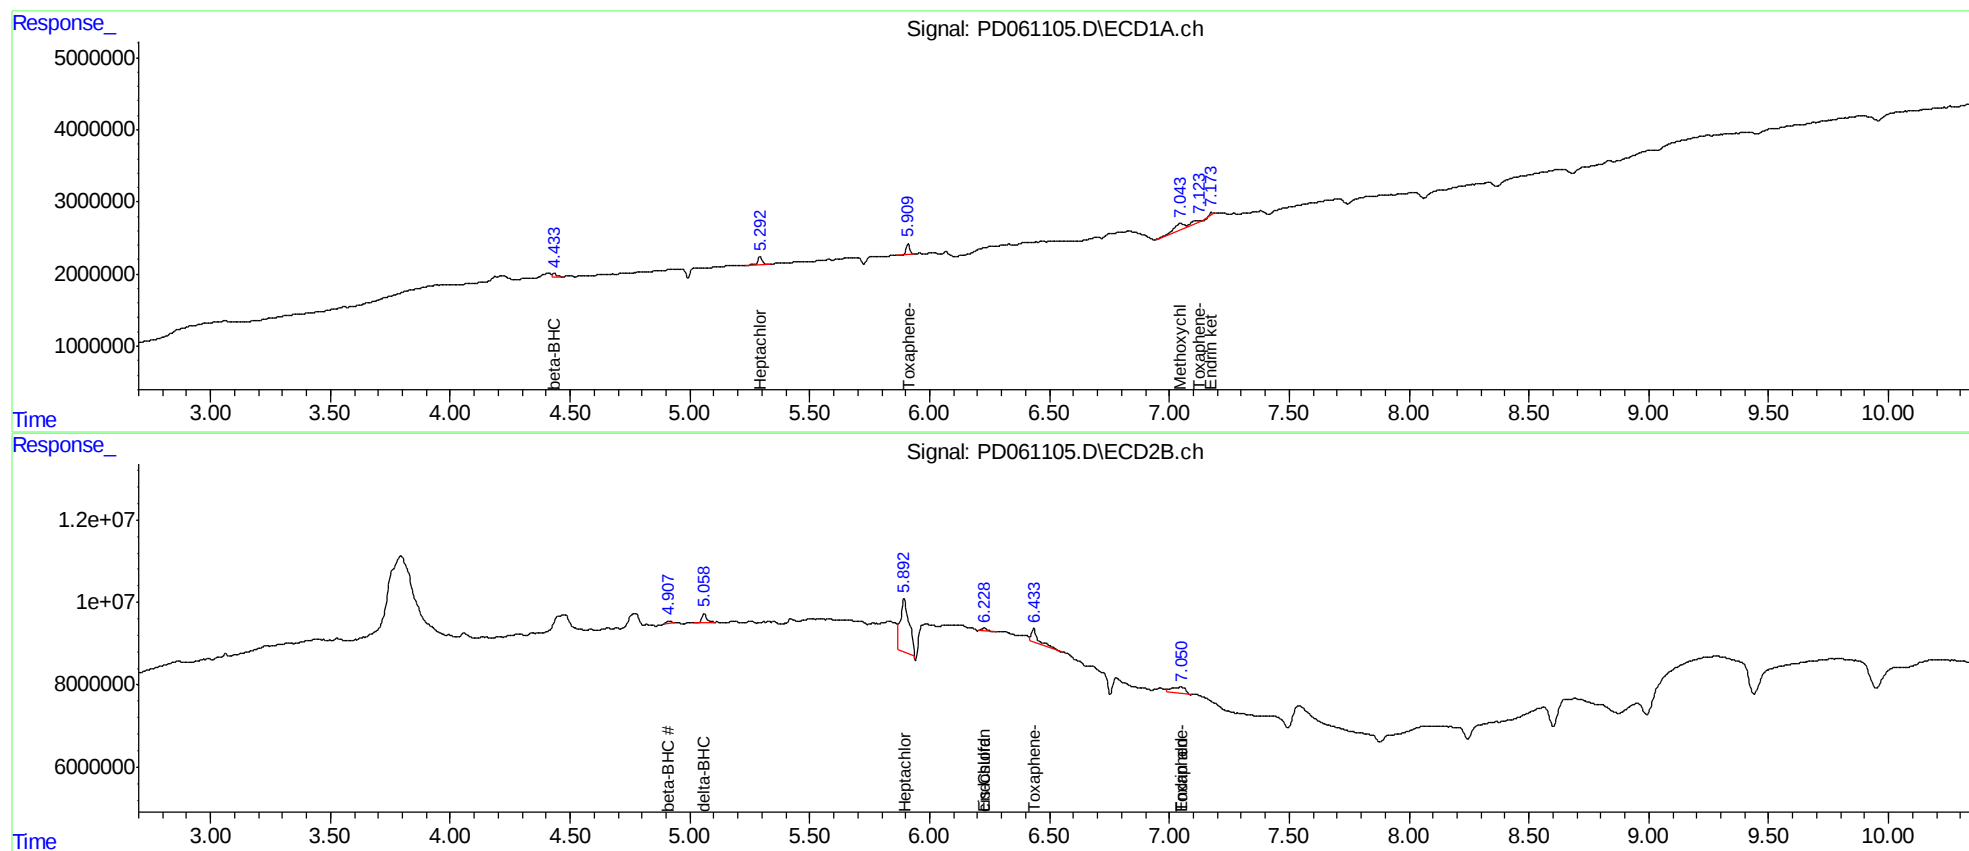


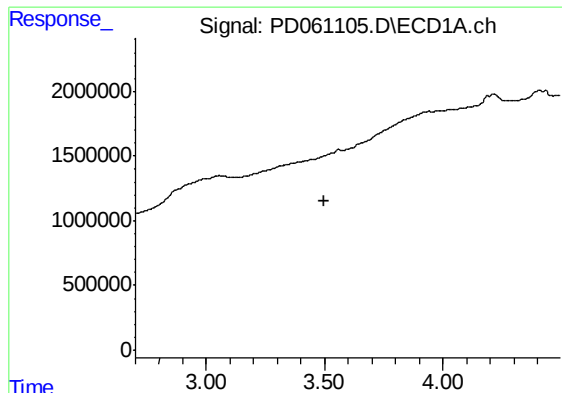

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.497 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

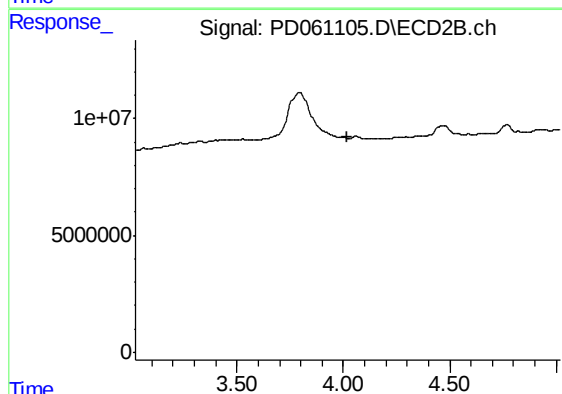


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.021 min
Response: 0
Conc: N.D.

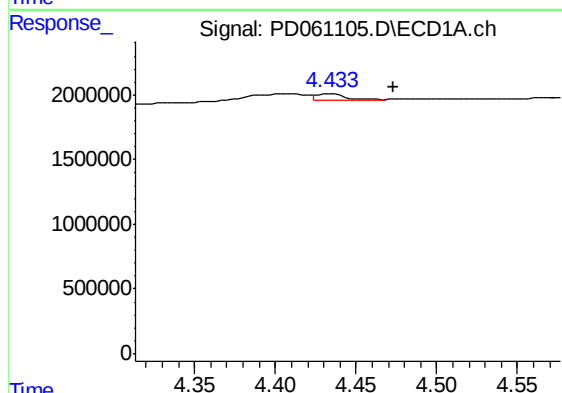


#6 beta-BHC

R.T.: 4.435 min
Delta R.T.: -0.038 min
Response: 660193
Conc: 1.06 ng/ml

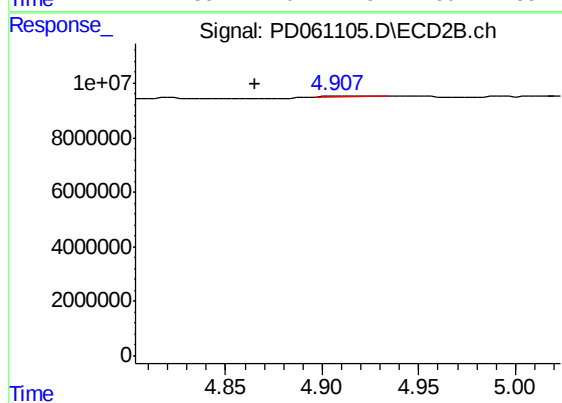

#6 beta-BHC


R.T.: 4.909 min
Delta R.T.: 0.044 min
Response: 600138
Conc: 0.14 ng/ml

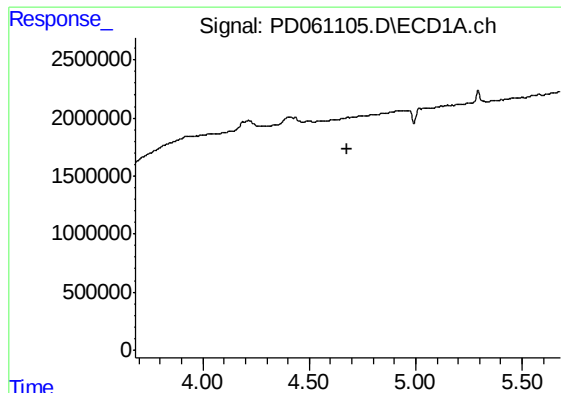

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.680 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

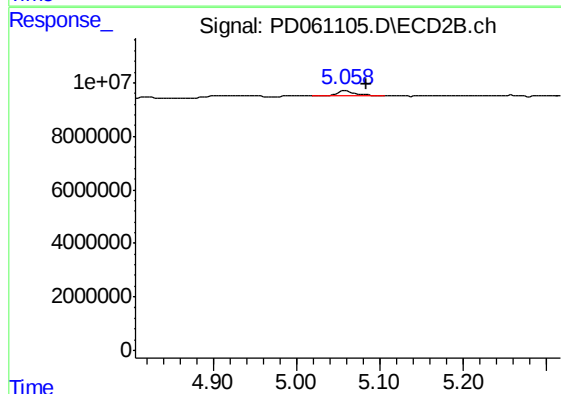


#7 delta-BHC

R.T.: 5.060 min
Delta R.T.: -0.024 min
Response: 2960558
Conc: 0.29 ng/ml

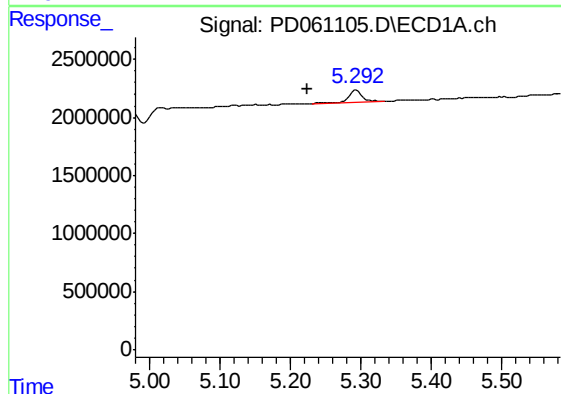


#8 Heptachlor epoxide

R.T.: 5.293 min
Delta R.T.: 0.070 min
Response: 1343584
Conc: 0.99 ng/ml

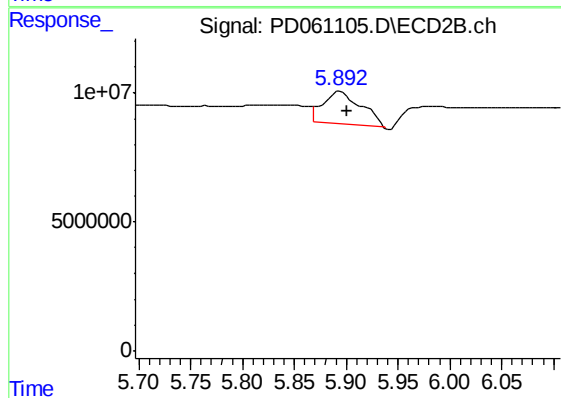

#8 Heptachlor epoxide


R.T.: 5.894 min
Delta R.T.: -0.008 min
Response: 31798928
Conc: 3.67 ng/ml

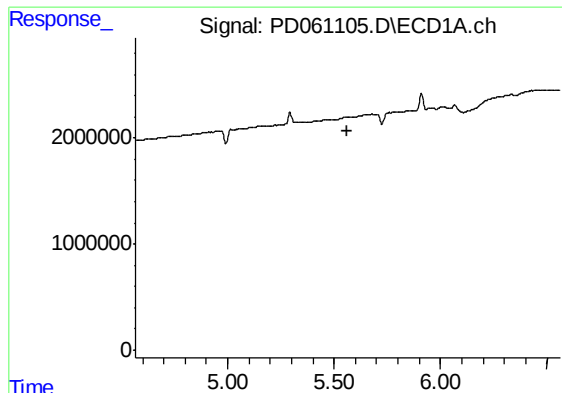

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.564 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

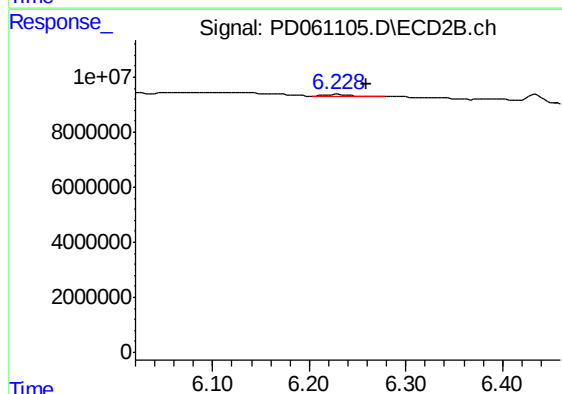


#9 Endosulfan I

R.T.: 6.229 min
Delta R.T.: -0.030 min
Response: 1317160
Conc: 0.15 ng/ml

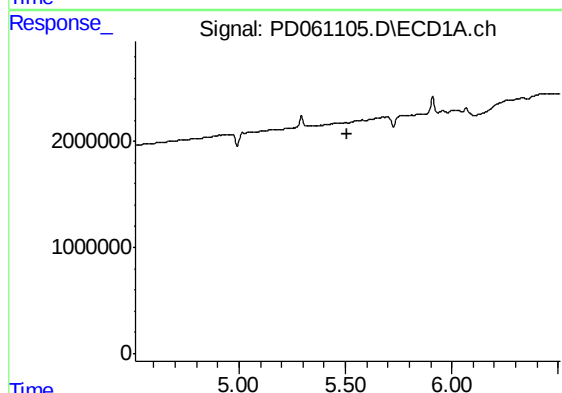


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.511 min
Response: 0
Conc: N.D.

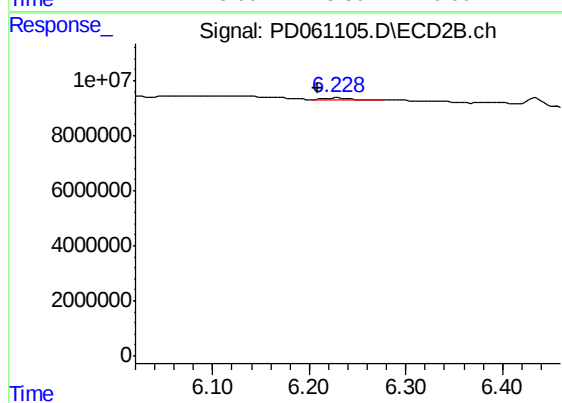

#11 cis-Chlordane


R.T.: 6.229 min
Delta R.T.: 0.020 min
Response: 1317160
Conc: 0.15 ng/ml

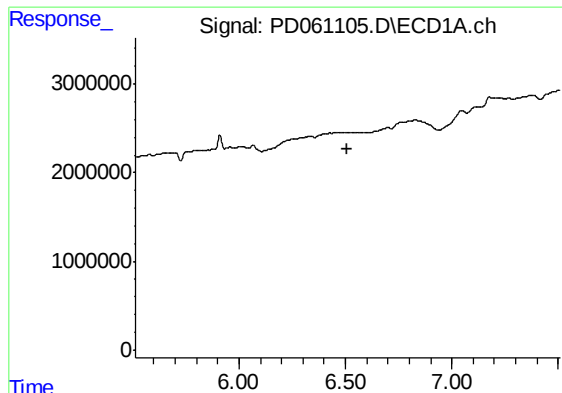

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.511 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

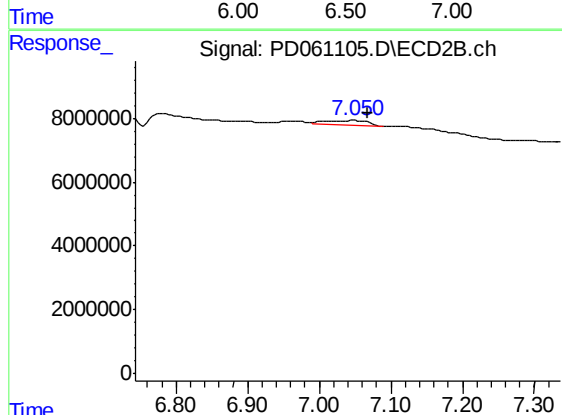


#18 Endrin aldehyde

R.T.: 7.050 min
Delta R.T.: -0.018 min
Response: 6250833
Conc: 1.05 ng/ml

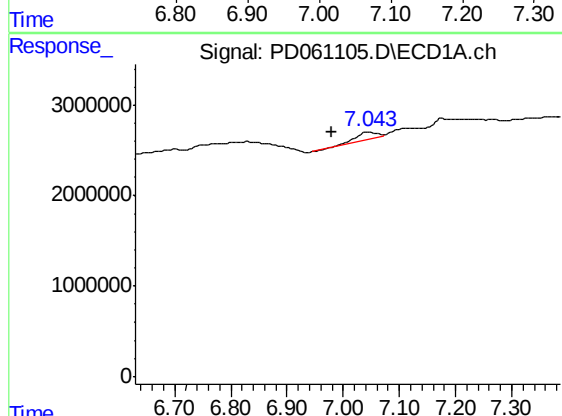


#20 Methoxychlor

R.T.: 7.046 min
Delta R.T.: 0.065 min
Response: 2327822
Conc: 3.73 ng/ml

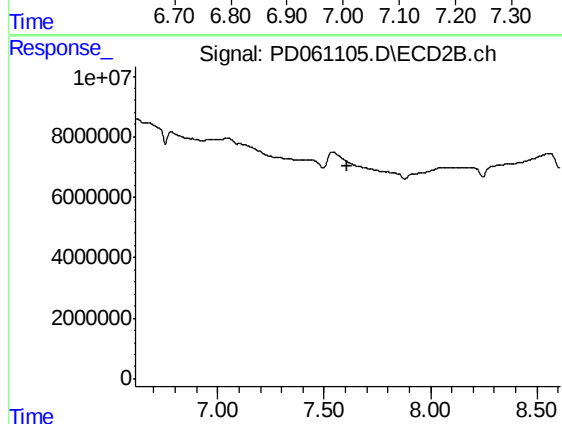

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.611 min
Response: 0
Conc: N.D.

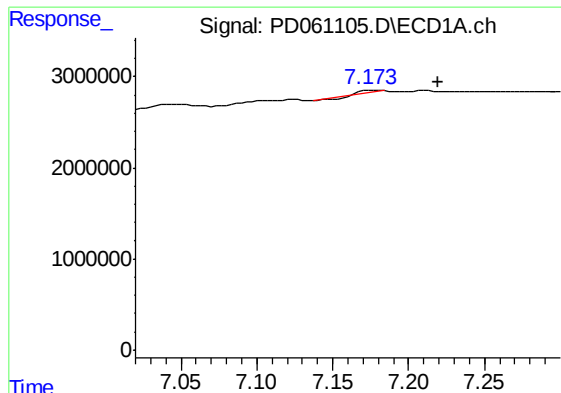

#21 Endrin ketone


R.T.: 7.176 min
Delta R.T.: -0.044 min
Response: 295649
Conc: 0.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

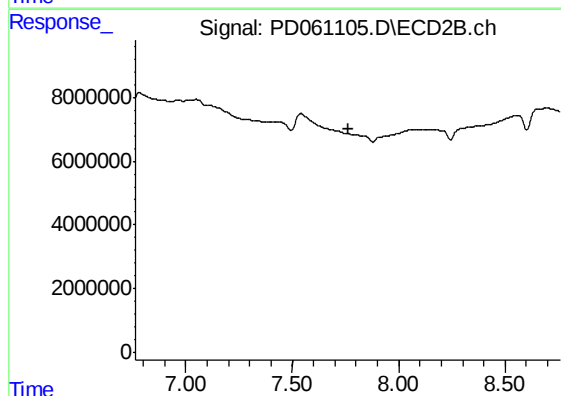


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.763 min
Response: 0
Conc: N.D.

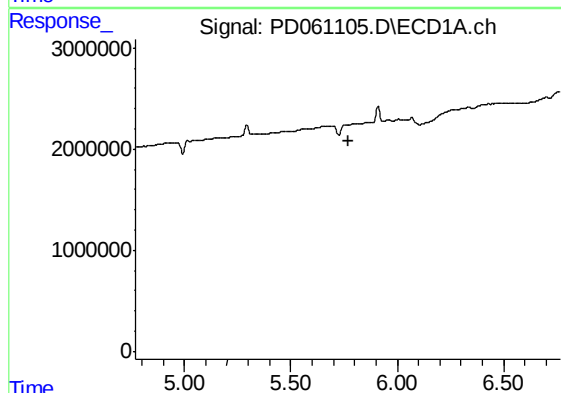


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T. : 5.770 min
Response: 0
Conc: N.D.

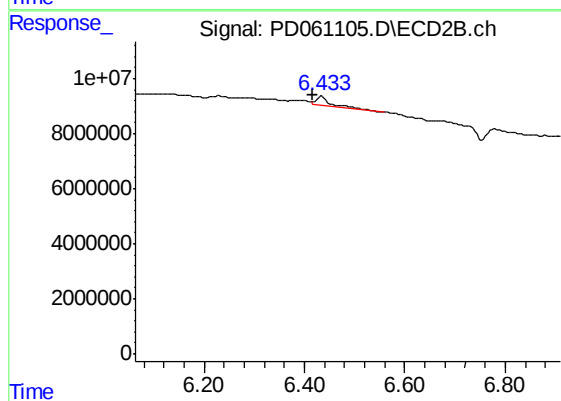

#22 Toxaphene-1


R.T.: 6.434 min
Delta R.T.: 0.019 min
Response: 6439650
Conc: 118.15 ng/ml

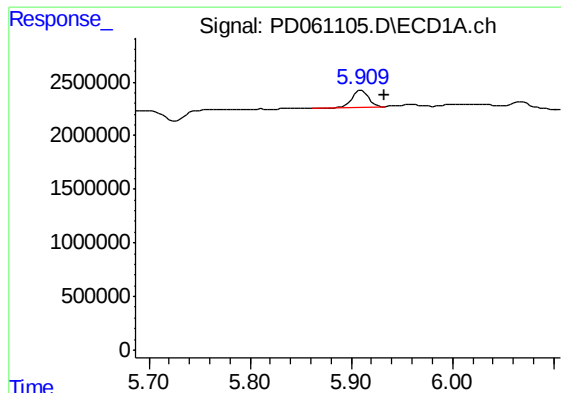

#23 Toxaphene-2


R.T.: 5.910 min
Delta R.T.: -0.022 min
Response: 1689104
Conc: 136.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

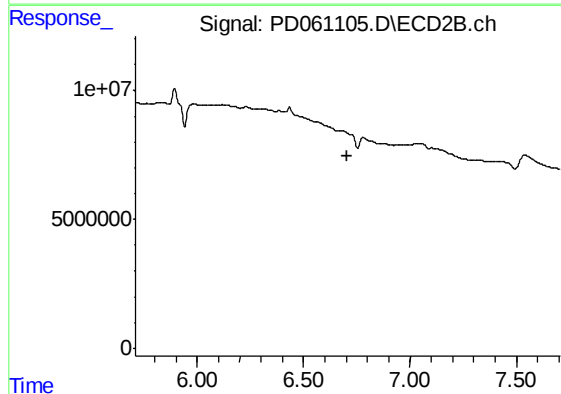


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T. : 6.707 min
Response: 0
Conc: N.D.

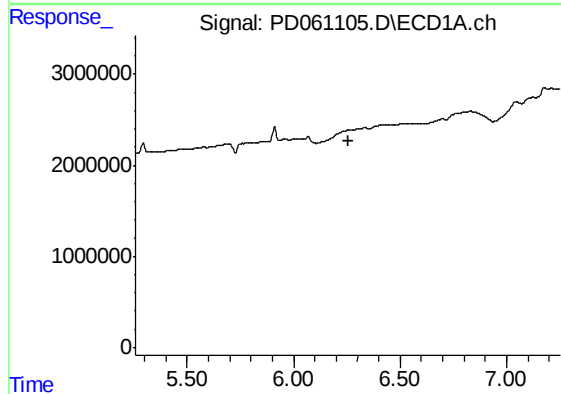


#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T. : 6.256 min
Response: 0
Conc: N.D.

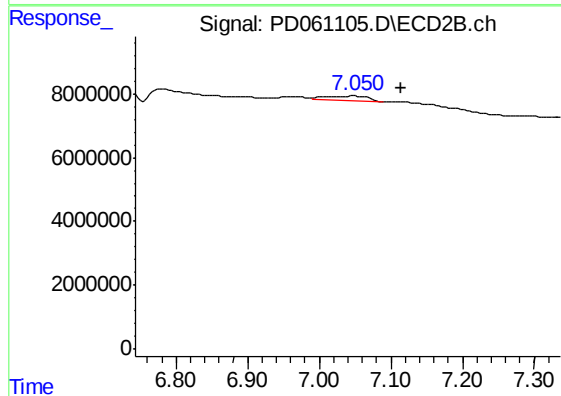

#24 Toxaphene-3


R.T.: 7.050 min
Delta R.T.: -0.065 min
Response: 6250833
Conc: 65.25 ng/ml

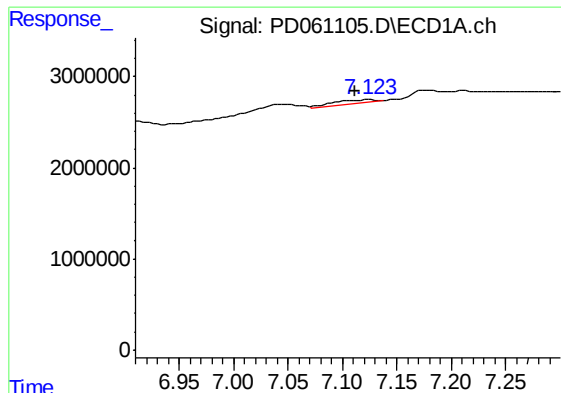

#26 Toxaphene-5


R.T.: 7.125 min
Delta R.T.: 0.013 min
Response: 990935
Conc: 28.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

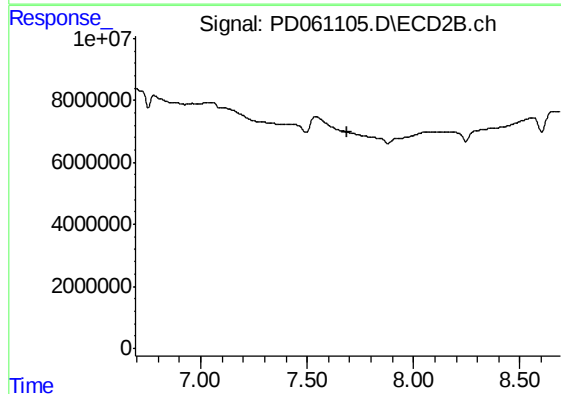


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T. : 7.692 min
Response: 0
Conc: N.D.

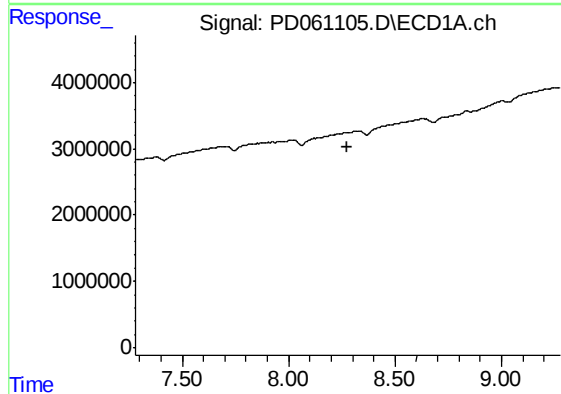

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.278 min
Response: 0
Conc: N.D.

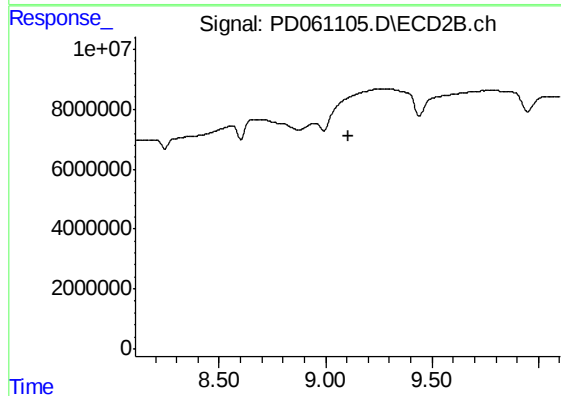

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.106 min
Response: 0
Conc: N.D.