

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020421\
 Data File : PD061118.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2021 11:44
 Operator : DD\AJ
 Sample : M1274-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AD2

Manual Integrations
 APPROVED

Ankita
 2/8/2021 8:44:46 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 00:52:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 26 00:33:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	3.993f	4228.8E6	28430.1E6	4166.273m	3973.015m
27)	SA Decachlor...	8.276	9.106	33914503	208.2E6	26.916	30.656
Target Compounds							
8)	B Heptachlo...	5.216	5.891	6104915	7717853	4.486	0.891 #
13)	MA Dieldrin	5.808	6.517	12596087	83504578	8.578	8.982
14)	MA Endrin	6.081	6.746	2917338	22452952	2.347	3.039 #
17)	MA 4,4'-DDT	6.433	7.136	4535690	26626224	3.704	3.667

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020421\
Data File : PD061118.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2021 11:44
Operator : DD\AJ
Sample : M1274-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 00:52:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jan 26 00:33:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

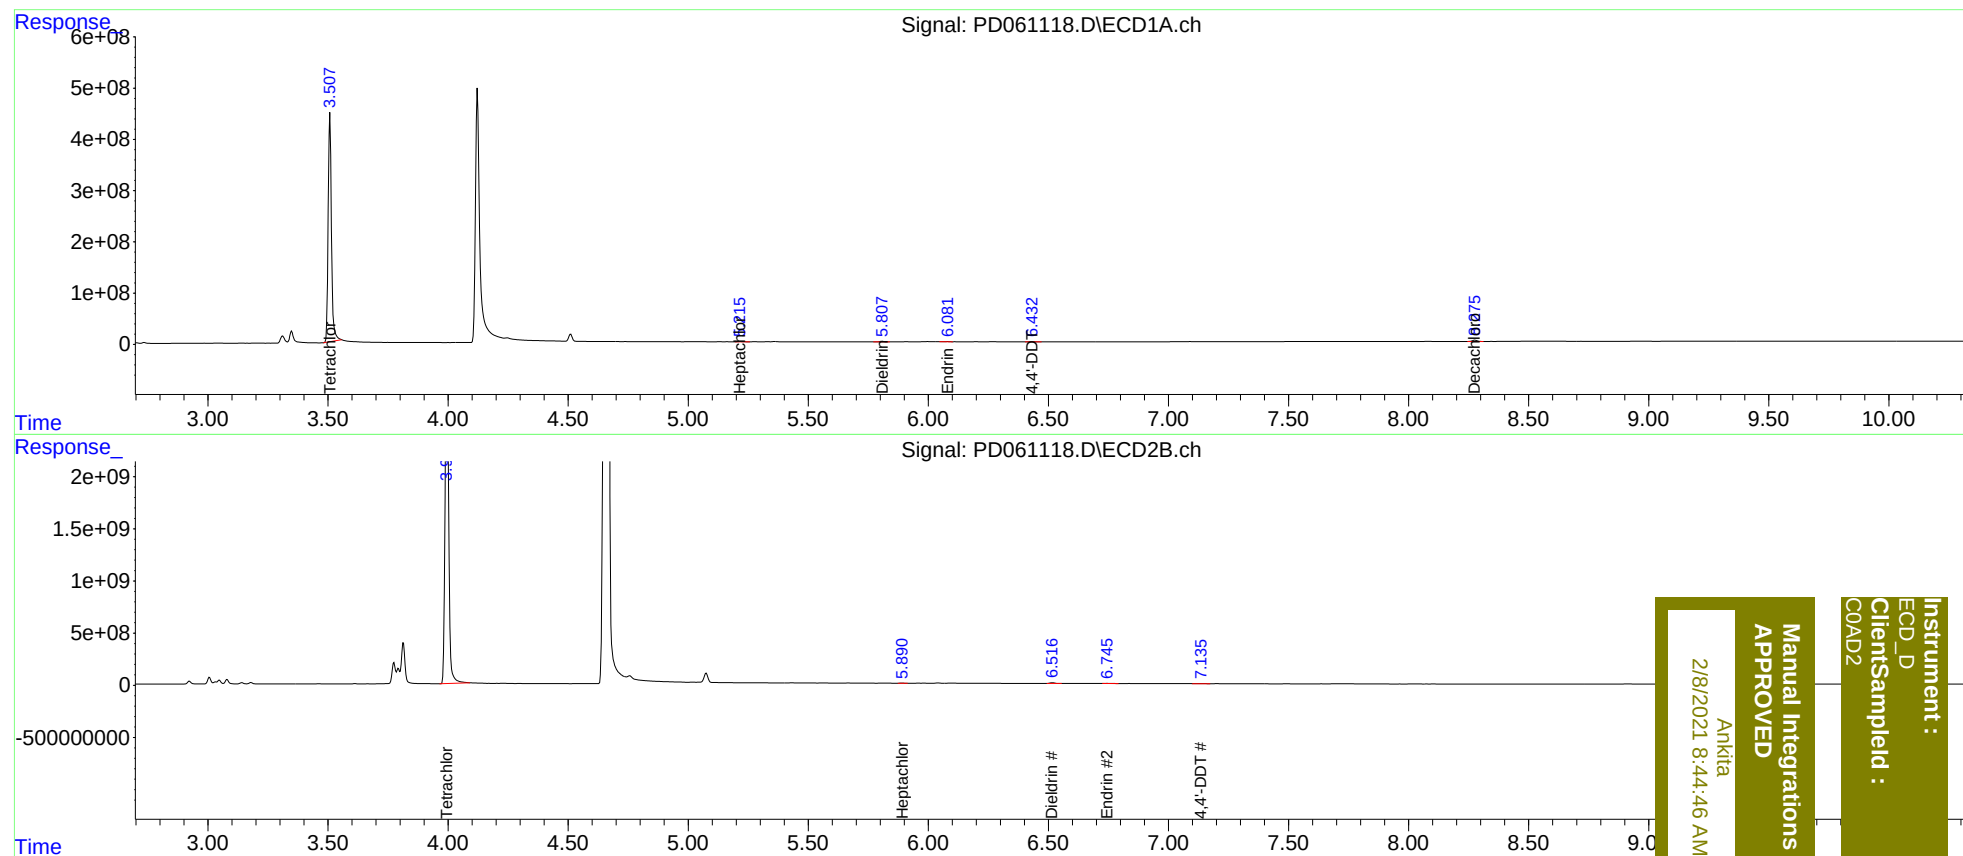

Manual Integrations
APPROVED

Ankita

2/8/2021 8:44:46 AM

Instrument :
ECD_D
ClientSampleId :
C0AD2