

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020421\
 Data File : PD061113.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2021 10:34
 Operator : DD\AJ
 Sample : M1274-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AC5

Manual Integrations
 APPROVED

Ankita
 2/8/2021 8:44:37 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 00:49:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 26 00:33:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.495	4.021	21137970	151.6E6	20.826	21.182
27)	SA Decachlor...	8.277	9.106	41680111	260.3E6	33.079	38.328
Target Compounds							
3)	MA gamma-BHC...	4.221	4.697	7681044	55319778	5.250	5.453
8)	B Heptachlo...	5.221	5.900	10780116	111.6E6	7.921m	12.876 #
10)	B trans-Chl...	5.451	6.134	3457685	43722867	2.445	4.651m#
11)	B cis-Chlor...	5.508	6.210	5704156	48009777	4.157	5.404 #
13)	MA Dieldrin	5.808	6.517	58446436	423.3E6	39.803	45.527

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020421\
Data File : PD061113.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2021 10:34
Operator : DD\AJ
Sample : M1274-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 00:49:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jan 26 00:33:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

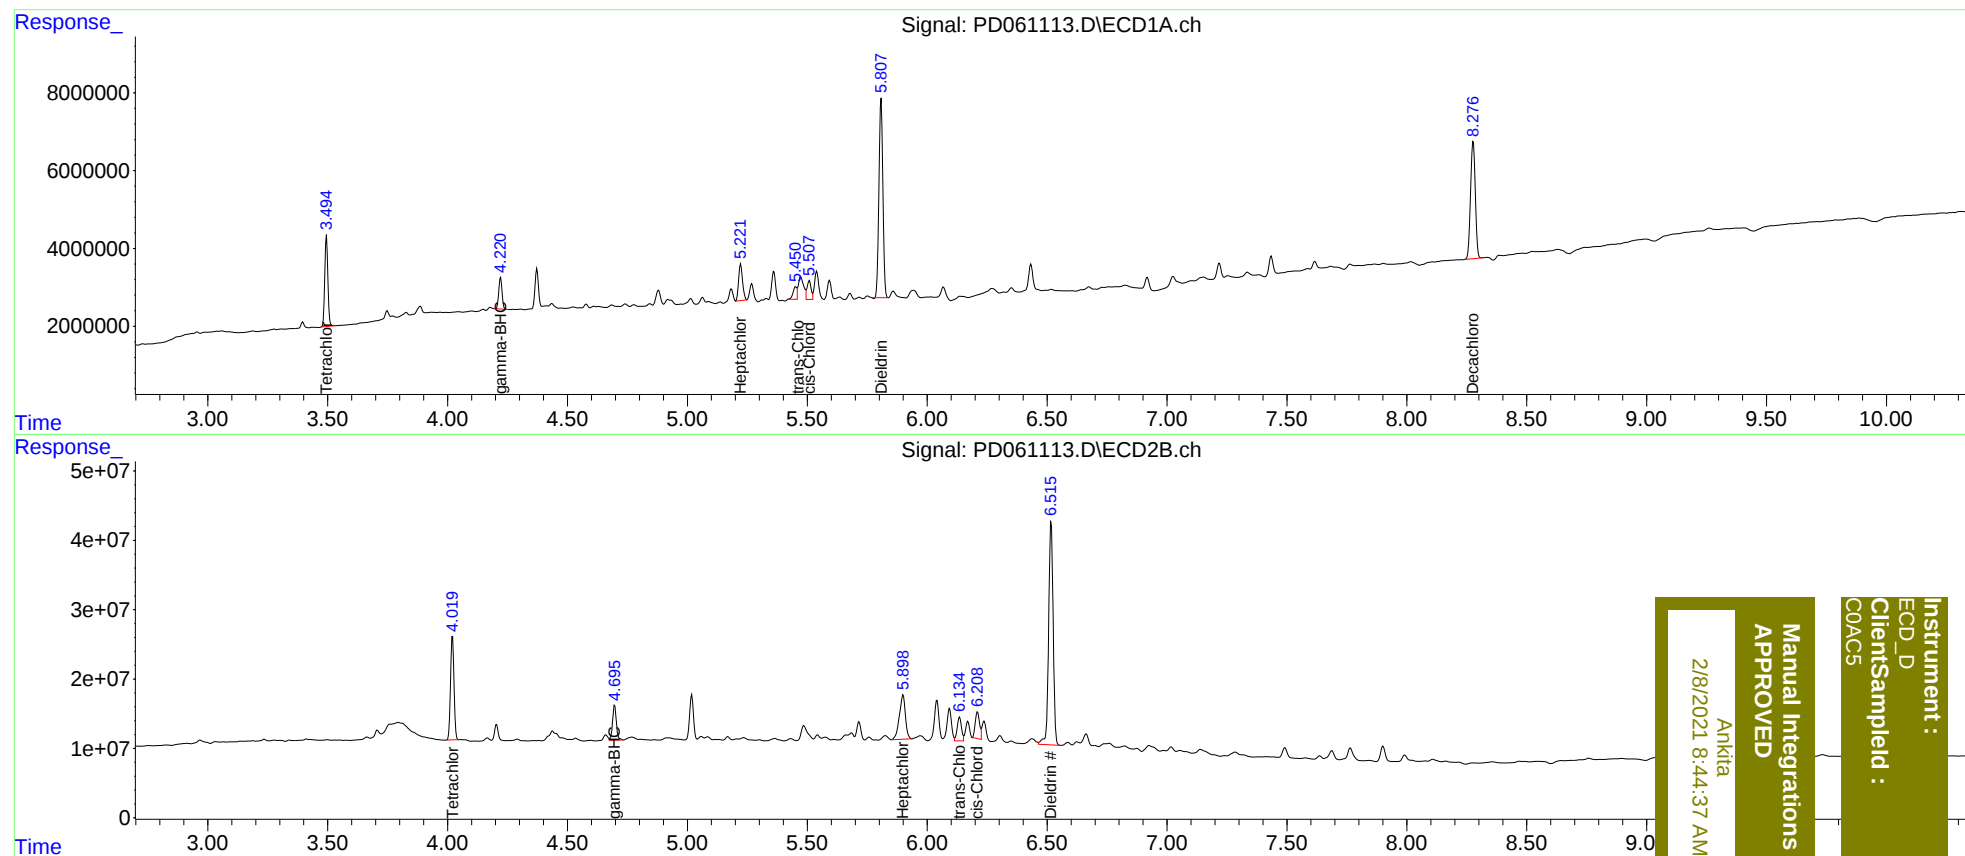

Manual Integrations
APPROVED

Ankita
2/8/2021 8:44:37 AM

Instrument :
ECD_D
ClientSampled :
C0AC5