

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020421\
 Data File : PD061115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2021 11:02
 Operator : DD\AJ
 Sample : M1274-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Ankita
 2/8/2021 8:44:40 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 00:50:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 26 00:33:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.495	4.021	21531229	151.1E6	21.213	21.109
27)	SA Decachlor...	8.277	9.105	42999322	270.8E6	34.126	39.872
Target Compounds							
8)	B Heptachlo...	5.220	5.900	7341009	64334772	5.394m	7.424 #
10)	B trans-Chl...	5.450	6.134	2717719	26459967	1.921	2.815m#
11)	B cis-Chlor...	5.508	6.210	5044645	38873664	3.676	4.376
13)	MA Dieldrin	5.808	6.517	32063711	213.0E6	21.836	22.906
15)	B Endosulfa...	6.351	6.933	1019002	5720366	0.938	0.795m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020421\
Data File : PD061115.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2021 11:02
Operator : DD\AJ
Sample : M1274-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 00:50:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jan 26 00:33:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

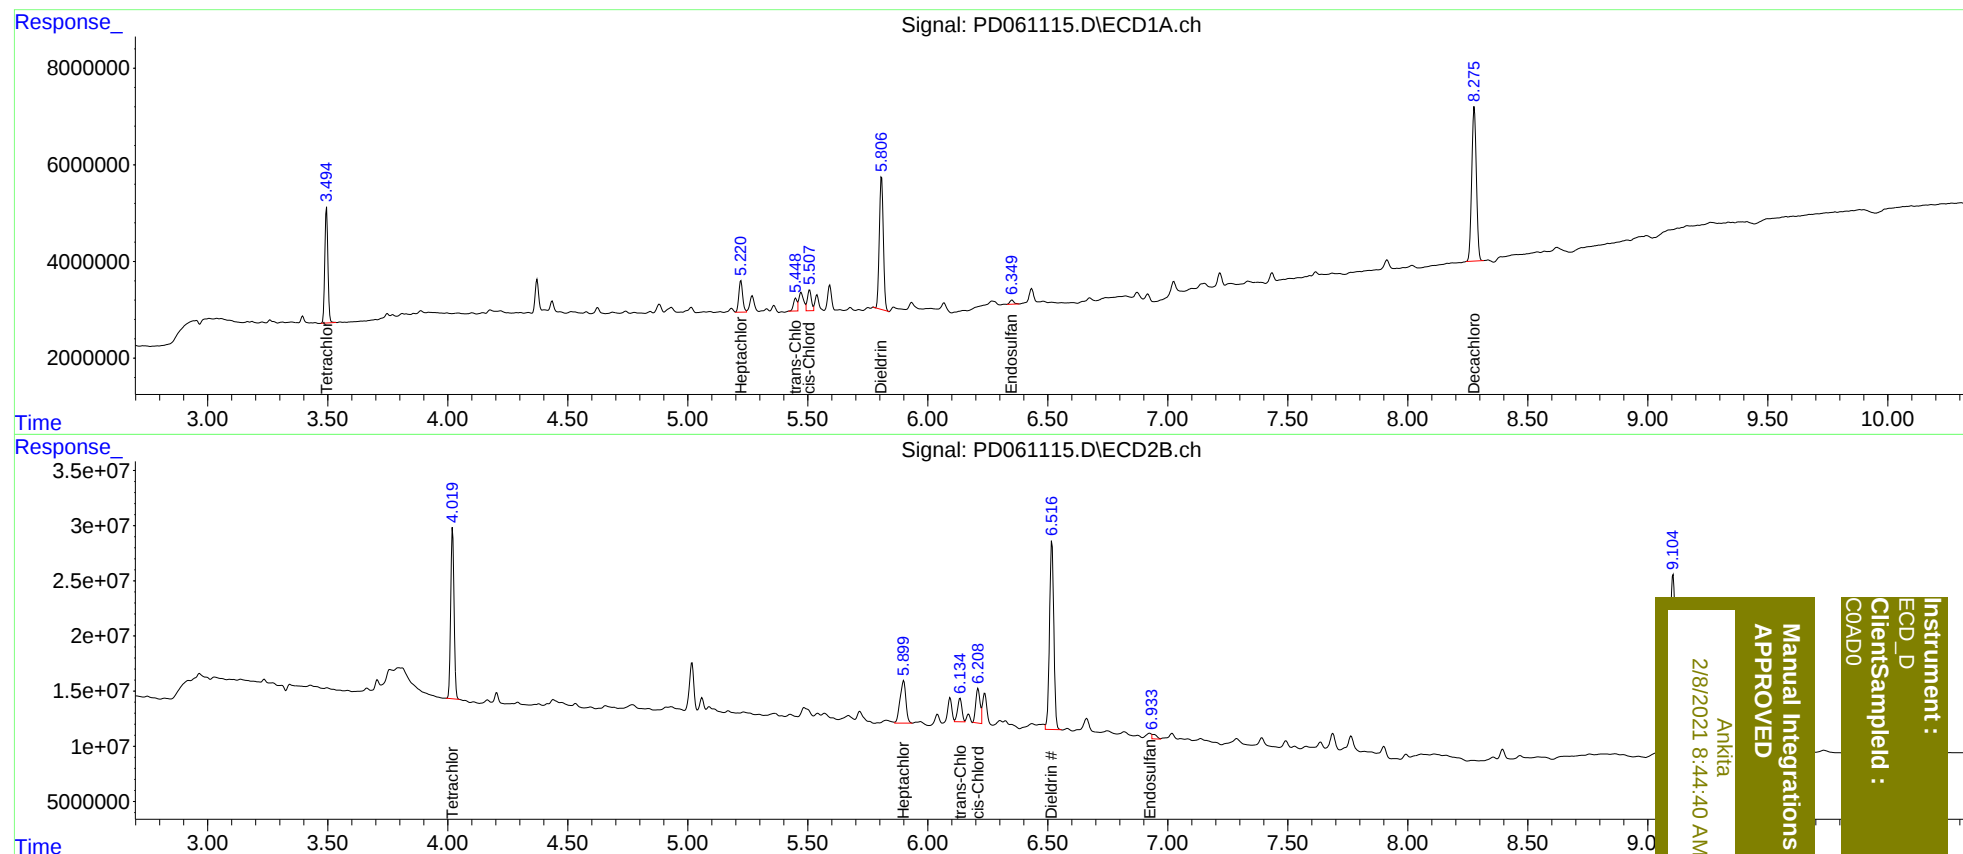

Manual Integrations
APPROVED

Ankita

2/8/2021 8:44:40 AM

Instrument :
ECD_D
ClientSampled :
C0AD0