

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020422\
 Data File : PD067934.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2022 08:49
 Operator : AR\AJ
 Sample : PIBLK220
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 00:33:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020322CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 04 02:10:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.431	3.959	44658770	188.1E6	22.081	23.971
27)	SA Decachlor...	8.152	9.012	33181676	195.0E6	36.313	39.815
Target Compounds							
2)	A alpha-BHC	3.858	4.303f	156424	253300	<MDL	<MDL #
3)	MA gamma-BHC...	0.000	4.601f	0	856.1E6	N.D.	89.996
4)	MA Heptachlor	4.405f	0.000	193236	0	<MDL	N.D. #
6)	B beta-BHC	4.405	0.000	193236	0	0.145	N.D. #
7)	B delta-BHC	0.000	4.998f	0	2111617	N.D.	0.258
8)	B Heptachlo...	5.129	0.000	28128	0	<MDL	N.D. #
9)	A Endosulfan I	5.488	0.000	106552	0	<MDL	N.D. #
10)	B trans-Chl...	5.379	0.000	18893	0	<MDL	N.D. #
11)	B cis-Chlor...	5.379	0.000	18893	0	<MDL	N.D. #
12)	B 4,4'-DDE	5.579	0.000	58120	0	<MDL	N.D. #
13)	MA Dieldrin	5.669	6.373f	30436	978220	<MDL	0.136 #
14)	MA Endrin	5.971	0.000	213368	0	<MDL	N.D. #
17)	MA 4,4'-DDT	6.325	0.000	870177	0	0.454	N.D. #
18)	B Endrin al...	6.418	0.000	27380	0	<MDL	N.D. #
20)	A Methoxychlor	6.801f	0.000	788234	0	0.897	N.D. #
22)	Toxaphene-1	5.669	6.373	30436	978220	1.906	29.167 #
24)	Toxaphene-3	6.325	0.000	870177	0	23.396	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020422\
Data File : PD067934.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2022 08:49
Operator : AR\AJ
Sample : PIBLK220
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 00:33:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020322CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 04 02:10:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

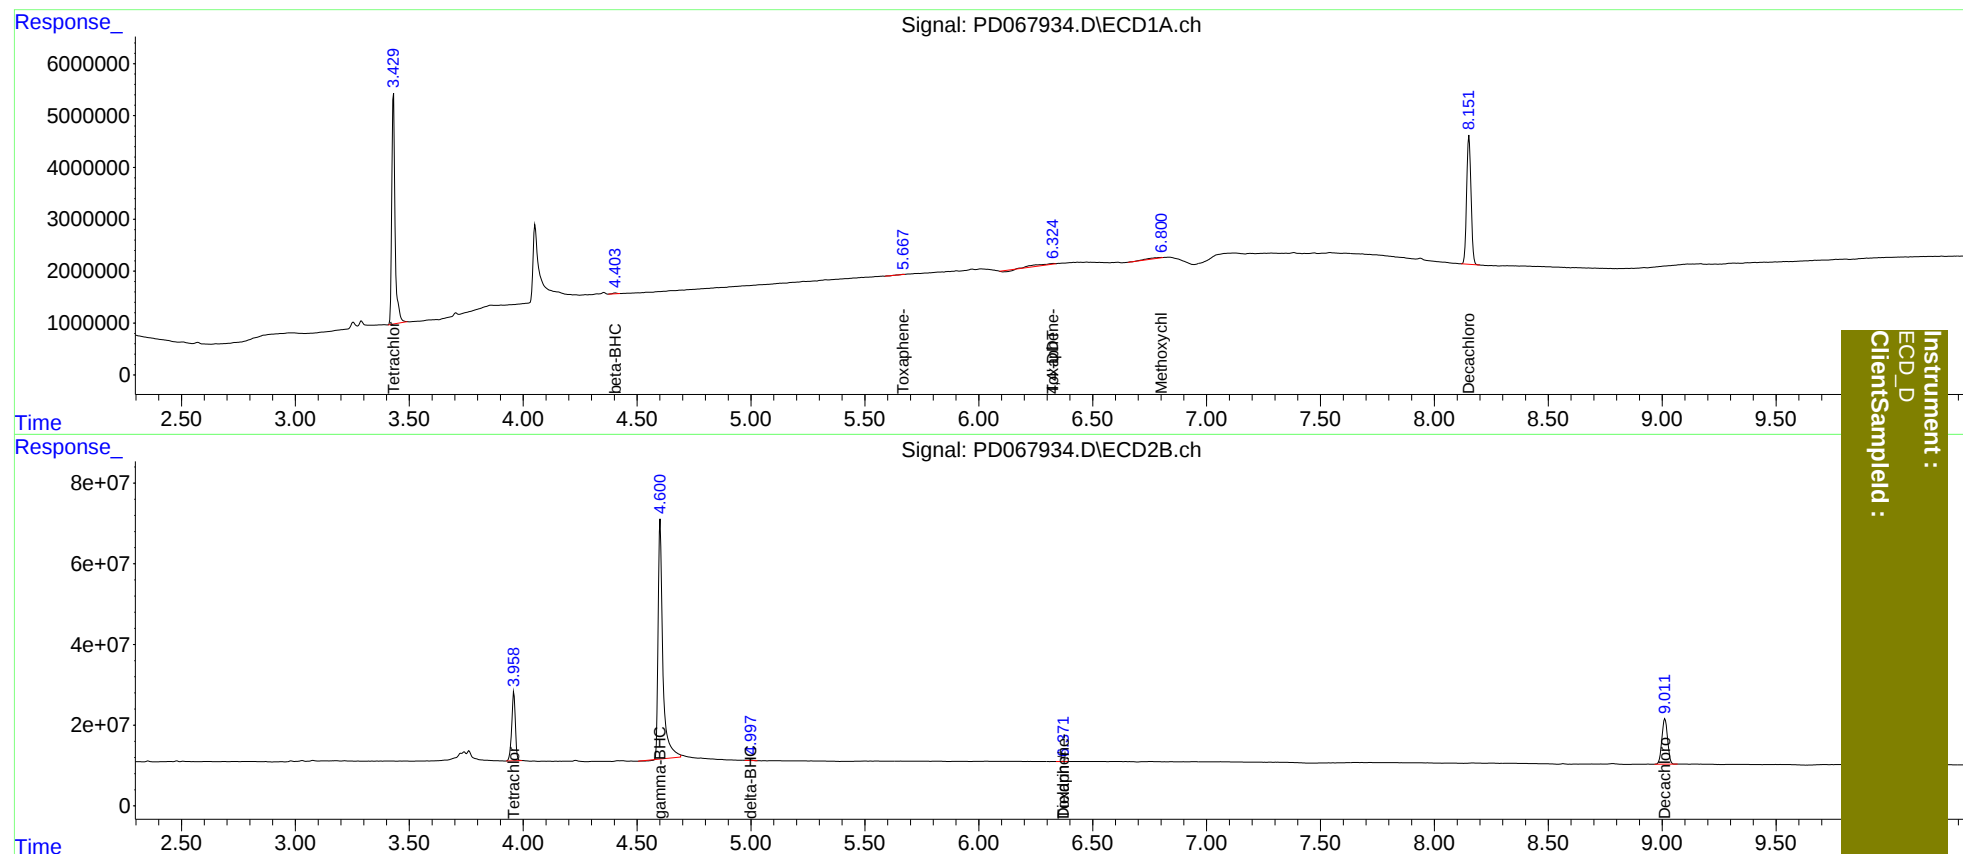


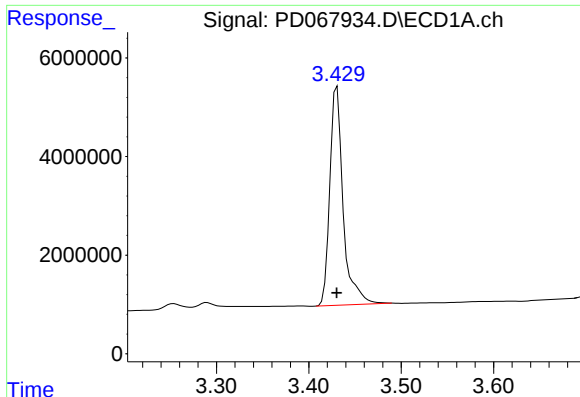

#1 Tetrachloro-m-xylene


R.T.: 3.431 min
Delta R.T.: 0.000 min
Response: 44658770
Conc: 22.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

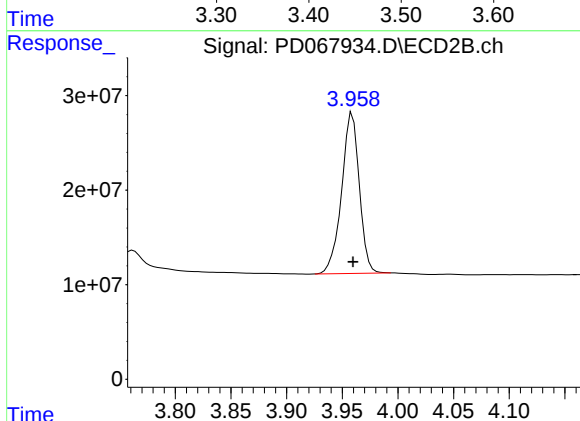


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: 0.000 min
Response: 188145892
Conc: 23.97 ng/ml

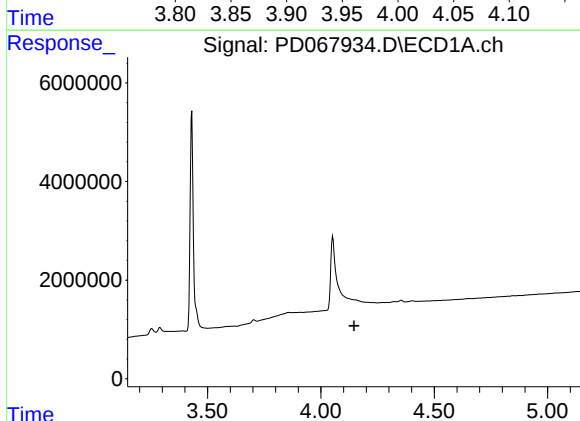


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.147 min
Response: 0
Conc: N.D.

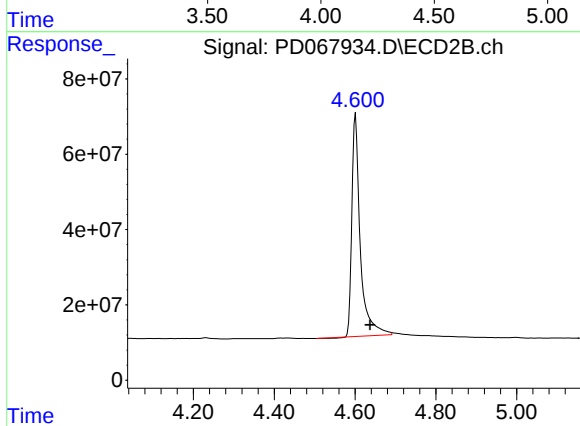

#3 gamma-BHC (Lindane)


R.T.: 4.601 min
Delta R.T.: -0.036 min
Response: 856091350
Conc: 90.00 ng/ml

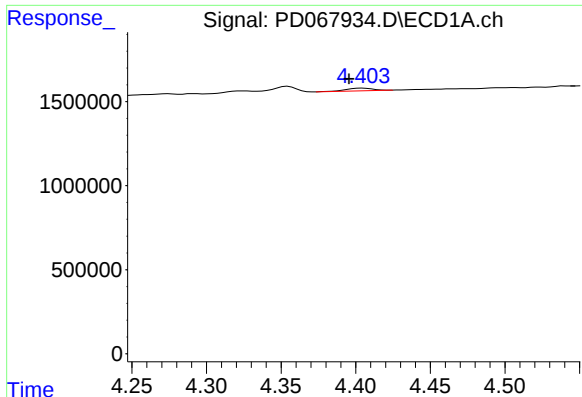

#6 beta-BHC


R.T.: 4.405 min
Delta R.T.: 0.009 min
Response: 193236
Conc: 0.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

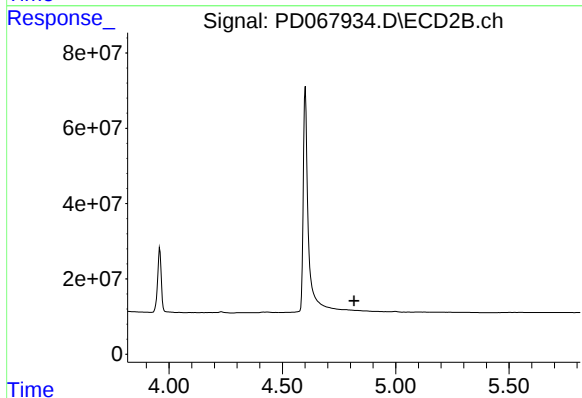


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.816 min
Response: 0
Conc: N.D.

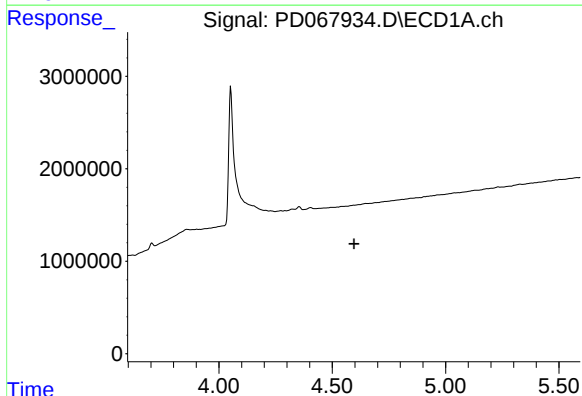


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.597 min
Response: 0
Conc: N.D.

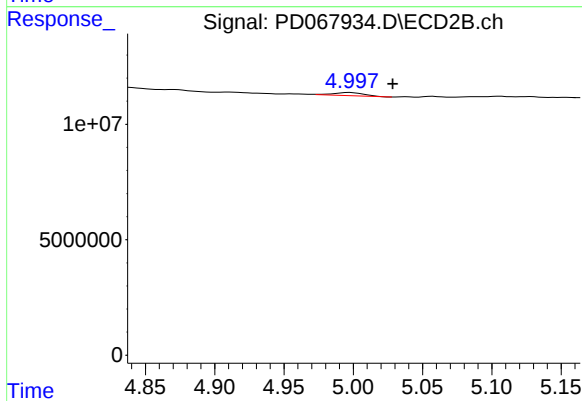

#7 delta-BHC


R.T.: 4.998 min
Delta R.T.: -0.031 min
Response: 2111617
Conc: 0.26 ng/ml

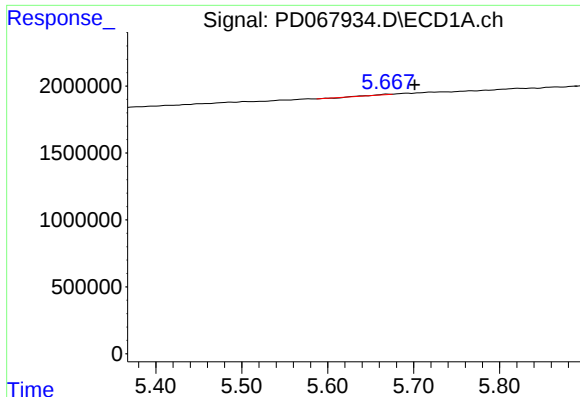

#13 Dieldrin


R.T.: 5.669 min
Delta R.T.: -0.032 min
Response: 30436
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

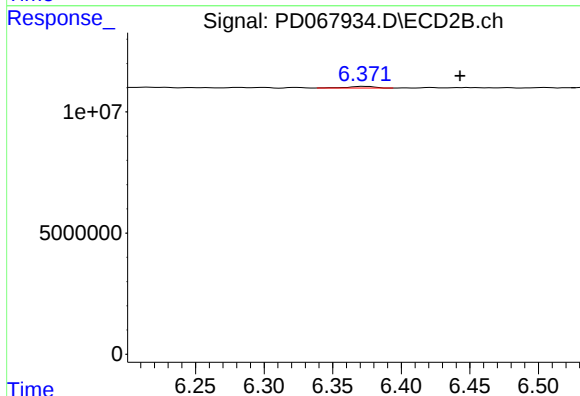


#13 Dieldrin

R.T.: 6.373 min
Delta R.T.: -0.070 min
Response: 978220
Conc: 0.14 ng/ml

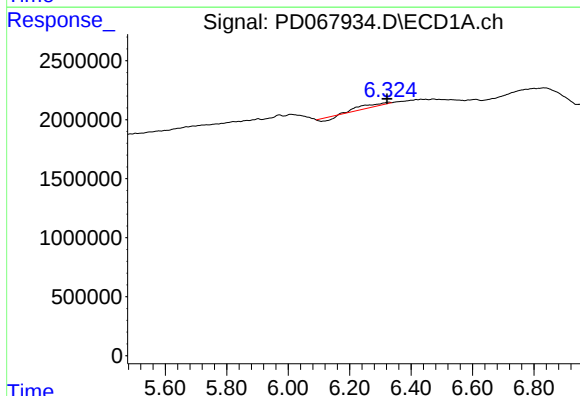


#17 4,4'-DDT

R.T.: 6.325 min
Delta R.T.: 0.004 min
Response: 870177
Conc: 0.45 ng/ml

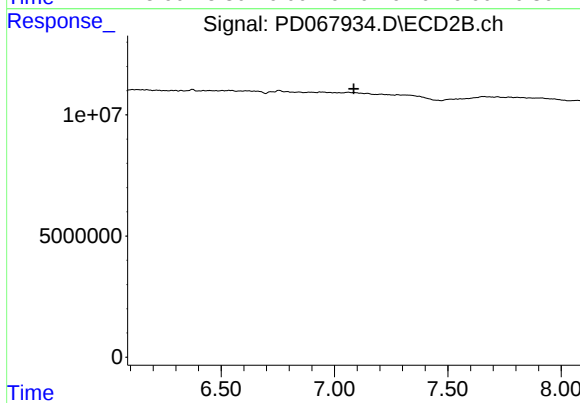

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.085 min
Response: 0
Conc: N.D.

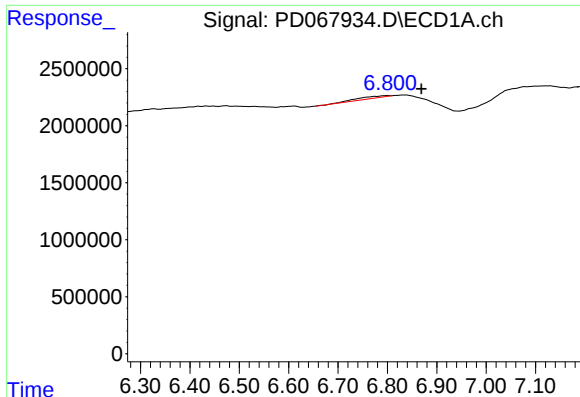

#20 Methoxychlor


R.T.: 6.801 min
Delta R.T.: -0.067 min
Response: 788234
Conc: 0.90 ng/ml

Instrument :
ECD_D
ClientSampleId :

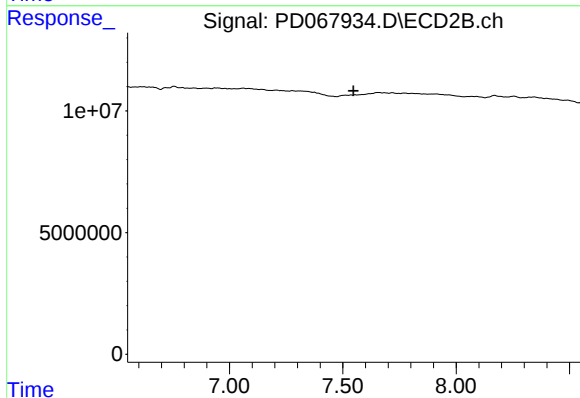


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.547 min
Response: 0
Conc: N.D.

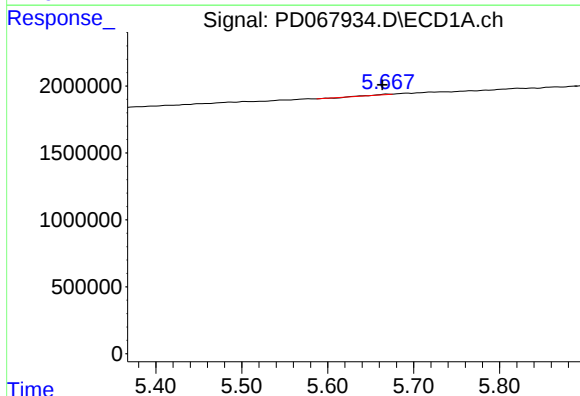


#22 Toxaphene-1

R.T.: 5.669 min
Delta R.T.: 0.006 min
Response: 30436
Conc: 1.91 ng/ml

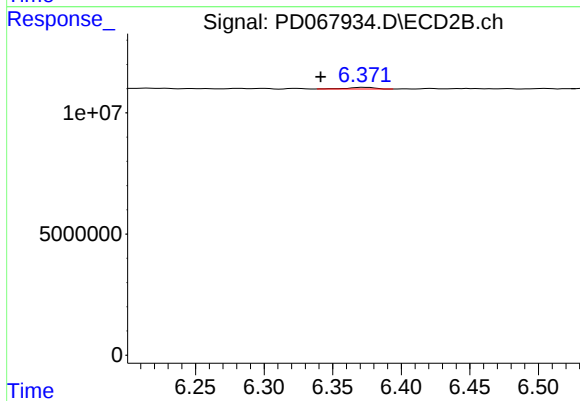

#22 Toxaphene-1


R.T.: 6.373 min
Delta R.T.: 0.032 min
Response: 978220
Conc: 29.17 ng/ml

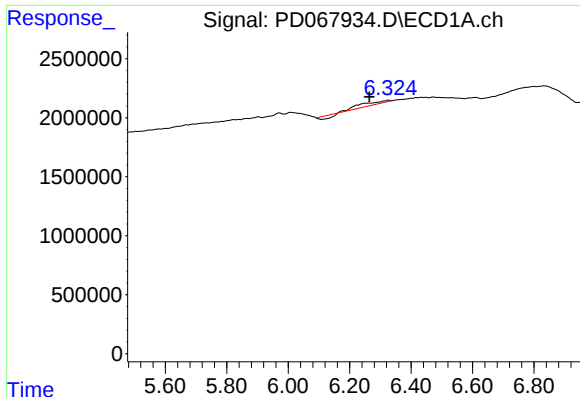

#24 Toxaphene-3


R.T.: 6.325 min
Delta R.T.: 0.061 min
Response: 870177
Conc: 23.40 ng/ml

Instrument :
ECD_D
ClientSampleId :

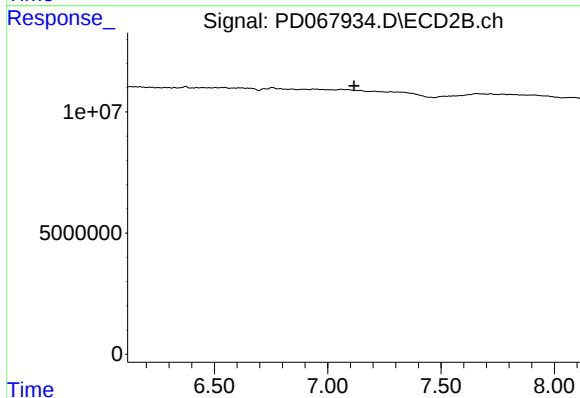


#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

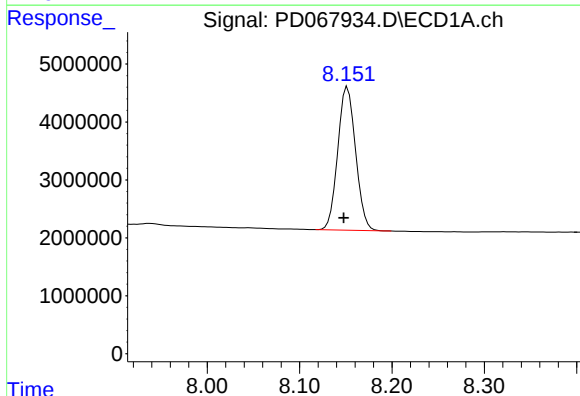

#27 Decachlorobiphenyl

R.T.: 8.152 min
Delta R.T.: 0.004 min
Response: 33181676
Conc: 36.31 ng/ml

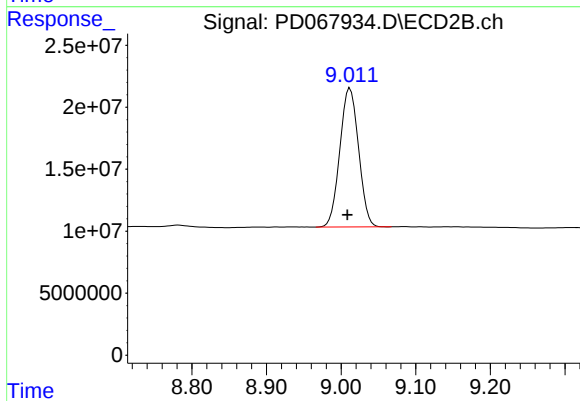

#27 Decachlorobiphenyl

R.T.: 9.012 min
Delta R.T.: 0.004 min
Response: 194997821
Conc: 39.82 ng/ml