

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020422\
 Data File : PD067944.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2022 15:00
 Operator : AR\AJ
 Sample : N1307-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0Q48

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/07/2022
 Supervised By :Ankita Jodhani 02/08/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 02:04:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020322CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 04 02:10:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.449	3.943	7229.5E6	24276.8E6	3574.502	3092.960m
2) SA Decachlor...	8.150	9.012	26379704	148.2E6	28.869	30.261
Target Compounds						
13) MA Dieldrin	5.703	6.444	11161013	29555626	4.199	4.118
17) MA 4,4'-DDT	6.328	7.075	14069535	7889566	7.347m	1.371 #
21) B Endrin ke...	7.105	7.675	2920767	31273524	1.545m	4.677 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020422\
Data File : PD067944.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2022 15:00
Operator : AR\AJ
Sample : N1307-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 02:04:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020322CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 04 02:10:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

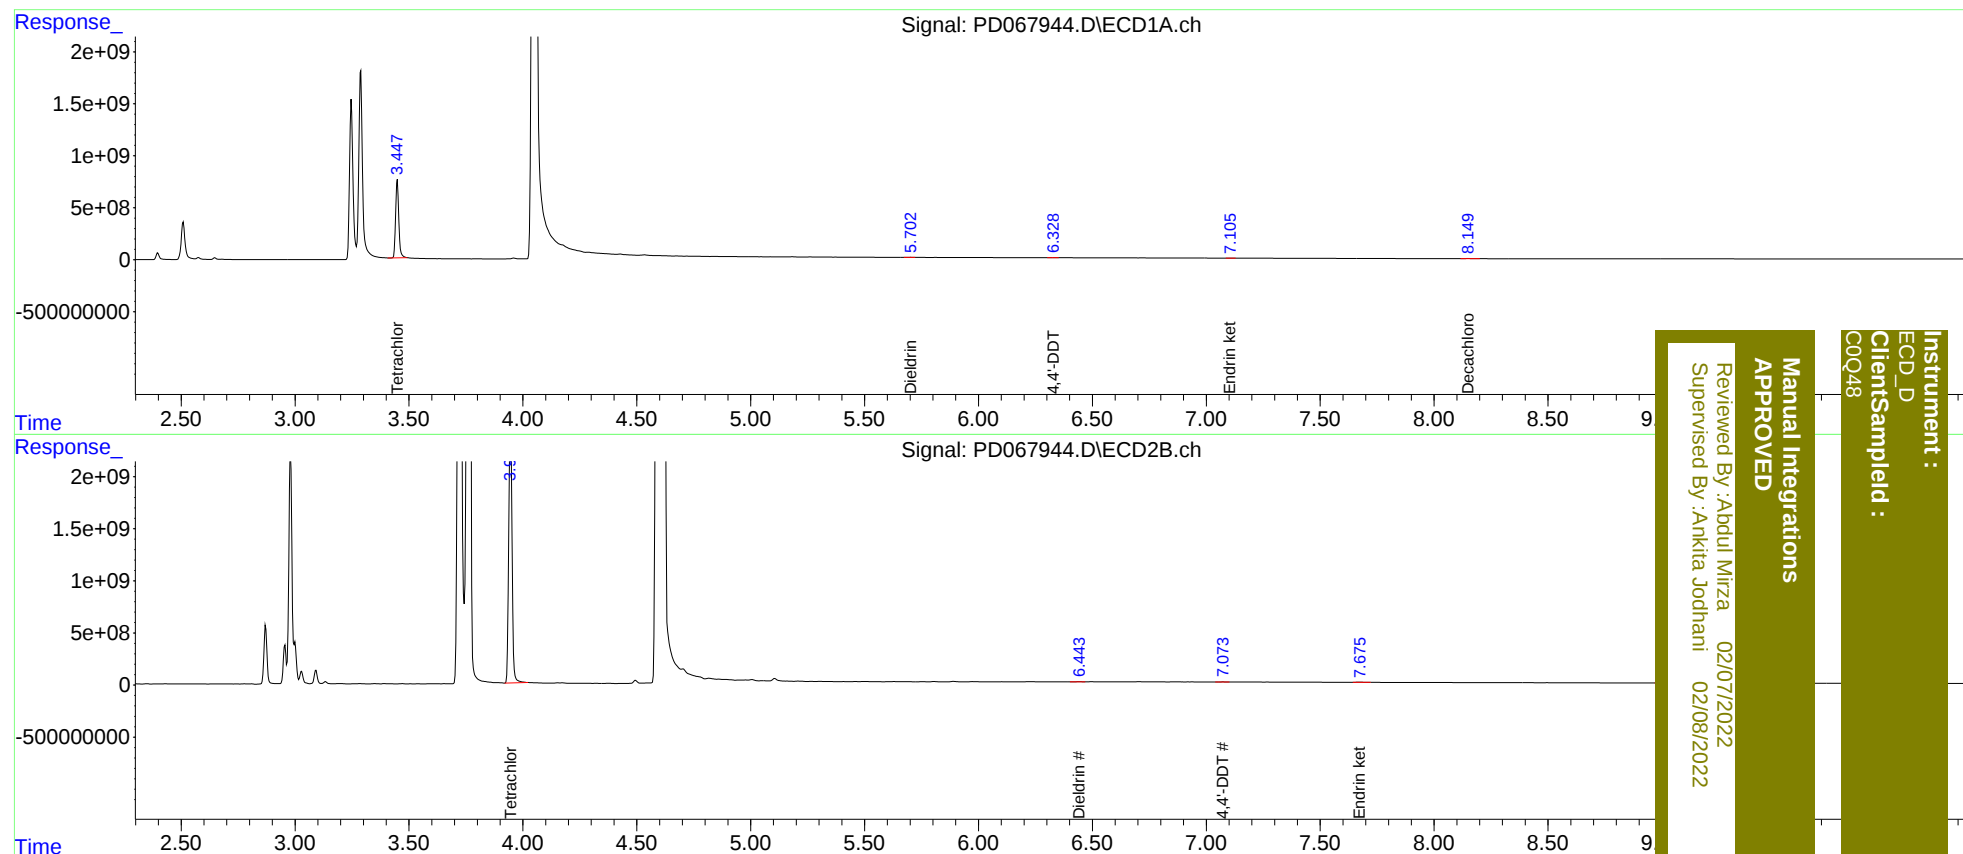

Reviewed By: Abdul Mirza 02/07/2022
Supervised By: Ankita Jodhani 02/08/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
C0048