

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020422\
 Data File : PD067940.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2022 13:55
 Operator : AR\AJ
 Sample : N1307-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0Q50

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/07/2022
 Supervised By : Ankita Jodhani 02/08/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 01:14:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020322CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 04 02:10:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.450	3.940	11703.5E6	31642.9E6	5786.596m	4031.441m#
27)	SA Decachlor...	8.152	9.014	24634695	153.4E6	26.960m	31.318
Target Compounds							
7)	B delta-BHC	4.601	5.008	47182579	682.3E6	16.767m	83.426m#
8)	B Heptachlo...	5.122	5.804	8927494	78187738	3.349m	11.522m#
10)	B trans-Chl...	5.345	6.064	2937849	10030026	1.080m	1.376m#
13)	MA Dieldrin	5.707	6.445	8699820	22441618	3.273	3.127

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020422\
Data File : PD067940.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2022 13:55
Operator : AR\AJ
Sample : N1307-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 01:14:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020322CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 04 02:10:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

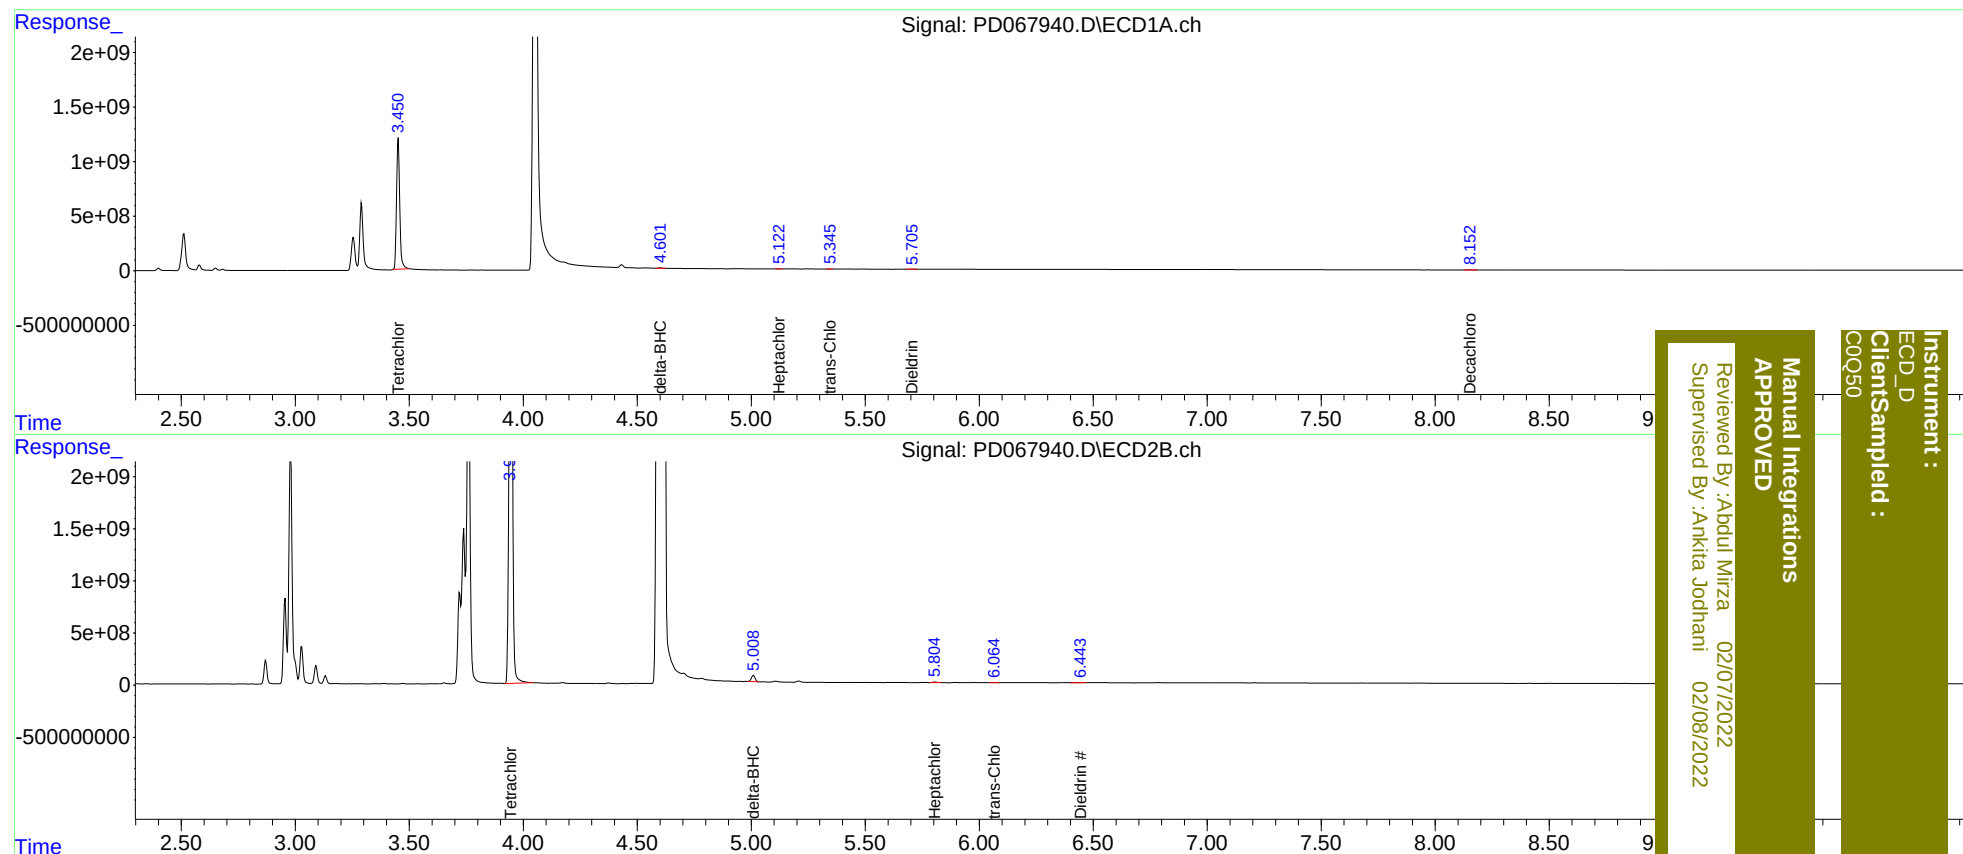

Instrument :
ECD_D
ClientSampled :
C0050

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/07/2022
Supervised By :Ankita Jodhani 02/08/2022