

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020422\
 Data File : PD067946.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2022 15:29
 Operator : AR\AJ
 Sample : N1307-15MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0Q05MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/07/2022
 Supervised By : Ankita Jodhani 02/08/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 00:36:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020322CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 04 02:10:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.449	3.945	4571.6E6	17365.8E6	2260.332	2212.475m
27)	SA Decachlor...	8.151	9.013	24407631	134.9E6	26.711	27.542
Target Compounds							
2)	A alpha-BHC	3.867	4.352	147.8E6	393.0E6	49.551	39.218m
3)	MA gamma-BHC...	4.147	4.631	99713911	1700.8E6	34.640m	178.790m#
4)	MA Heptachlor	4.434	5.136	308.2E6	383.3E6	104.990	44.981m#
5)	MB Aldrin	4.685	5.439	149.5E6	340.5E6	50.780	41.583m
6)	B beta-BHC	4.395	4.815	46782395	139.8E6	35.137m	31.055m
7)	B delta-BHC	4.597	5.030	101.6E6	142.2E6	36.107m	17.383 #
8)	B Heptachlo...	5.125	5.828	145.7E6	307.1E6	54.674	45.251m
9)	A Endosulfan I	5.462	6.187	122.0E6	284.2E6	49.698	40.800
10)	B trans-Chl...	5.349	6.064	135.2E6	312.7E6	49.698	42.907
11)	B cis-Chlor...	5.407	6.135	122.9E6	288.6E6	45.642	39.464
12)	B 4,4'-DDE	5.571	6.296	261.1E6	605.0E6	106.787	89.246
13)	MA Dieldrin	5.703	6.445	257.9E6	612.0E6	97.025	85.271
14)	MA Endrin	5.960	6.664	237.3E6	586.7E6	110.207	98.558
15)	B Endosulfa...	6.233	6.879	220.2E6	529.5E6	103.475	85.762
16)	A 4,4'-DDD	6.085	6.791	199.4E6	532.9E6	101.192	92.058
17)	MA 4,4'-DDT	6.324	7.087	214.9E6	515.6E6	112.190	89.570
18)	B Endrin al...	6.402	7.003	159.0E6	434.6E6	101.903	90.560
19)	B Endosulfa...	6.614	7.226	153.1E6	473.9E6	84.663	80.657
20)	A Methoxychlor	6.872	7.551	421.4E6	1224.7E6	479.842	437.648
21)	B Endrin ke...	7.105	7.699	191.7E6	723.2E6	101.408	108.141

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020422\
Data File : PD067946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2022 15:29
Operator : AR\AJ
Sample : N1307-15MS
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 00:36:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD020322CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 04 02:10:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

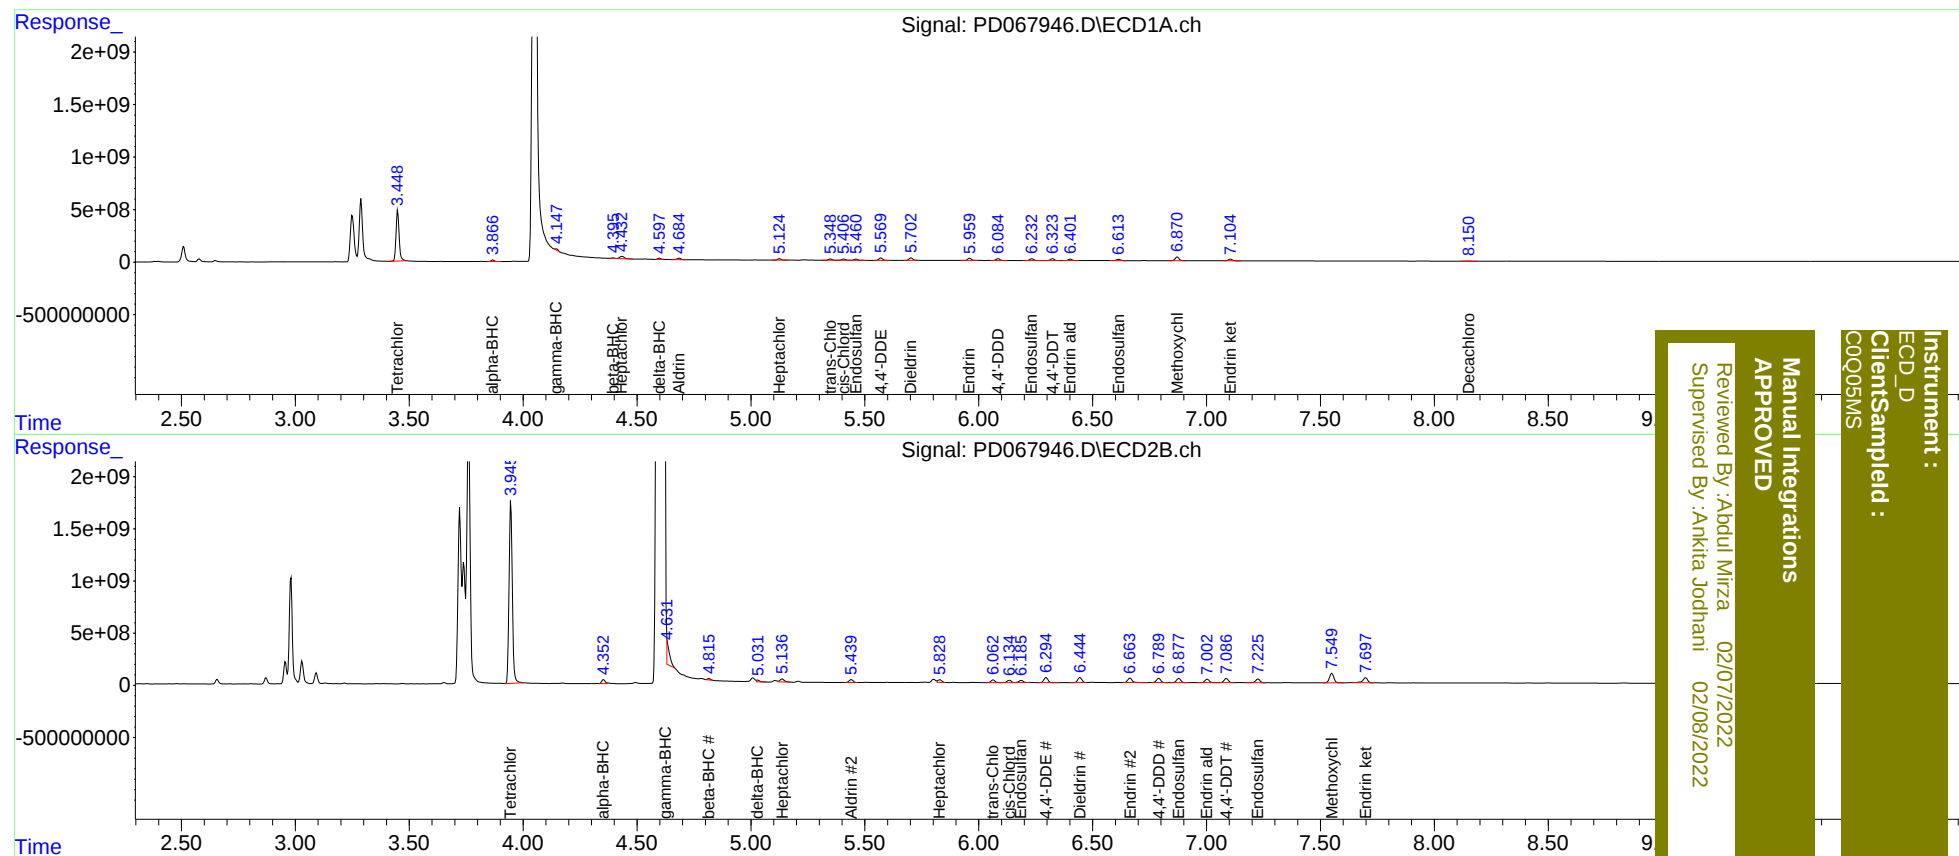

Reviewed By: Abdul Mirza 02/07/2022
Supervised By: Ankita Jodhani 02/08/2022


Manual Integrations
APPROVED

Instrument :
ECD_D
Client/Sampled :
C0005MS

File :Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020422\PD067946.D
Operator : AR\AJ
Acquired : 04 Feb 2022 15:29 using AcqMethod ECD_D.M
Instrument : ECD_D
Sample Name: N1307-15MS
Misc Info :
Vial Number: 14

Instrument :
ECD_D
ClientSampleId :
C0Q05MS

Manual Integrations
APPROVED
Reviewed By :Abdul Mirza 02/07/2022
Supervised By :Ankita Jodhani 02/08/2022

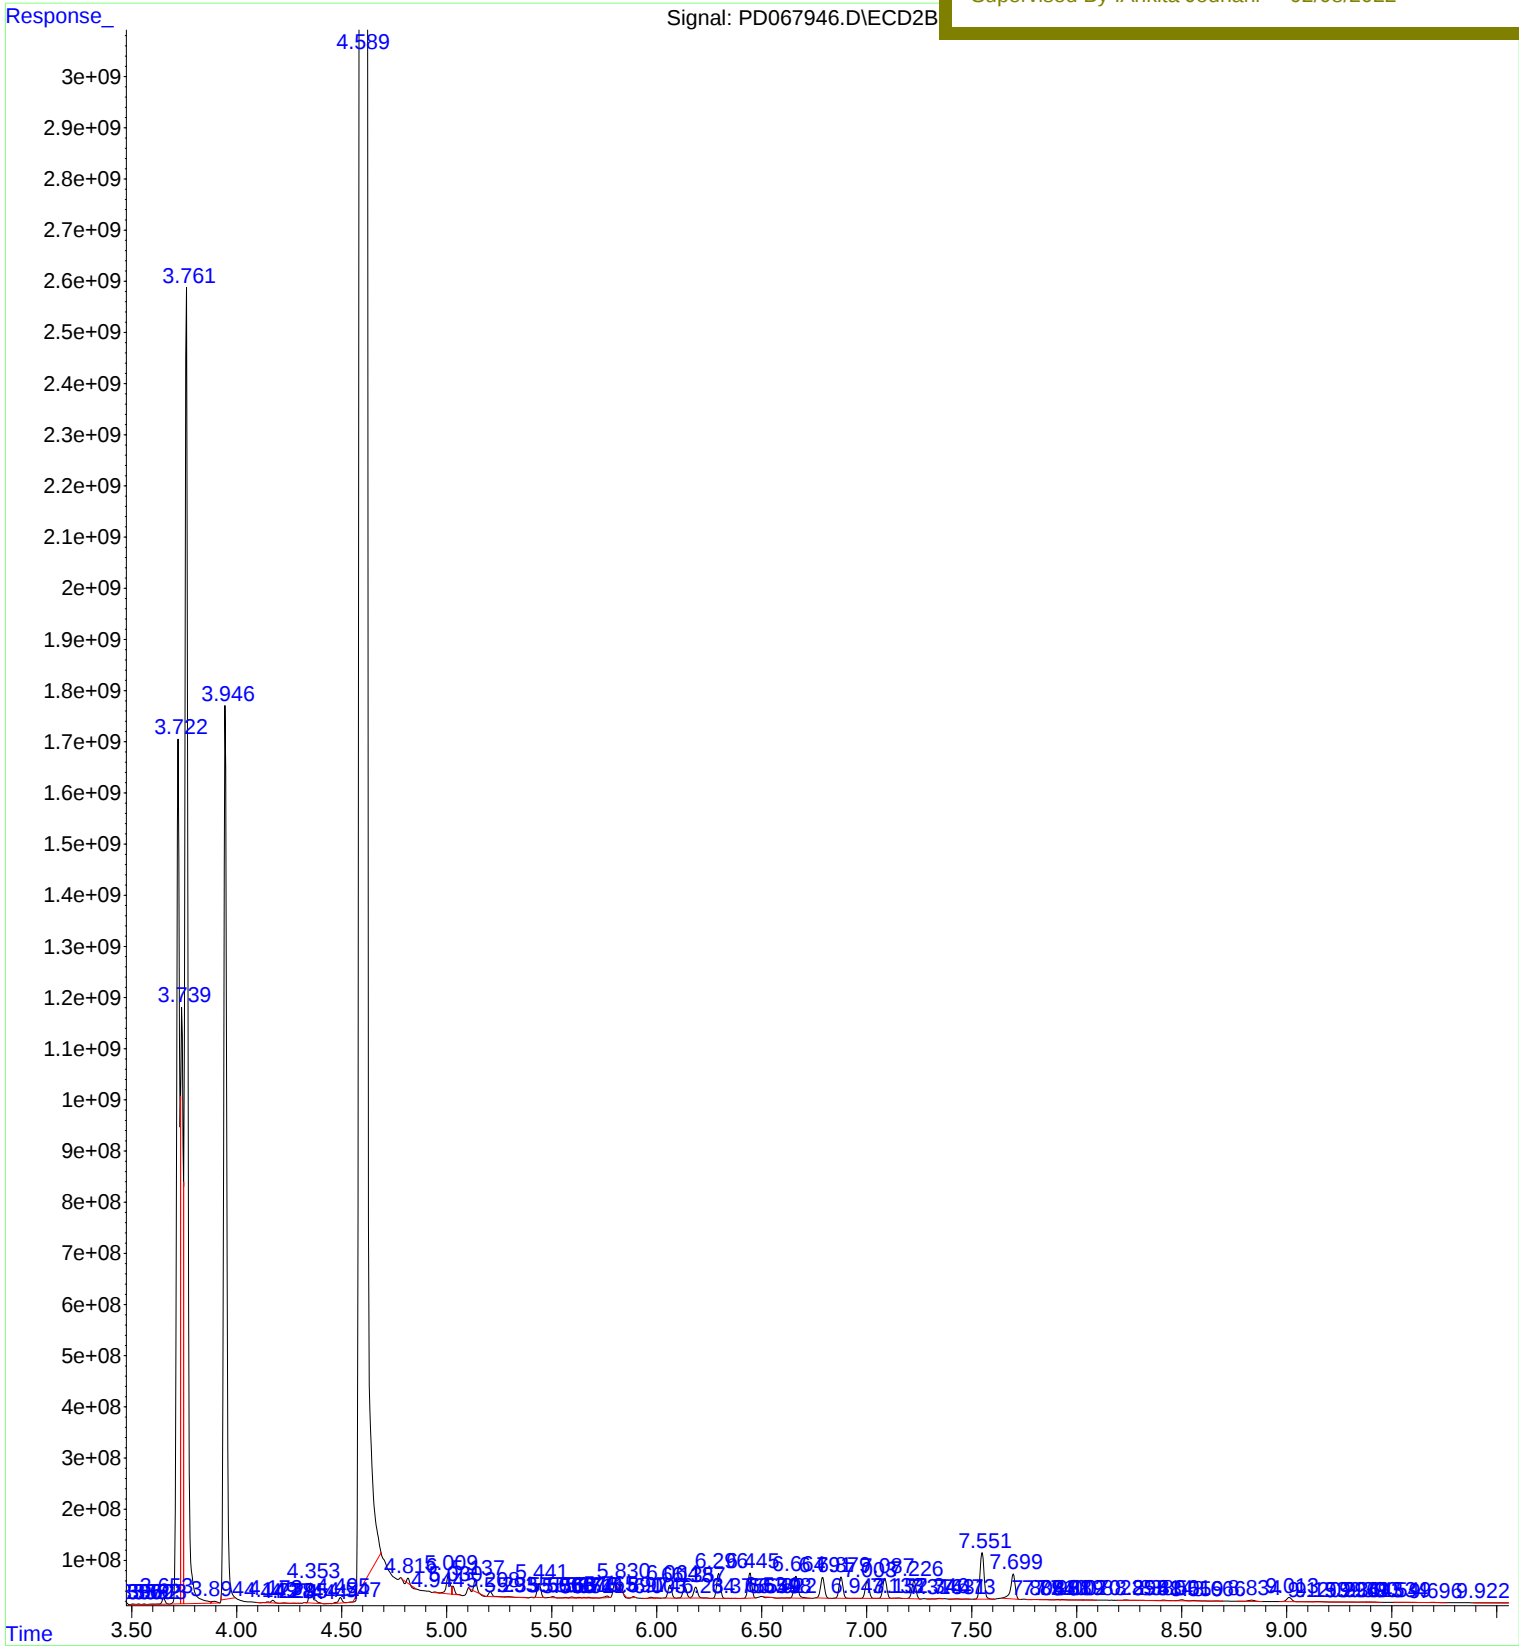

File : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020422\PD067946.D
Operator : AR\AJ
Acquired : 04 Feb 2022 15:29 using AcqMethod ECD_D.M
Instrument : ECD_D
Sample Name: N1307-15MS
Misc Info :
Vial Number: 14

Instrument :
ECD_D
ClientSampleId :
C0Q05MS

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/07/2022
Supervised By : Ankita Jodhani 02/08/2022

