

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020425\
 Data File : PD087709.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2025 15:32
 Operator : AR\AJ
 Sample : Q1226-08DL 2X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCZP0DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/05/2025
 Supervised By : Ankita Jodhani 02/05/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 08:04:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 16 13:39:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.553	2.881	24935903	118.0E6	12.236m	9.540m
2) SA Decachlor...	9.084	8.081	36352620	167.6E6	10.873	11.574
Target Compounds						
2) A alpha-BHC	4.005	3.396	29317483	174.2E6	7.057	8.798
3) MA gamma-BHC...	4.326	3.733	15767122	30273832	3.920m	1.653 #
6) B beta-BHC	4.520	4.029	6489696	35115156	3.613	4.116
7) B delta-BHC	4.769	4.266	346.5E6	1427.3E6	83.861	76.475

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020425\
Data File : PD087709.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2025 15:32
Operator : AR\AJ
Sample : Q1226-08DL 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 08:04:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 16 13:39:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

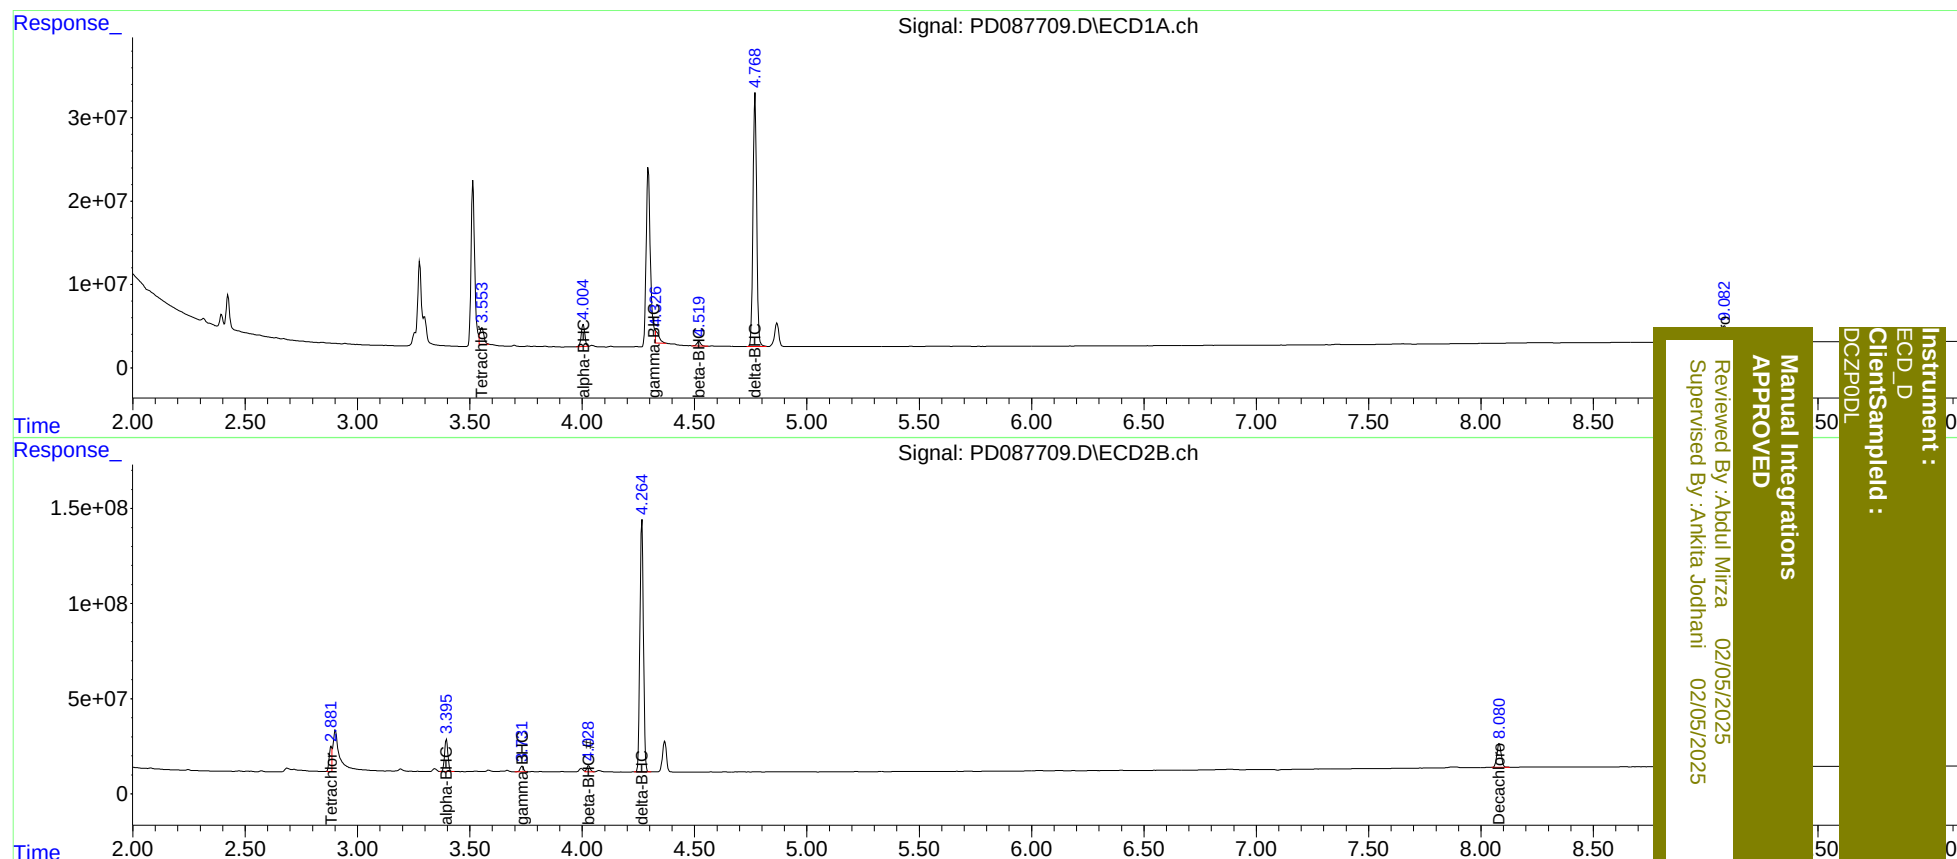

Instrument :
ECD_D
ClientSampled :
DCZP0DL

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/05/2025
Supervised By : Ankita Jodhani 02/05/2025