Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020425\
Data File : PD087702.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2025 13:43
Operator : AR\AJ
Sample : Q1226-24
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
DCZN2

Manual Integrations APPROVED

Reviewed By :Abdul Mirza 02/05/2025
Supervised By :Ankita Jodhani 02/05/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 08:02:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 16 13:39:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
	System Monitoring Compounds						
1) SA	Tetrachlo...	3.554	2.882	37392469	260.3E6	18.348m	21.045
27) SA	Decachlor...	9.085	8.082	52984576	238.5E6	15.848	16.466
	Target Compounds						
2) A	alpha-BHC	4.005	3.395	10974465	57027120	2.642	2.880
6) B	beta-BHC	4.518	4.028	2509826	4207779	1.397	0.493 #
7) B	delta-BHC	4.770	4.265	16531421	84557365	4.000	4.531m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020425\
Data File : PD087702.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2025 13:43
Operator : AR\AJ
Sample : Q1226-24
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 08:02:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 16 13:39:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

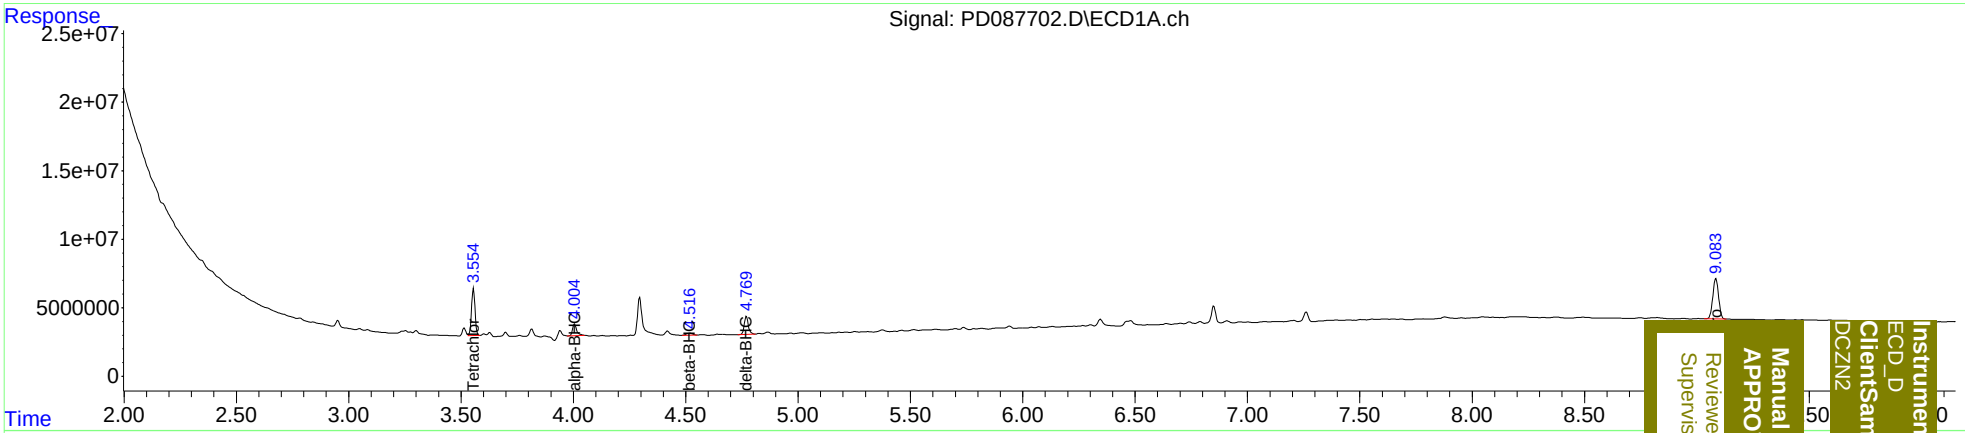

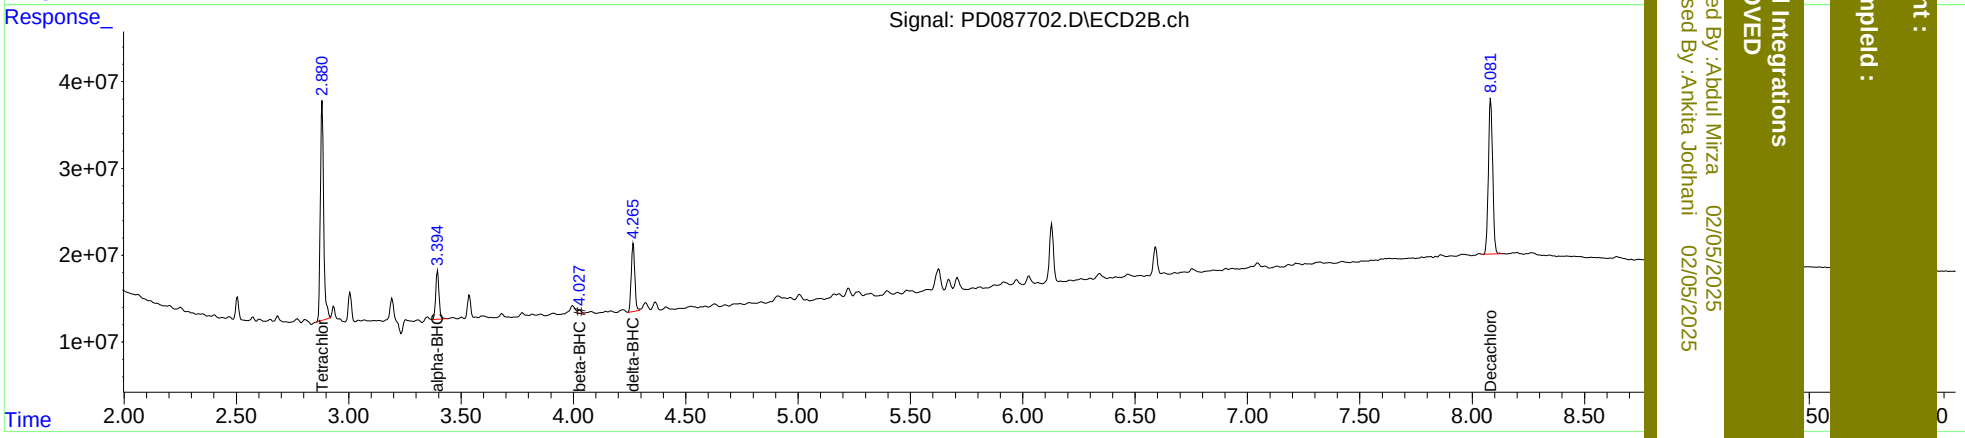

Manual Integrations APPROVED
Reviewed By :Abdul Mirza 02/05/2025
Supervised By :Ankita Jodhani 02/05/2025

Instrument : ECD_D
ClientSampleId : DCZN2