

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020425\
 Data File : PD087726.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2025 19:51
 Operator : AR\AJ
 Sample : Q1229-11
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E29B5

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/07/2025
 Supervised By : Ankita Jodhani 02/11/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 08:19:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 16 13:39:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.553	2.879	28831333	219.6E6	14.147m	17.752m#
27)	SA Decachlor...	9.082	8.081	24225633	101.6E6	7.246	7.013
Target Compounds							
4)	MA Heptachlor	4.919	4.089	97238716	137.0E6	23.789m	7.342m#
10)	B trans-Chl...	5.951	5.154	16676650	45313663	4.527m	2.521m#
14)	MA Endrin	6.577	5.800	7818012	41736133	2.409m	2.793m
20)	A Methoxychlor	7.512	6.757	6938015	111.8E6	4.379m	18.157m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020425\
Data File : PD087726.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2025 19:51
Operator : AR\AJ
Sample : Q1229-11
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 08:19:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 16 13:39:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

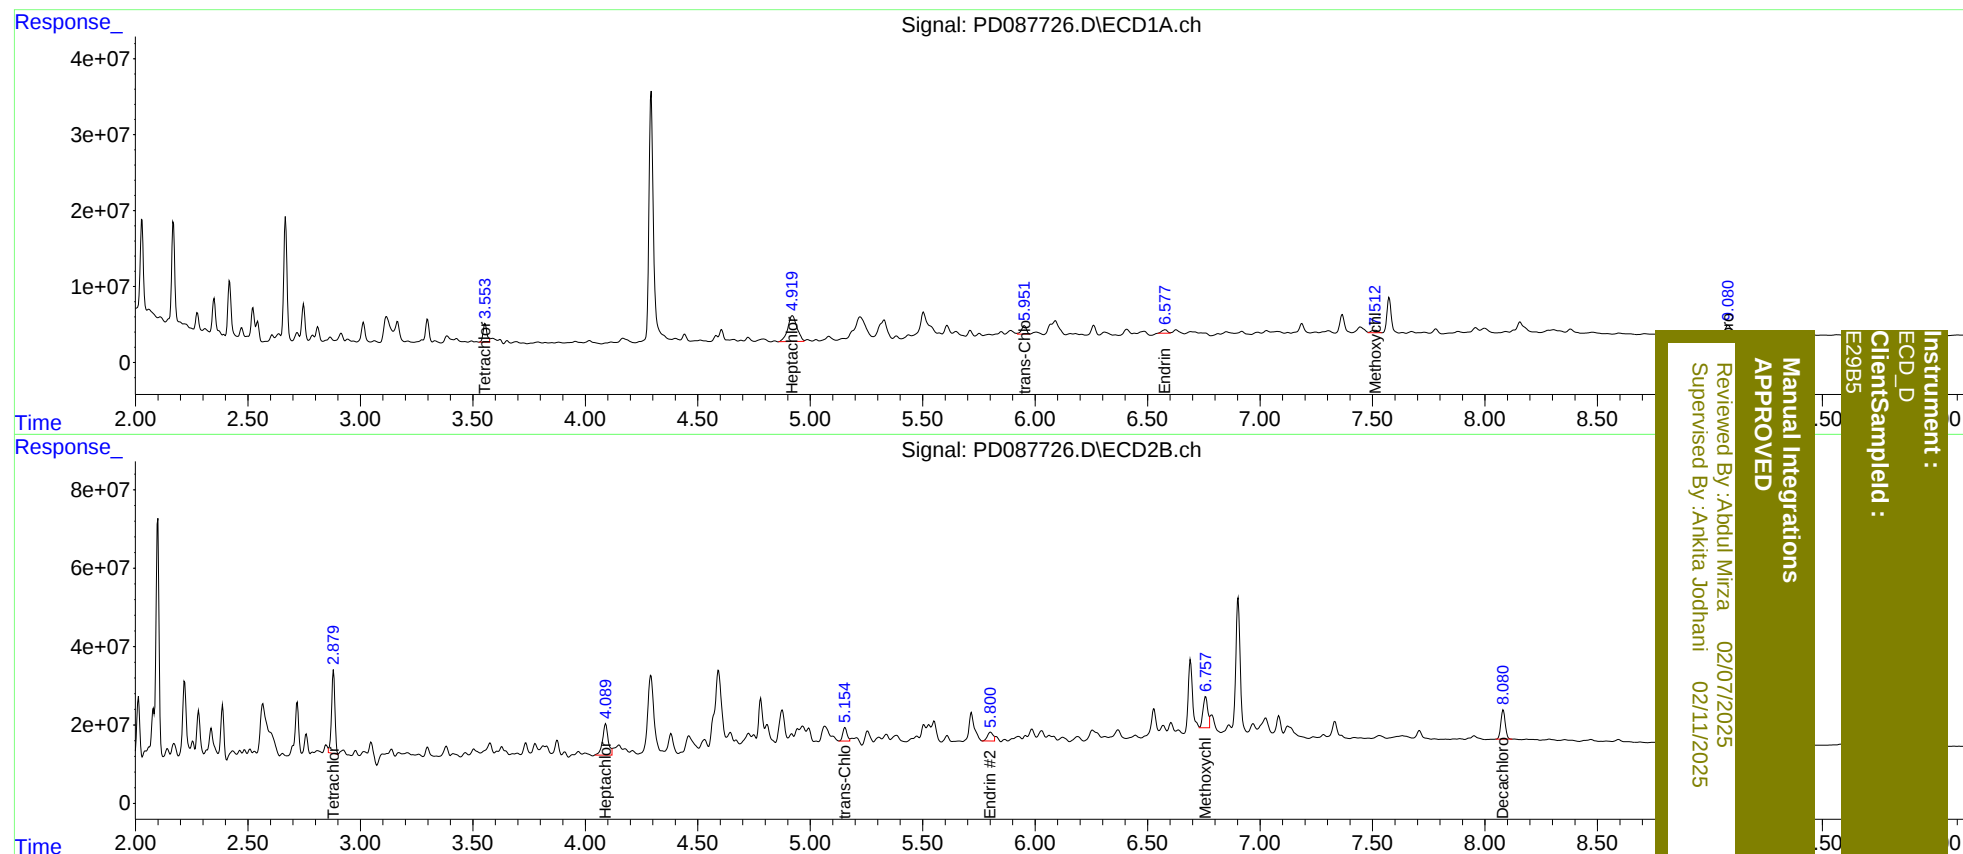

Instrument :
ECD_D
ClientSampled :
E29B5

Manual Integrations
APPROVED

Reviewed By : Abdul Miza 02/07/2025
Supervised By : Ankita Jodhani 02/11/2025