

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD020525\  
 Data File : PD087746.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 05 Feb 2025 15:23  
 Operator : AR\AJ  
 Sample : INDA311  
 Misc :  
 ALS Vial : 99 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 INDA3225

Manual Integrations  
 APPROVED

Reviewed By : Abdul Mirza 02/06/2025  
 Supervised By : Ankita Jodhani 02/06/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Feb 06 07:54:03 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD011625CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Jan 16 13:39:07 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm


|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml   | ng/ml   |
|-----------------------------|-----------------|-------|-------|----------|----------|---------|---------|
| -----                       |                 |       |       |          |          |         |         |
| System Monitoring Compounds |                 |       |       |          |          |         |         |
| 1)                          | SA Tetrachlo... | 3.555 | 2.882 | 41208424 | 264.9E6  | 20.220  | 21.417  |
| 27)                         | SA Decachlor... | 9.082 | 8.080 | 119.8E6  | 545.0E6  | 35.839  | 37.628  |
| Target Compounds            |                 |       |       |          |          |         |         |
| 2)                          | A alpha-BHC     | 4.004 | 3.395 | 81596635 | 414.6E6  | 19.641  | 20.940  |
| 3)                          | MA gamma-BHC... | 4.334 | 3.732 | 78892888 | 379.5E6  | 19.612m | 20.716  |
| 4)                          | MA Heptachlor   | 4.936 | 4.086 | 76528720 | 377.3E6  | 18.722  | 20.213  |
| 9)                          | A Endosulfan I  | 6.080 | 5.251 | 63687439 | 319.1E6  | 18.280  | 20.105  |
| 13)                         | MA Dieldrin     | 6.353 | 5.517 | 138.6E6  | 676.2E6  | 36.355  | 40.513  |
| 14)                         | MA Endrin       | 6.580 | 5.794 | 108.8E6  | 587.3E6  | 33.507  | 39.305  |
| 16)                         | A 4,4'-DDD      | 6.711 | 5.935 | 98994059 | 551.2E6  | 36.005  | 41.226  |
| 17)                         | MA 4,4'-DDT     | 7.027 | 6.189 | 92580065 | 506.6E6  | 31.944  | 36.761  |
| 20)                         | A Methoxychlor  | 7.499 | 6.760 | 261.2E6  | 1177.0E6 | 164.861 | 191.090 |
| -----                       |                 |       |       |          |          |         |         |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD087746\  
Data File : PD087746.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 05 Feb 2025 15:23  
Operator : AR\AJ  
Sample : INDA311  
Misc :  
ALS Vial : 99 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Feb 06 07:54:03 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD011625CLP.M  
Quant Title : GC Extractables  
QLast Update : Thu Jan 16 13:39:07 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

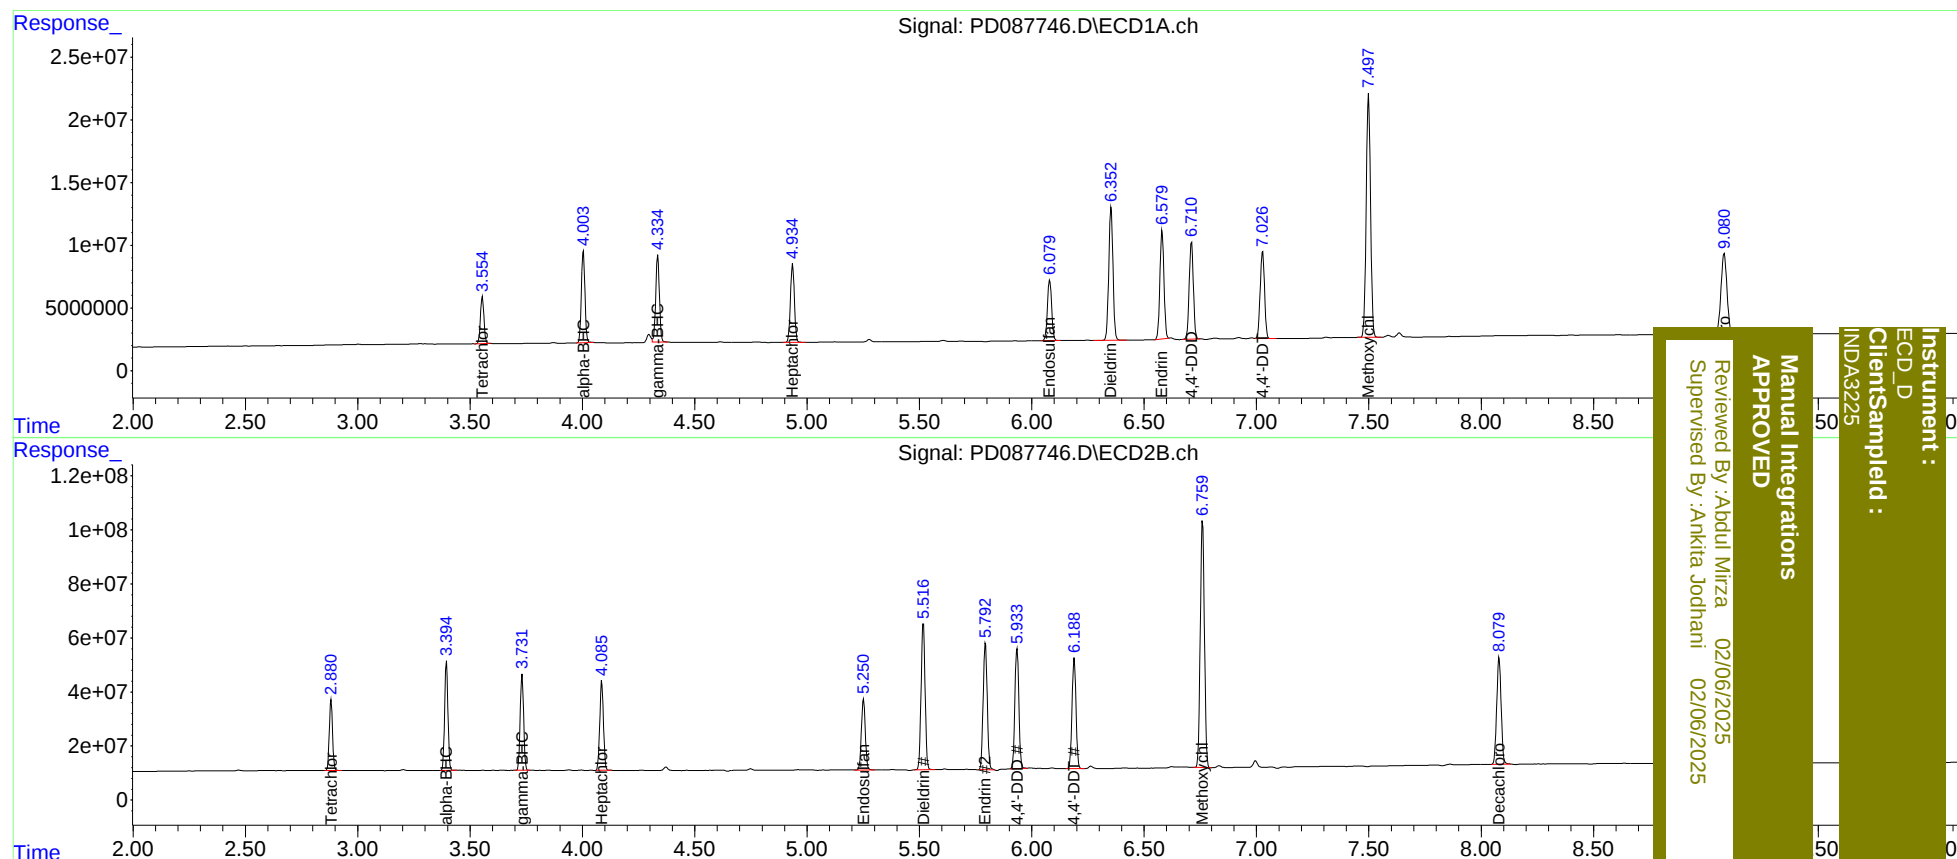

Reviewed By: Abdul Mirza 02/06/2025  
Supervised By: Ankita Jodhani 02/06/2025

Manual Integrations  
APPROVED

Instrument :  
ECD\_D  
Client Sampled :  
INDA3225