

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020623\
 Data File : PD073830.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2023 10:57
 Operator : AR\AJ
 Sample : PB150662BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 21:22:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 25 02:23:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.776	45735326	24747793	19.313	19.496
27)	SA Decachlor...	9.101	7.933	107.2E6	45924441	38.838	38.158
Target Compounds							
6)	B beta-BHC	4.567f	3.870f	264833	358222	0.158	0.438 #
7)	B delta-BHC	4.782	0.000	2653880	0	0.812	N.D. #
8)	B Heptachlo...	5.703	0.000	485381	0	0.149	N.D. #
15)	B Endosulfa...	6.852	0.000	110424	0	<MDL	N.D. #
21)	B Endrin ke...	7.700	0.000	7918	0	<MDL	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020623\
Data File : PD073830.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2023 10:57
Operator : AR\AJ
Sample : PB150662BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 21:22:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jan 25 02:23:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

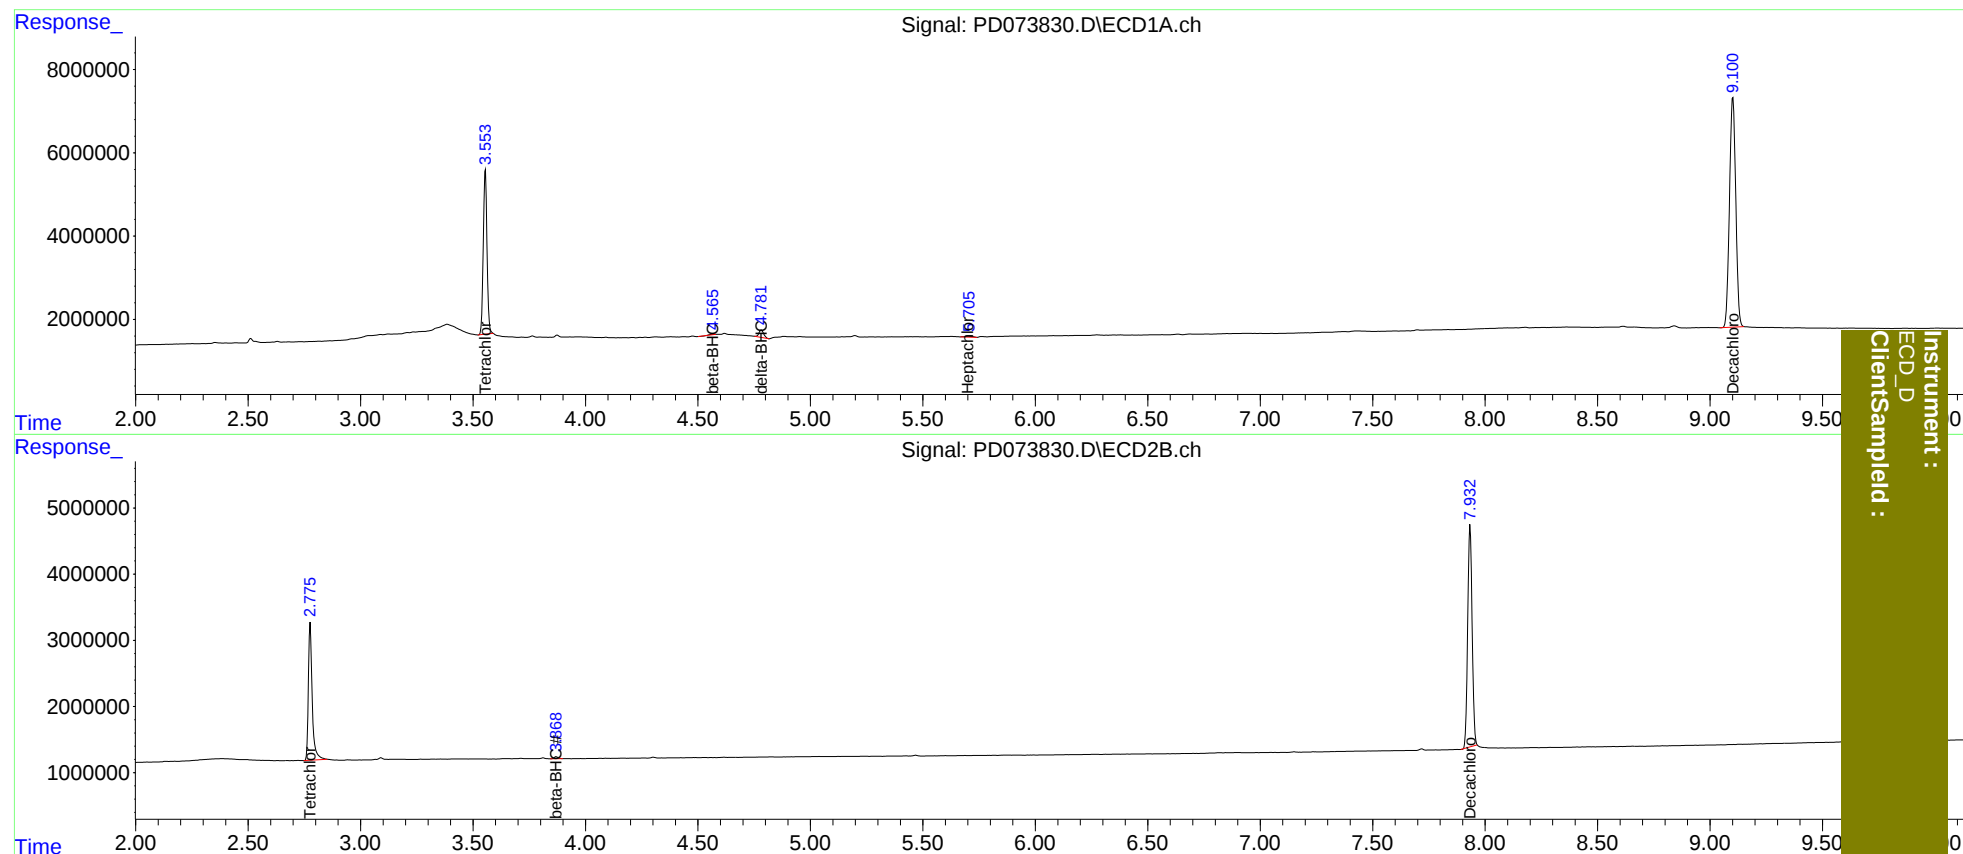


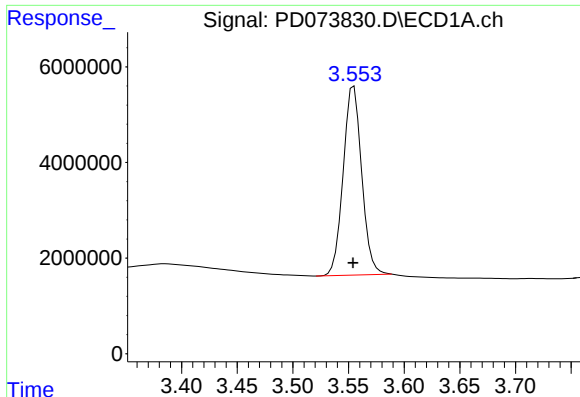

#1 Tetrachloro-m-xylene


R.T.: 3.555 min
Delta R.T.: 0.000 min
Response: 45735326
Conc: 19.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

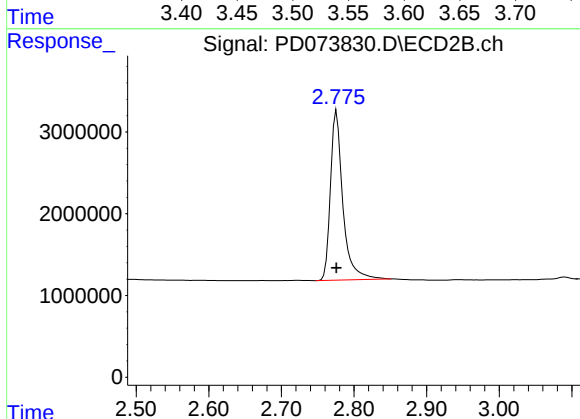


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.000 min
Response: 24747793
Conc: 19.50 ng/ml

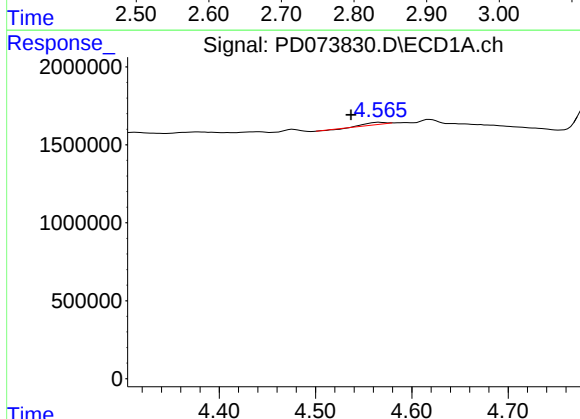


#6 beta-BHC

R.T.: 4.567 min
Delta R.T.: 0.030 min
Response: 264833
Conc: 0.16 ng/ml

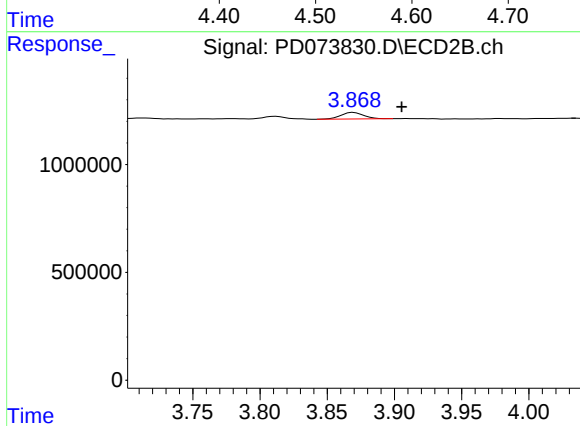

#6 beta-BHC


R.T.: 3.870 min
Delta R.T.: -0.036 min
Response: 358222
Conc: 0.44 ng/ml

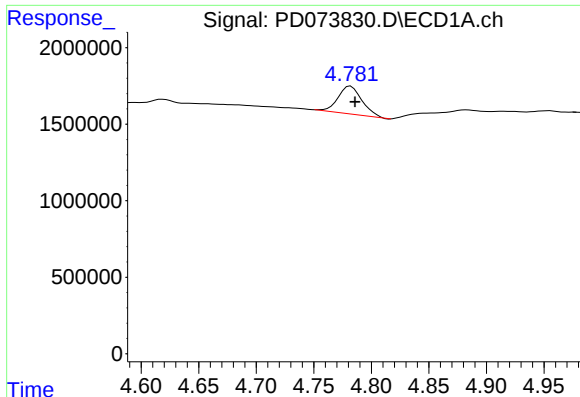

#7 delta-BHC


R.T.: 4.782 min
Delta R.T.: -0.004 min
Response: 2653880
Conc: 0.81 ng/ml

Instrument :
ECD_D
ClientSampleId :

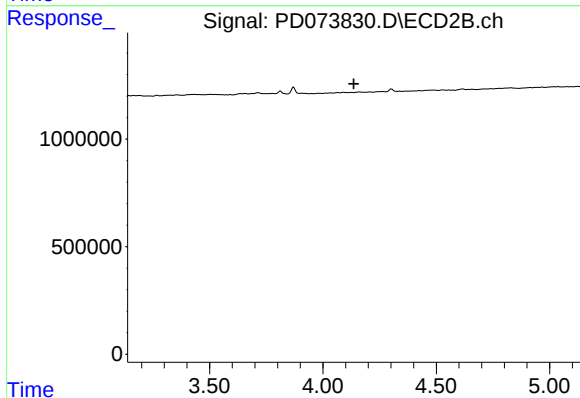


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.137 min
Response: 0
Conc: N.D.

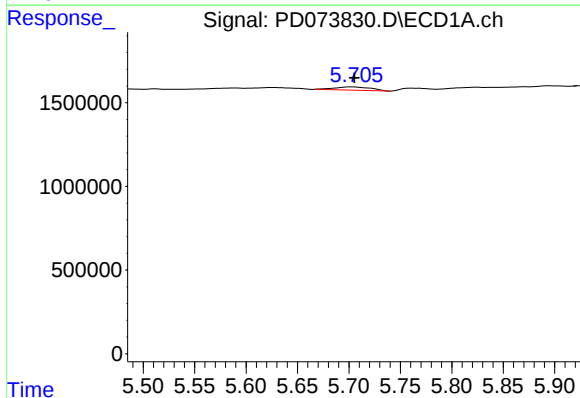


#8 Heptachlor epoxide

R.T.: 5.703 min
Delta R.T.: -0.003 min
Response: 485381
Conc: 0.15 ng/ml

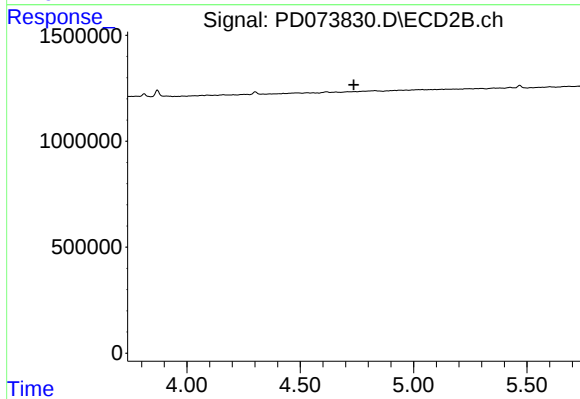

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.737 min
Response: 0
Conc: N.D.

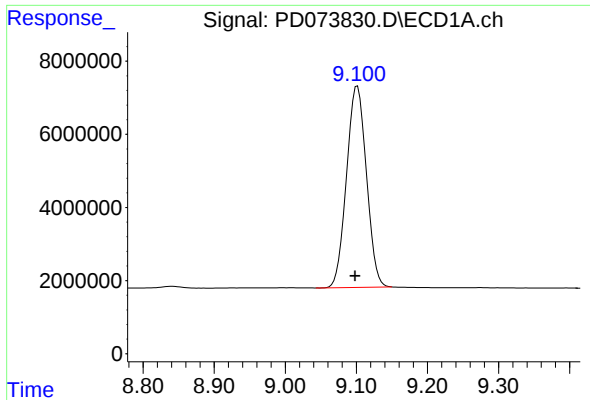

#27 Decachlorobiphenyl

R.T.: 9.101 min
Delta R.T.: 0.003 min
Response: 107153238
Conc: 38.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

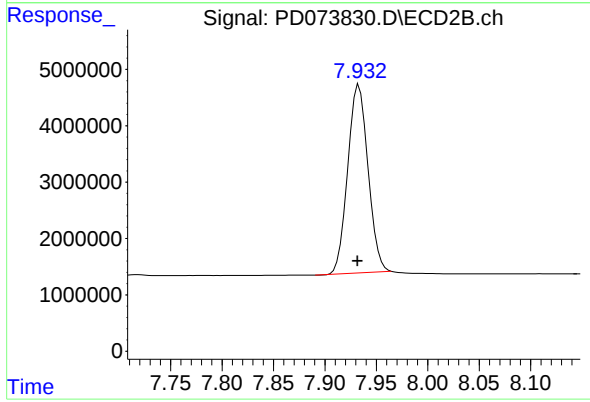

#27 Decachlorobiphenyl

R.T.: 7.933 min
Delta R.T.: 0.001 min
Response: 45924441
Conc: 38.16 ng/ml