

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020623\
 Data File : PD073834.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2023 14:38
 Operator : AR\AJ
 Sample : PIBLK020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 21:27:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 25 02:23:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.554	2.775	50298328	27647091	21.240	21.780
27)	SA Decachlor...	9.103	7.933	120.4E6	51300428	43.635	42.625
Target Compounds							
4)	MA Heptachlor	4.952	0.000	403432	0	0.111	N.D. #
6)	B beta-BHC	4.572f	3.868f	182145	276585	0.108	0.338 #
7)	B delta-BHC	4.782	0.000	1715330	0	0.525	N.D. #
8)	B Heptachlo...	5.700	0.000	298943	0	<MDL	N.D. #
15)	B Endosulfa...	6.793	0.000	153355	0	<MDL	N.D. #
16)	A 4,4'-DDD	6.793f	0.000	153355	0	<MDL	N.D. #
21)	B Endrin ke...	7.700	0.000	84401	0	<MDL	N.D. #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020623\
Data File : PD073834.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2023 14:38
Operator : AR\AJ
Sample : PIBLK020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 21:27:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jan 25 02:23:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

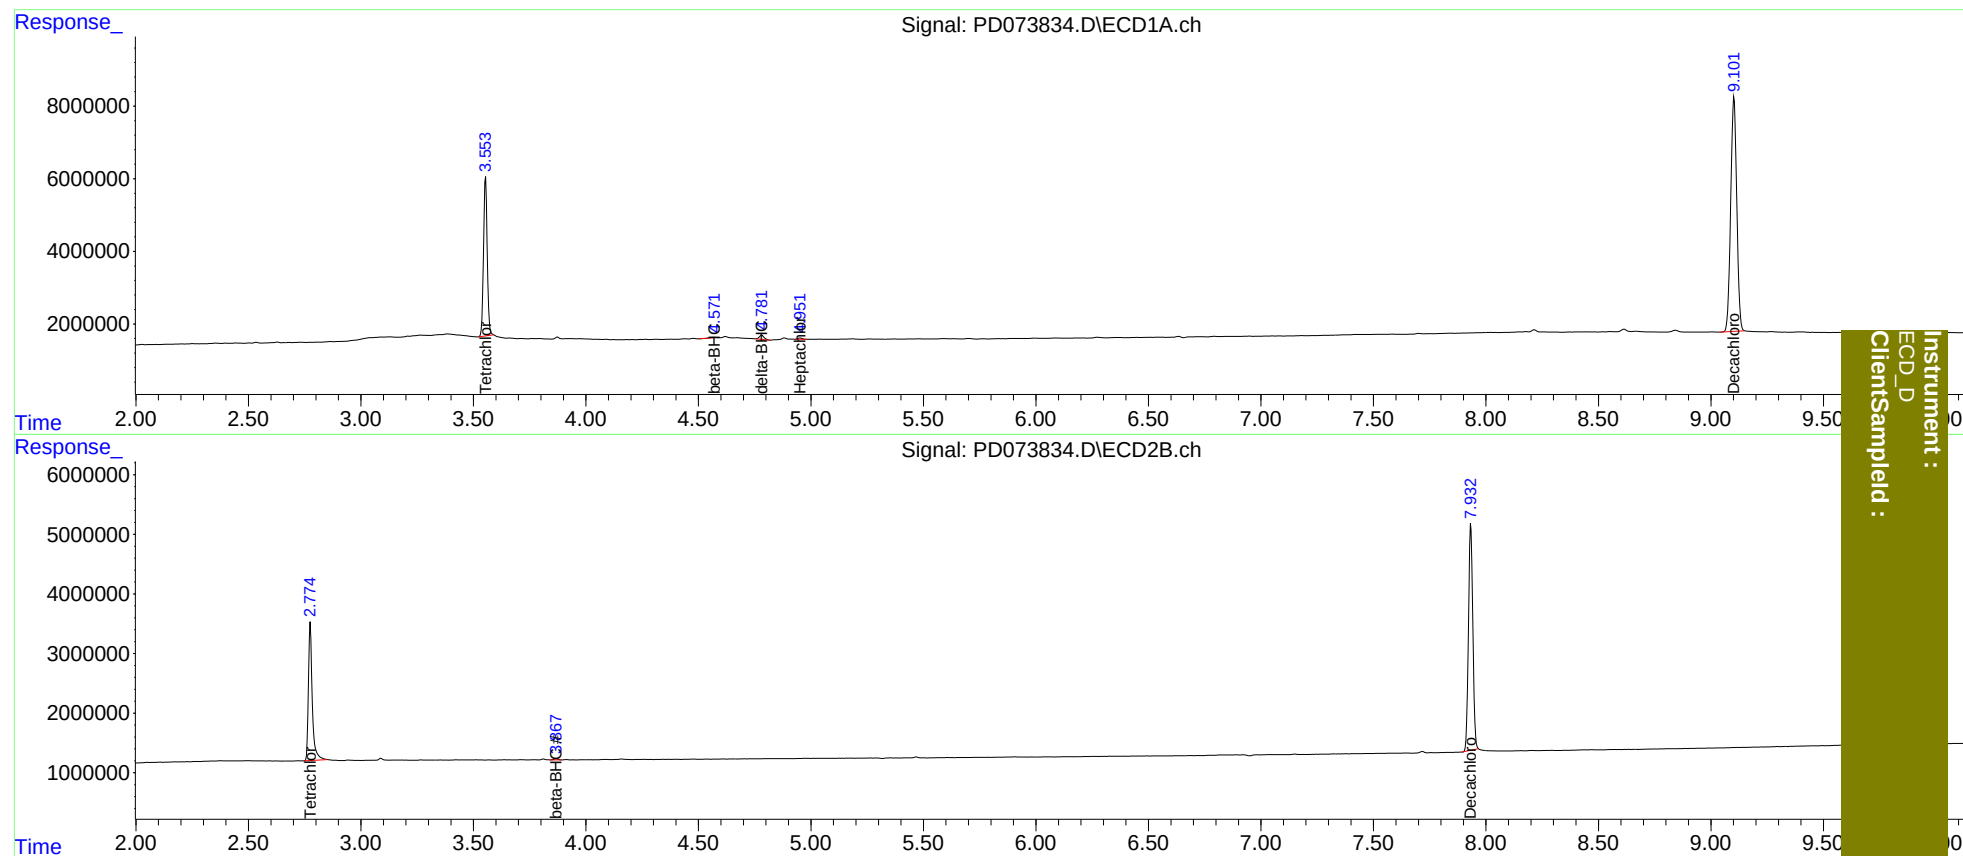


Instrument :
ECD_D
ClientSampled :
10

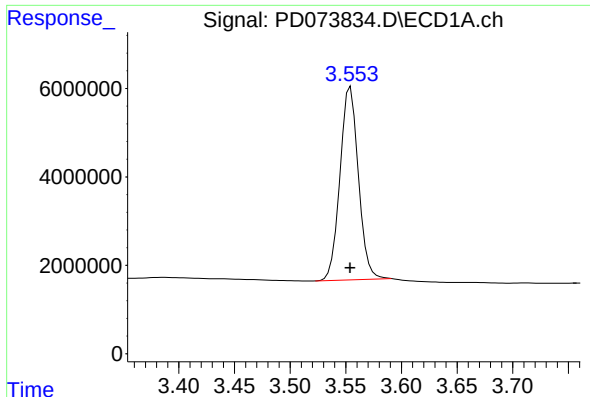

#1 Tetrachloro-m-xylene


R.T.: 3.554 min
Delta R.T.: 0.000 min
Response: 50298328
Conc: 21.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

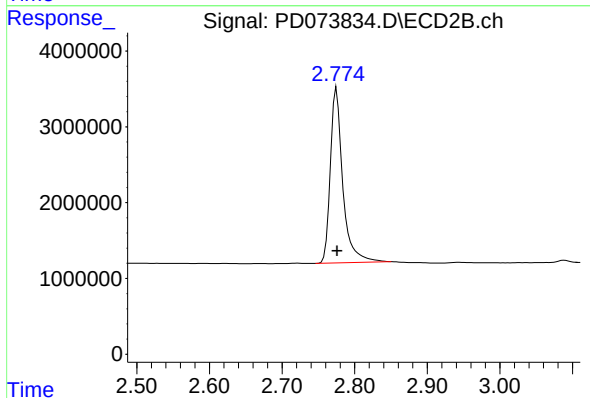


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: 0.000 min
Response: 27647091
Conc: 21.78 ng/ml

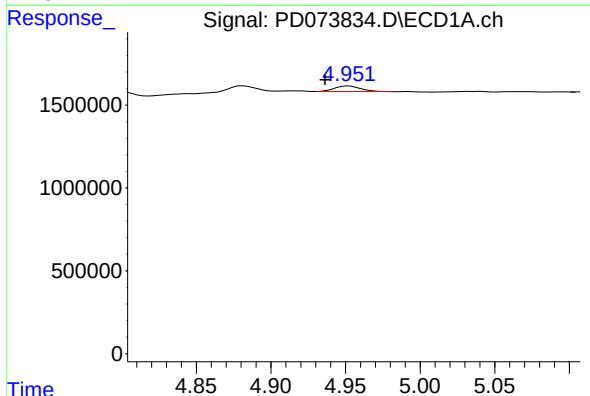


#4 Heptachlor

R.T.: 4.952 min
Delta R.T.: 0.016 min
Response: 403432
Conc: 0.11 ng/ml

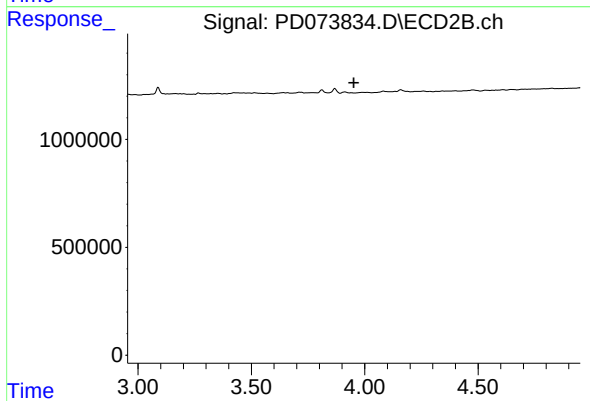

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.952 min
Response: 0
Conc: N.D.

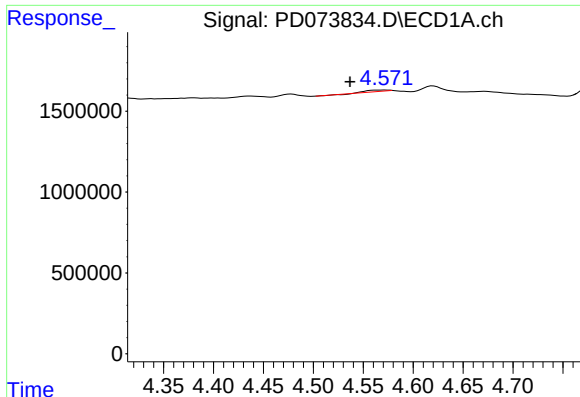

#6 beta-BHC


R.T.: 4.572 min
Delta R.T.: 0.035 min
Response: 182145
Conc: 0.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

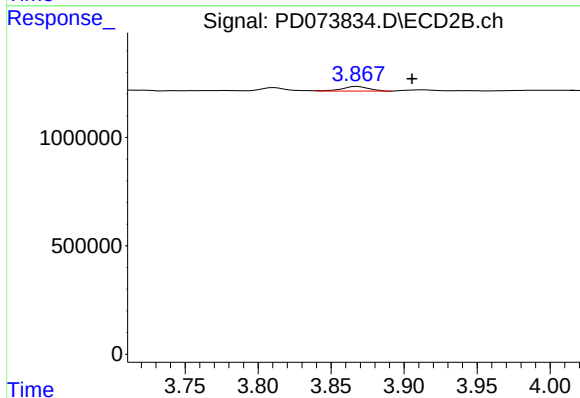


#6 beta-BHC

R.T.: 3.868 min
Delta R.T.: -0.037 min
Response: 276585
Conc: 0.34 ng/ml

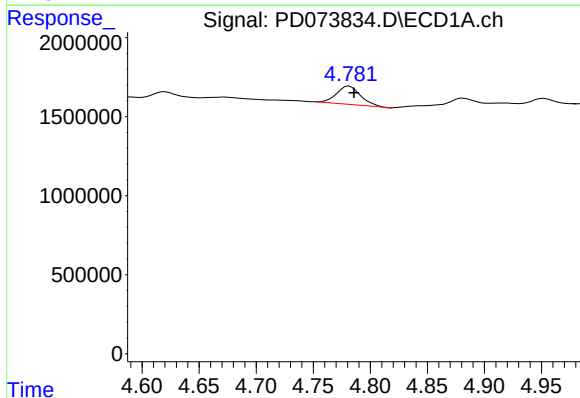


#7 delta-BHC

R.T.: 4.782 min
Delta R.T.: -0.004 min
Response: 1715330
Conc: 0.52 ng/ml

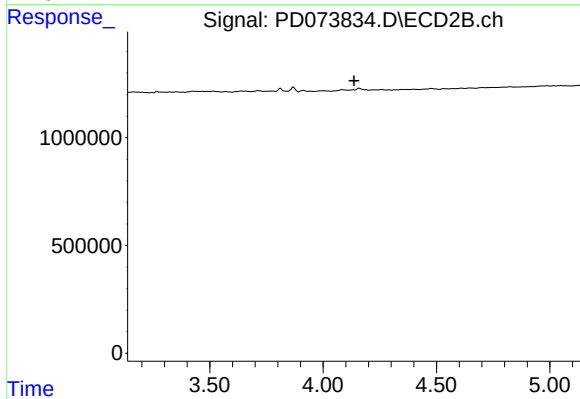

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.137 min
Response: 0
Conc: N.D.

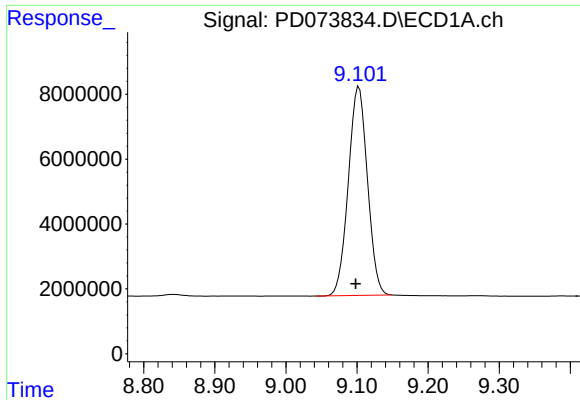

#27 Decachlorobiphenyl

R.T.: 9.103 min
Delta R.T.: 0.005 min
Response: 120385240
Conc: 43.63 ng/ml

Instrument :
ECD_D
ClientSampleId :

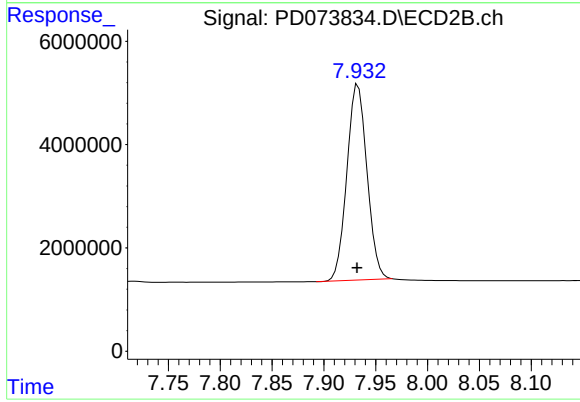

#27 Decachlorobiphenyl

R.T.: 7.933 min
Delta R.T.: 0.001 min
Response: 51300428
Conc: 42.62 ng/ml