

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020623\
 Data File : PD073829.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2023 10:44
 Operator : AR\AJ
 Sample : 01378-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-QT1-2023-02

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/07/2023
 Supervised By : Ankita Jodhani 02/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 21:20:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 25 02:23:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.555	2.776	46175484	24754605	19.499	19.502
2) SA Decachlor...	9.103	7.932	108.6E6	47931930	39.361	39.826m
Target Compounds						
2) A alpha-BHC	4.011	3.280	3776460	1721702	0.991	0.972
3) MA gamma-BHC...	4.345	3.610	3725019	1602626	1.023	0.953
4) MA Heptachlor	4.938	3.952	4325261	1674789	1.189	1.110
5) MB Aldrin	5.282	4.234	4260813	1833331	1.191	1.080
6) B beta-BHC	4.540	3.906	2295096	905390	1.366	1.108
7) B delta-BHC	4.785	4.137	5834144	1695886	1.785m	0.978 #
8) B Heptachlo...	5.708	4.737	4578471	1700398	1.408	1.092
9) A Endosulfan I	6.095	5.108	3884966	1621914	1.266	1.130
10) B trans-Chl...	5.965	4.988	4051722	1769630	1.258	1.133
11) B cis-Chlor...	6.045	5.052	4168458	1800133	1.251	1.120
12) B 4,4'-DDE	6.216	5.242	3508433	1437856	1.113	0.979
13) MA Dieldrin	6.371	5.373	3913387	1656582	1.165	1.064
14) MA Endrin	6.600	5.648	3179168	1451282	1.136m	1.128
15) B Endosulfa...	6.820	5.942	3573799	1508225	1.209	1.096
16) A 4,4'-DDD	6.732	5.797	2869597	1292265	1.128m	1.071
17) MA 4,4'-DDT	7.049	6.049	3046688	1135564	1.116	0.962
18) B Endrin al...	6.950	6.122	3181172	1271179	1.330	1.164
19) B Endosulfa...	7.184	6.345	3663480	1448197	1.319	1.152
20) A Methoxychlor	7.524	6.626	2037419	637419	1.369	1.156
21) B Endrin ke...	7.670	6.851	3649554	1703197	1.145m	1.132m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073829\
 Data File : PD073829.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2023 10:44
 Operator : AR\AJ
 Sample : 01378-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 21:20:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 25 02:23:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

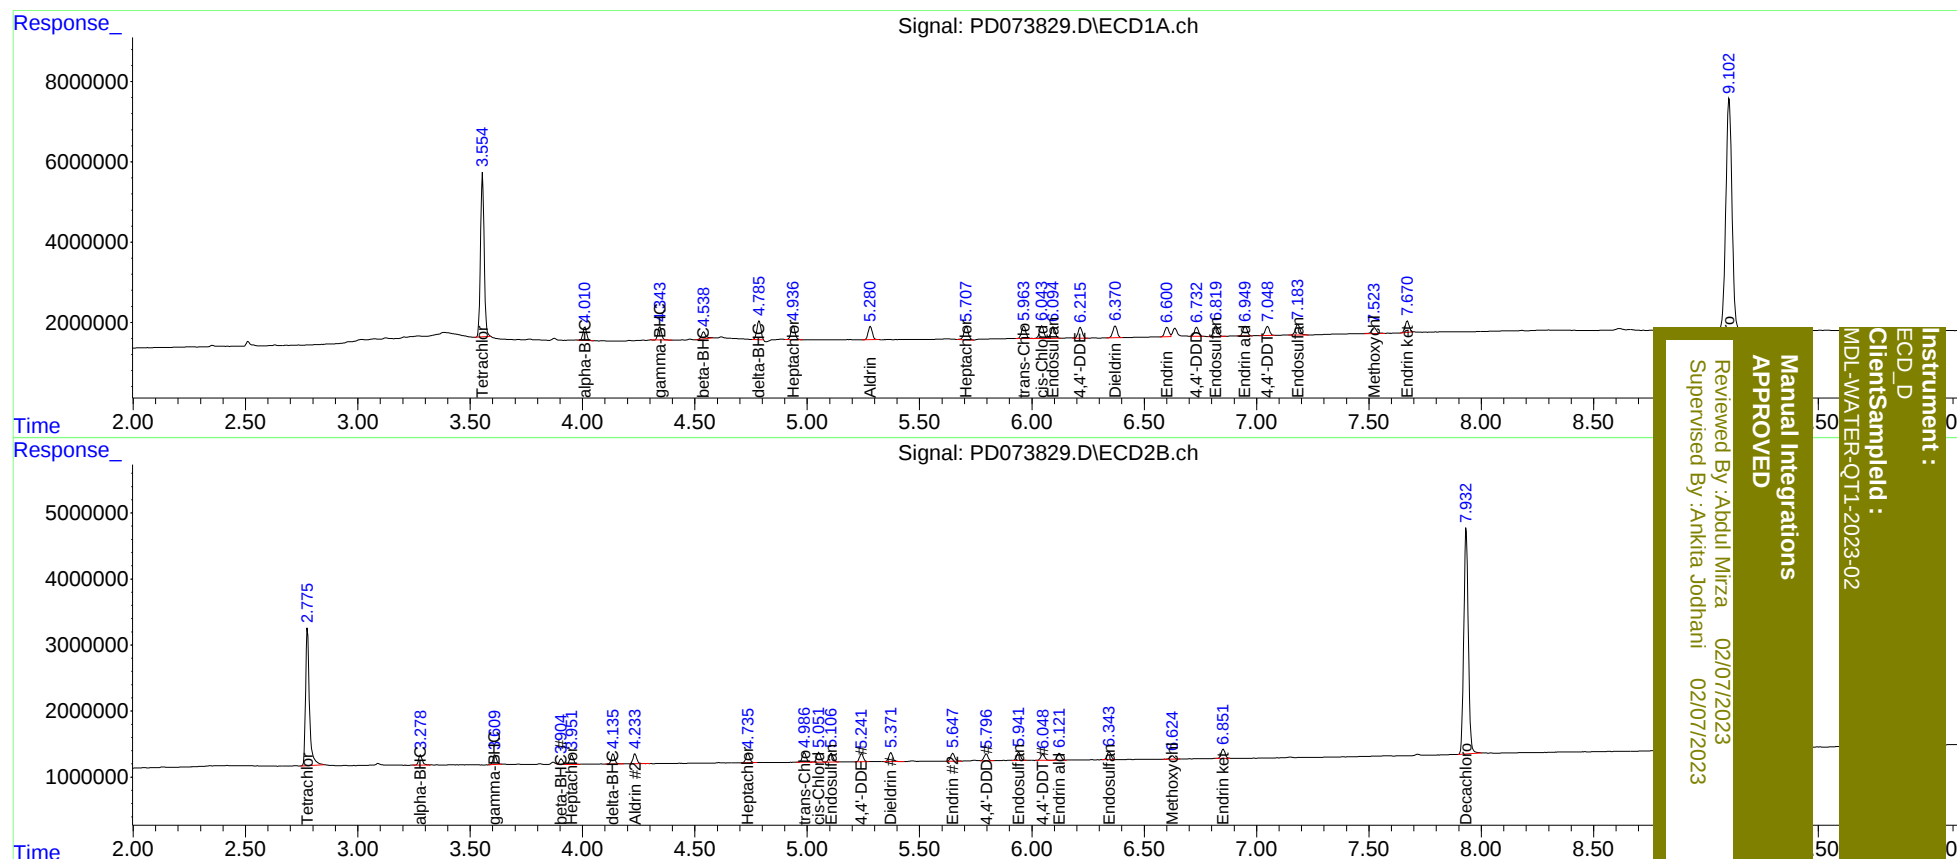

Manual Integrations
 APPROVED
 Reviewed By: Abdul Miza 02/07/2023
 Supervised By: Ankita Jodhani 02/07/2023

Instrument :
 ECD_D
 Client Sample :
 MDL-WATER-QT1-2023-02