

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD020623\  
 Data File : PD073830.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 06 Feb 2023 10:57  
 Operator : AR\AJ  
 Sample : PB150662BL  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 PBLK662

Manual Integrations  
 APPROVED

Reviewed By : Abdul Mirza 02/07/2023  
 Supervised By : Ankita Jodhani 02/07/2023

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Feb 06 21:22:22 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD012523CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Wed Jan 25 02:23:06 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml   |
|-----------------------------|-------|-------|----------|----------|--------|---------|
| -----                       |       |       |          |          |        |         |
| System Monitoring Compounds |       |       |          |          |        |         |
| 1) SA Tetrachlo...          | 3.555 | 2.776 | 45735326 | 24747793 | 19.313 | 19.496  |
| 27) SA Decachlor...         | 9.101 | 7.932 | 107.2E6  | 47122906 | 38.838 | 39.154m |


Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD020623\  
Data File : PD073830.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 06 Feb 2023 10:57  
Operator : AR\AJ  
Sample : PB150662BL  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Feb 06 21:22:22 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD012523CLP.M  
Quant Title : GC Extractables  
QLast Update : Wed Jan 25 02:23:06 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

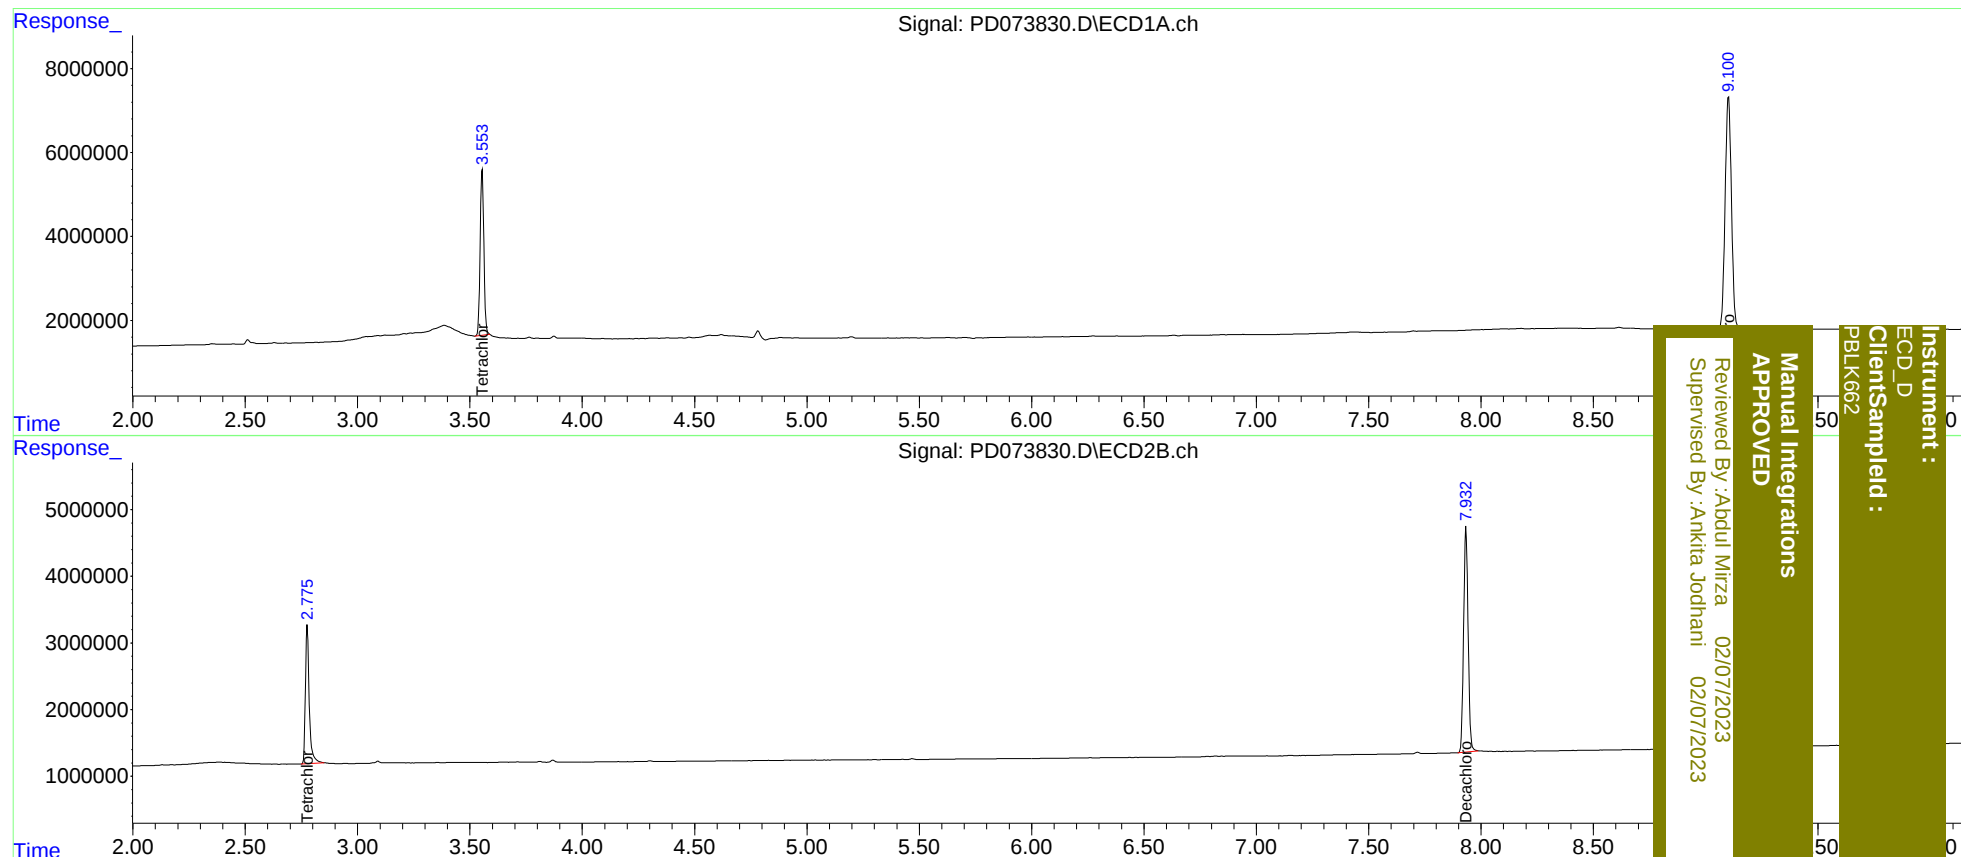

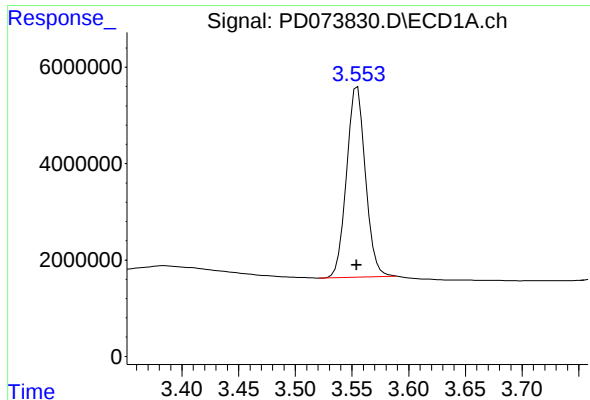


#1 Tetrachloro-m-xylene

R.T.: 3.555 min  
Delta R.T.: 0.000 min  
Response: 45735326  
Conc: 19.31 ng/ml

Instrument :  
ECD\_D  
ClientSampleId :  
PBLK662


Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 02/07/2023  
Supervised By :Ankita Jodhani 02/07/2023

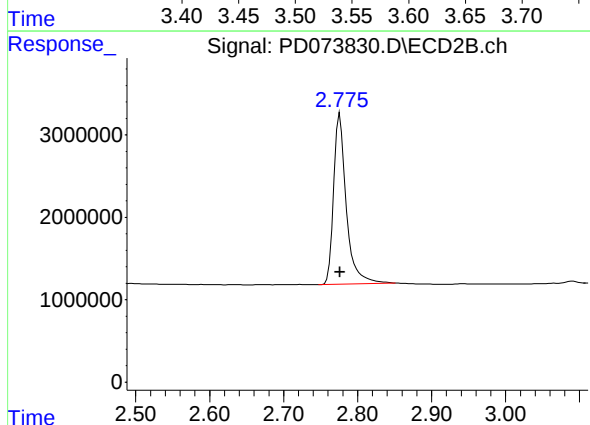


#1 Tetrachloro-m-xylene

R.T.: 2.776 min  
Delta R.T.: 0.000 min  
Response: 24747793  
Conc: 19.50 ng/ml

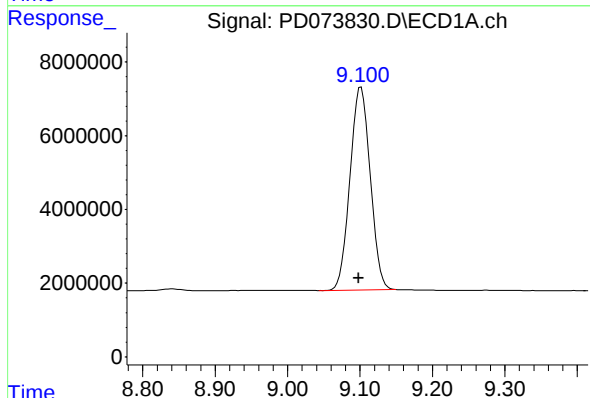

#27 Decachlorobiphenyl

R.T.: 9.101 min  
Delta R.T.: 0.003 min  
Response: 107153238  
Conc: 38.84 ng/ml

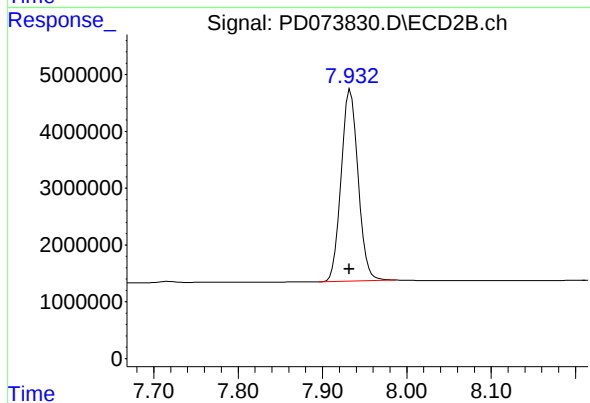

#27 Decachlorobiphenyl

R.T.: 7.932 min  
Delta R.T.: 0.000 min  
Response: 47122906  
Conc: 39.15 ng/ml m