

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020624\
 Data File : PD081129.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2024 17:33
 Operator : AR\AJ
 Sample : P1141-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EB-3-0-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 21:07:14 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.795	22944387	43193532	16.163	18.056
28)	SA Decachlor...	9.111	7.932	34656119	46574770	17.221	17.486
Target Compounds							
3)	MA gamma-BHC...	0.000	3.633	0	276244	N.D.	0.074 #
4)	MA Heptachlor	4.939	0.000	123239	0	0.050	N.D. #
7)	B delta-BHC	4.792	0.000	3711860	0	1.480	N.D. #
10)	B gamma-Chl...	5.940f	0.000	422787	0	0.193	N.D. #
13)	MA Dieldrin	6.398f	0.000	143931	0	0.065	N.D. #
14)	MA Endrin	0.000	5.676f	0	451785	N.D.	0.152 #
15)	B Endosulfa...	6.809f	0.000	373343	0	0.193	N.D. #
21)	B Endrin ke...	7.709f	0.000	204084	0	0.098	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020624\
Data File : PD081129.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2024 17:33
Operator : AR\AJ
Sample : P1141-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
EB-3-0-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 21:07:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

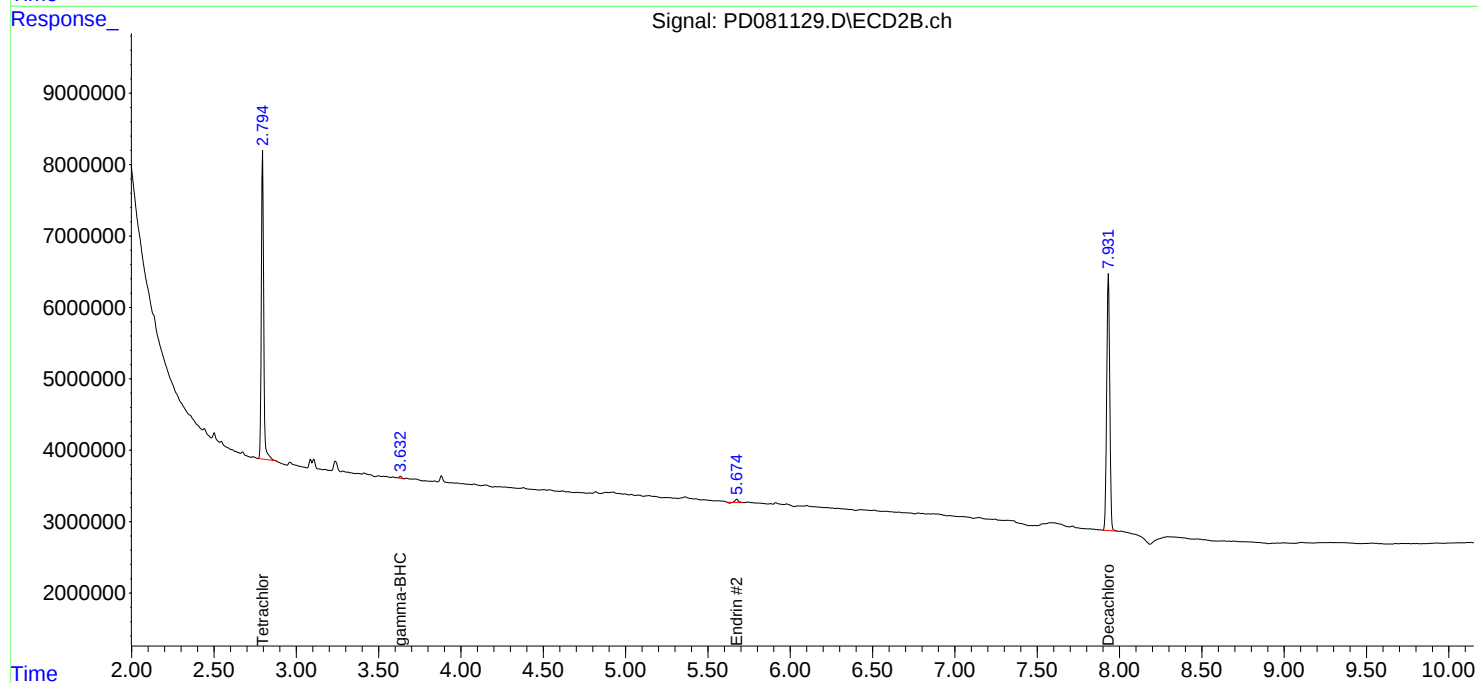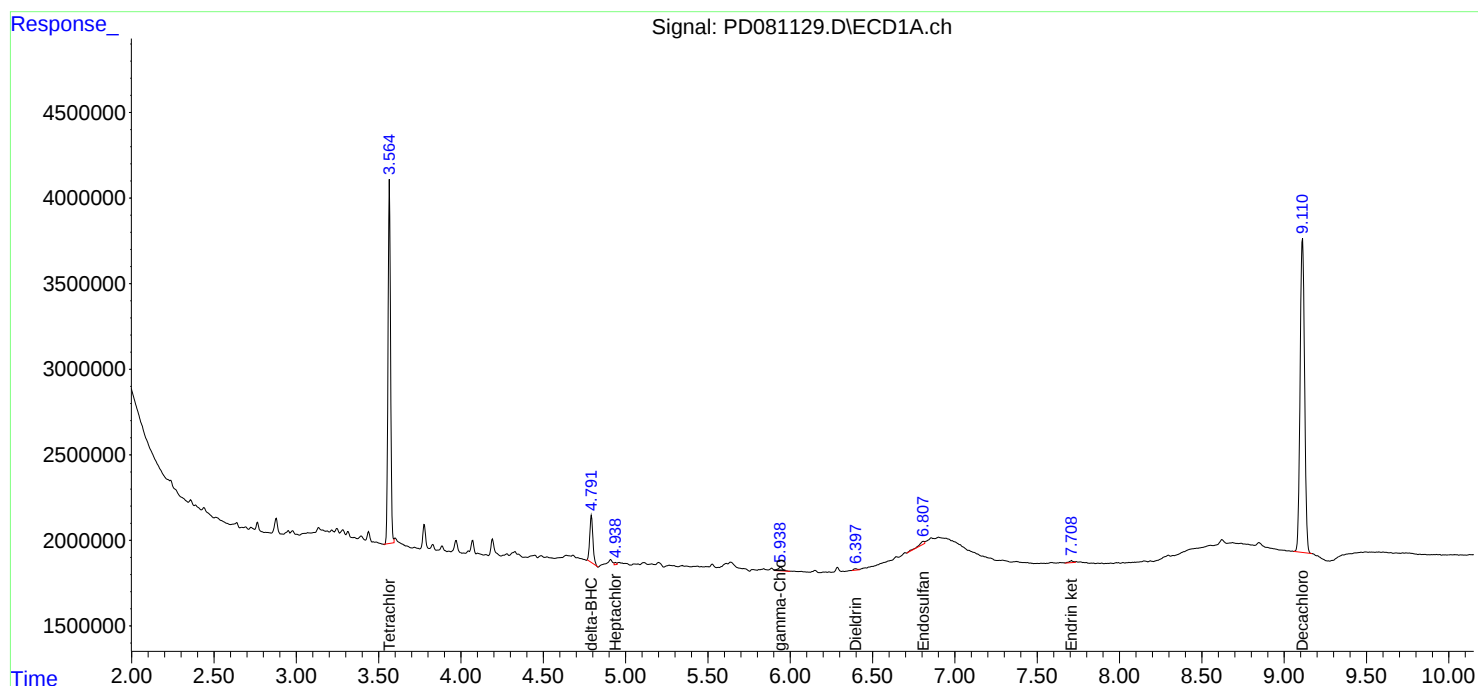


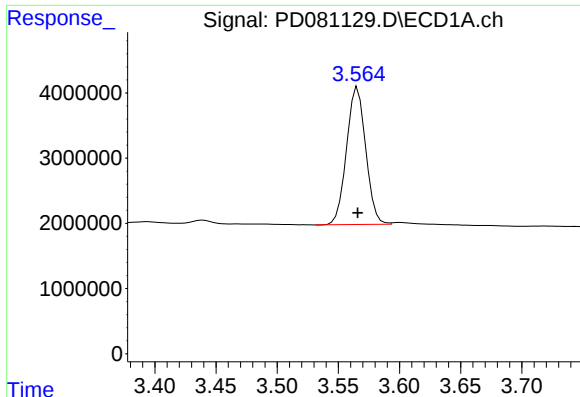

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 22944387
Conc: 16.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-3-0-2

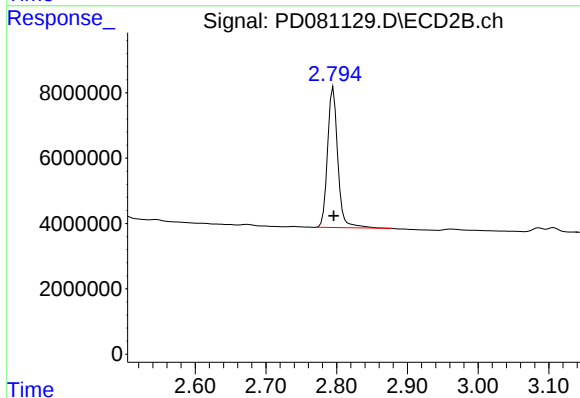


#1 Tetrachloro-m-xylene

R.T.: 2.795 min
Delta R.T.: 0.000 min
Response: 43193532
Conc: 18.06 ng/ml

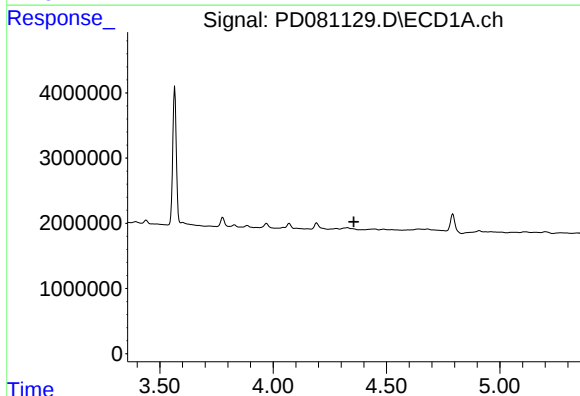


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.355 min
Response: 0
Conc: N.D.

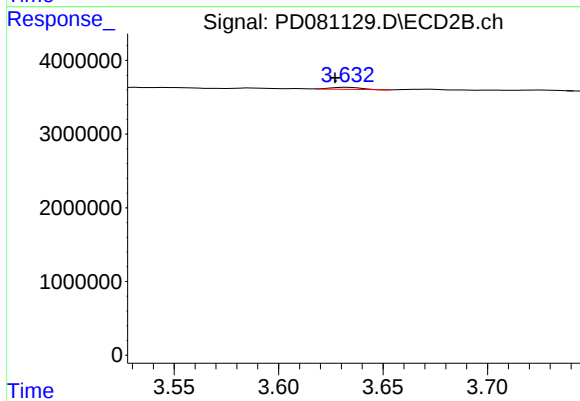

#3 gamma-BHC (Lindane)


R.T.: 3.633 min
Delta R.T.: 0.006 min
Response: 276244
Conc: 0.07 ng/ml

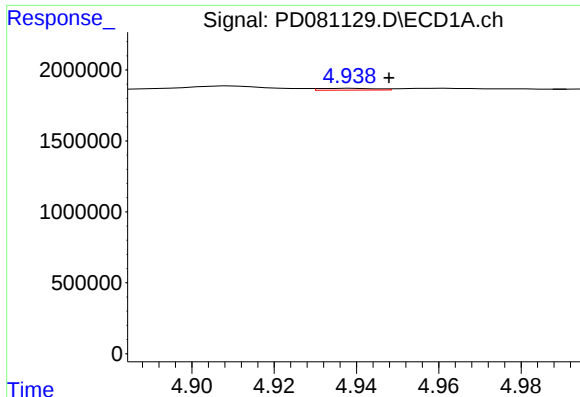

#4 Heptachlor


R.T.: 4.939 min
Delta R.T.: -0.009 min
Response: 123239
Conc: 0.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-3-0-2

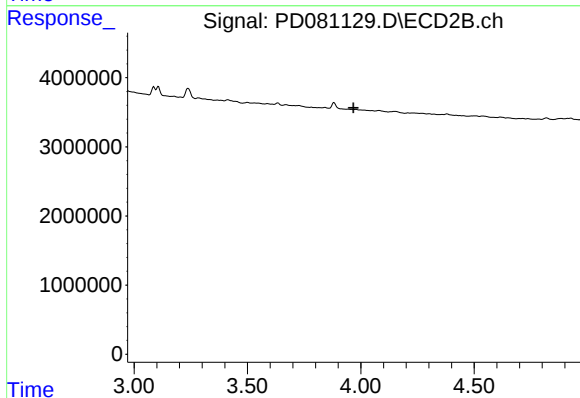


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 3.968 min
Response: 0
Conc: N.D.

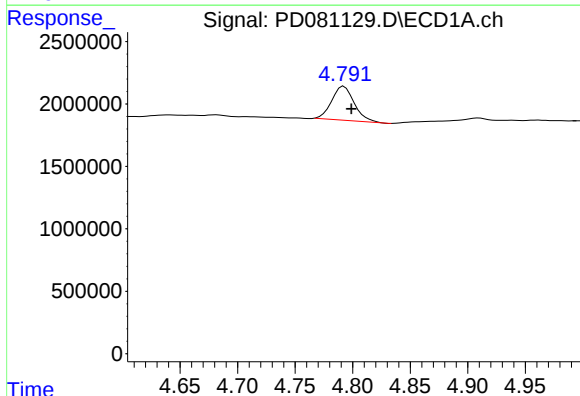


#7 delta-BHC

R.T.: 4.792 min
Delta R.T.: -0.007 min
Response: 3711860
Conc: 1.48 ng/ml

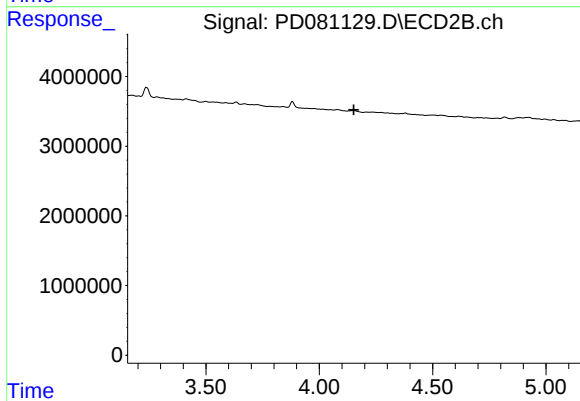

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.153 min
Response: 0
Conc: N.D.

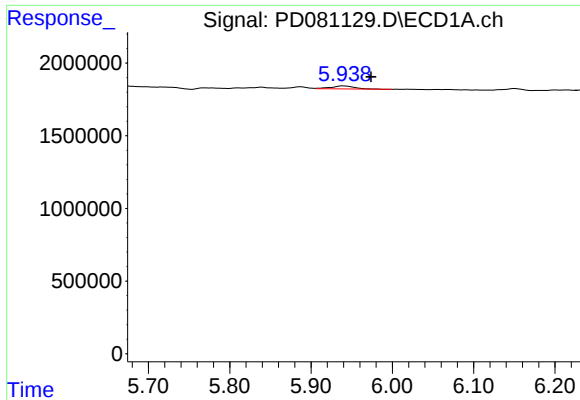

#10 gamma-Chlordane


R.T.: 5.940 min
Delta R.T.: -0.034 min
Response: 422787
Conc: 0.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-3-0-2

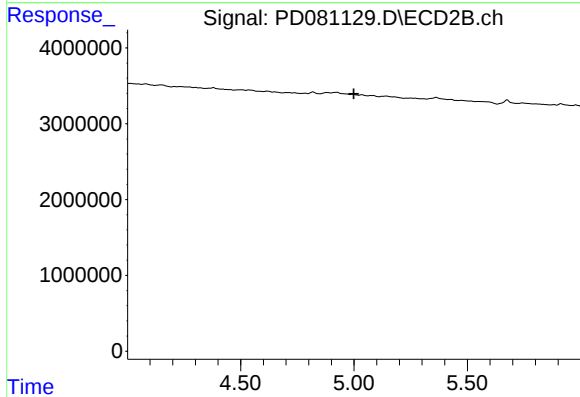


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.000 min
Response: 0
Conc: N.D.

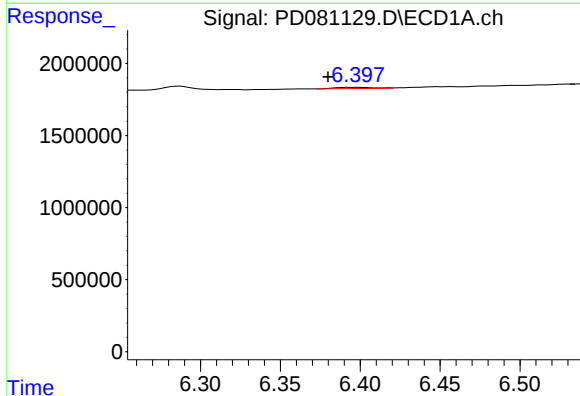


#13 Dieldrin

R.T.: 6.398 min
Delta R.T.: 0.018 min
Response: 143931
Conc: 0.07 ng/ml

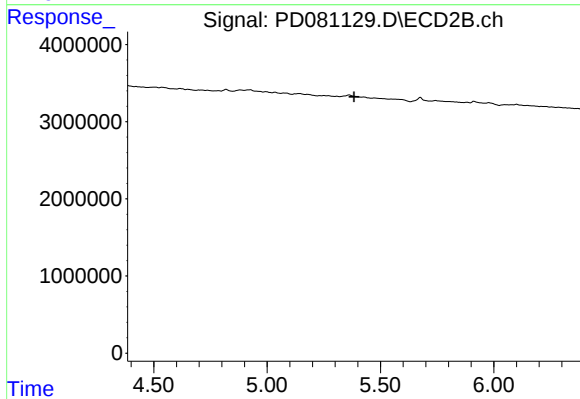

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 5.384 min
Response: 0
Conc: N.D.

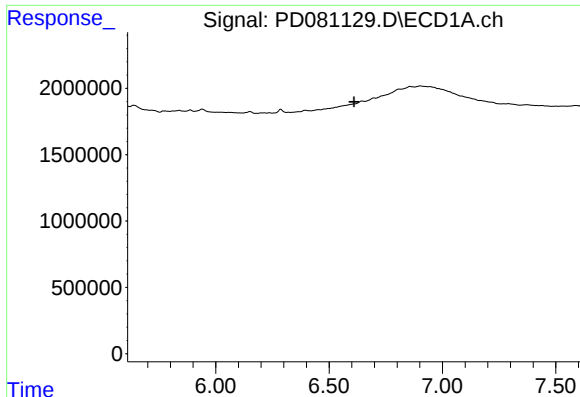

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.610 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
EB-3-0-2

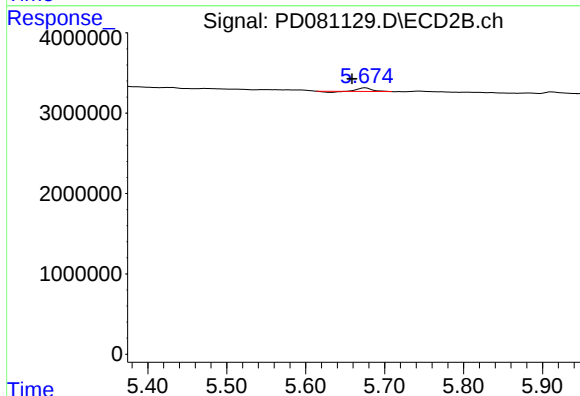


#14 Endrin

R.T.: 5.676 min
Delta R.T.: 0.017 min
Response: 451785
Conc: 0.15 ng/ml

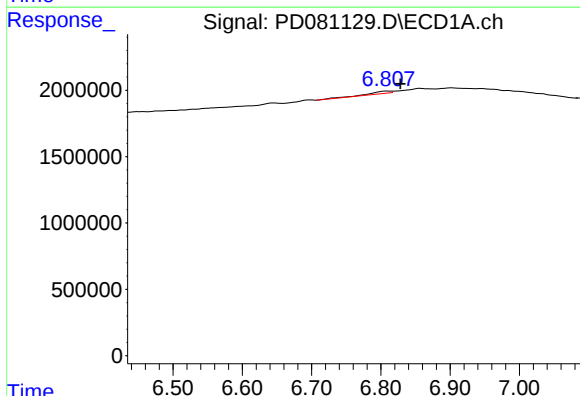


#15 Endosulfan II

R.T.: 6.809 min
Delta R.T.: -0.020 min
Response: 373343
Conc: 0.19 ng/ml

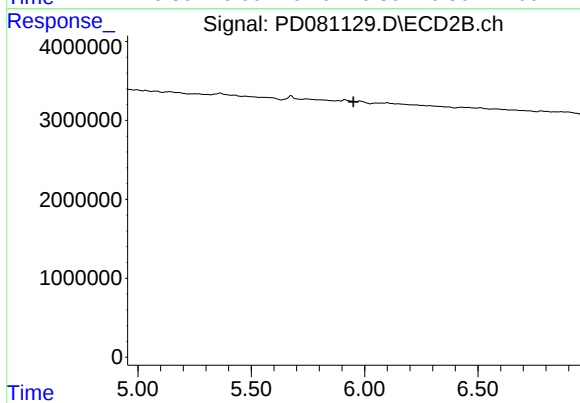

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.951 min
Response: 0
Conc: N.D.

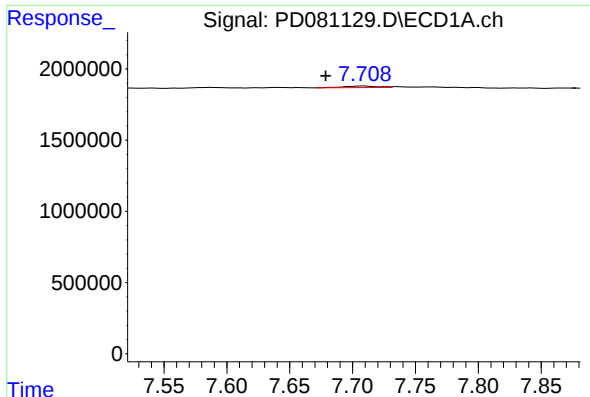

#21 Endrin ketone


R.T.: 7.709 min
Delta R.T.: 0.030 min
Response: 204084
Conc: 0.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-3-0-2

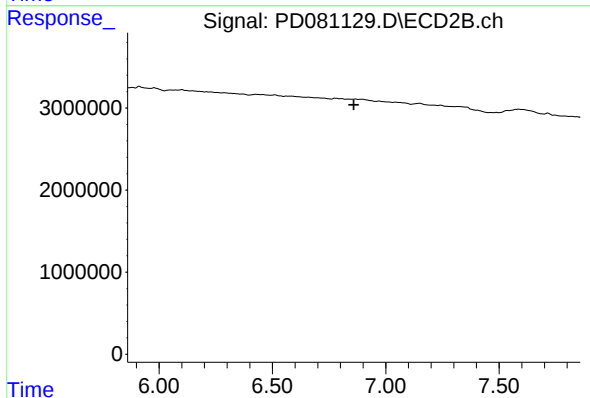


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.859 min
Response: 0
Conc: N.D.

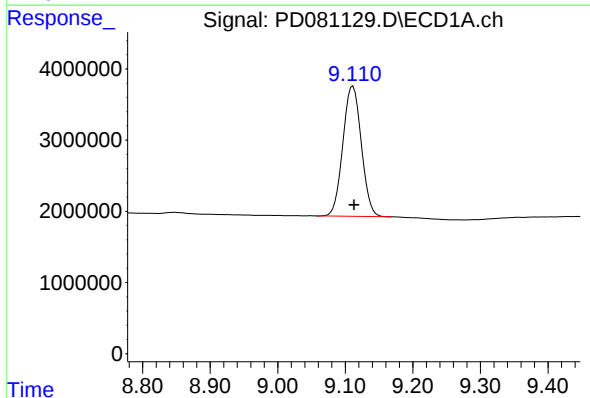

#28 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: -0.002 min
Response: 34656119
Conc: 17.22 ng/ml

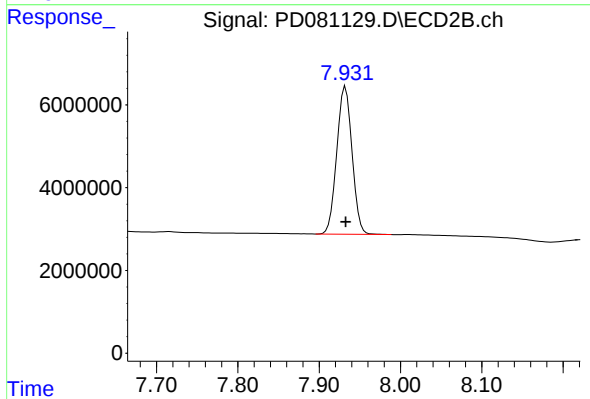

#28 Decachlorobiphenyl

R.T.: 7.932 min
Delta R.T.: 0.000 min
Response: 46574770
Conc: 17.49 ng/ml