

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020624\
 Data File : PD081131.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2024 18:00
 Operator : AR\AJ
 Sample : P1141-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EB-3-2-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 21:08:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.796	27049540	46281188	19.055	19.347
28)	SA Decachlor...	9.112	7.932	39914635	53559322	19.834	20.108
Target Compounds							
2)	A alpha-BHC	0.000	3.283	0	104033	N.D.	0.027 #
3)	MA gamma-BHC...	0.000	3.634	0	296000	N.D.	0.079 #
4)	MA Heptachlor	4.934	3.966	431381	135257	0.175	0.039 #
7)	B delta-BHC	4.793	0.000	11043994	0	4.402	N.D. #
13)	MA Dieldrin	6.388	0.000	176066	0	0.080	N.D. #
14)	MA Endrin	0.000	5.675f	0	970761	N.D.	0.328 #
15)	B Endosulfa...	6.809f	0.000	162431	0	0.084	N.D. #
21)	B Endrin ke...	7.706f	0.000	243935	0	0.117	N.D. #
27)	Chlordane-5	6.911	0.000	111831	0	1.602	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020624\
Data File : PD081131.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2024 18:00
Operator : AR\AJ
Sample : P1141-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
EB-3-2-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 21:08:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

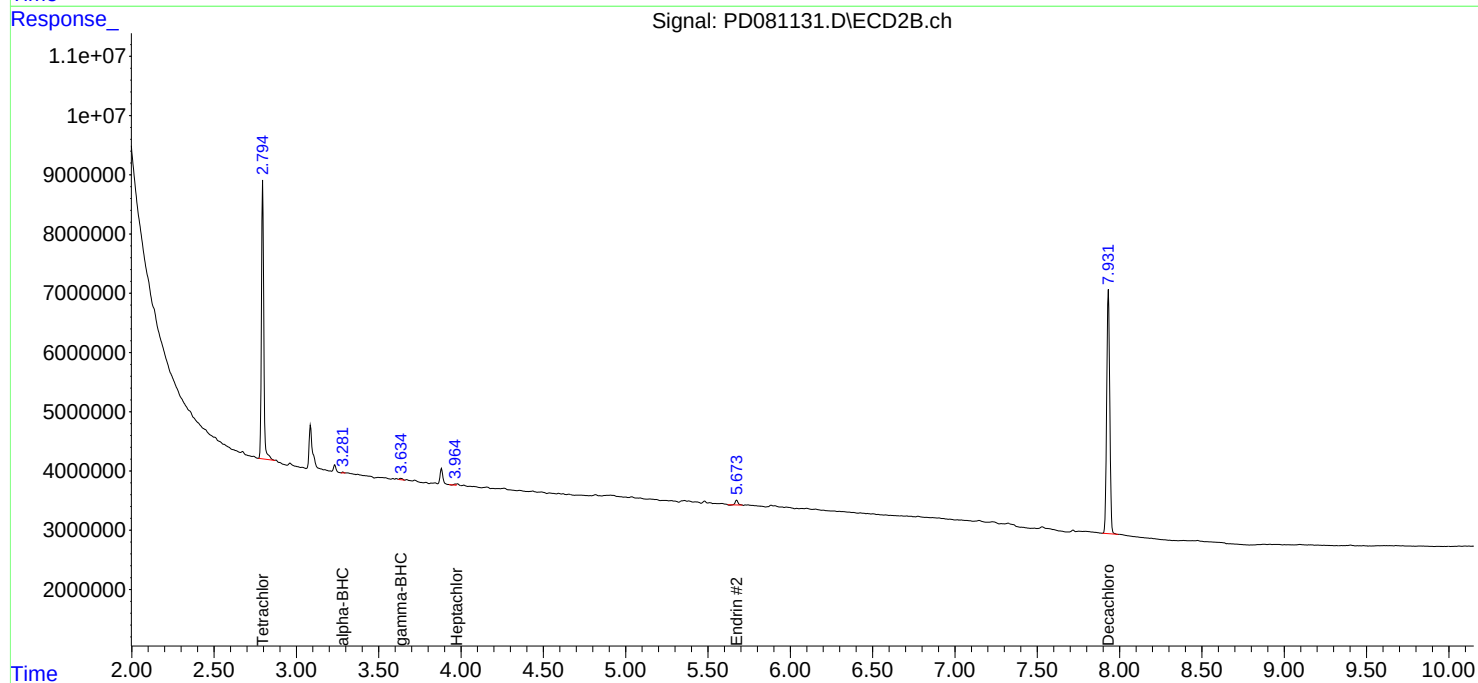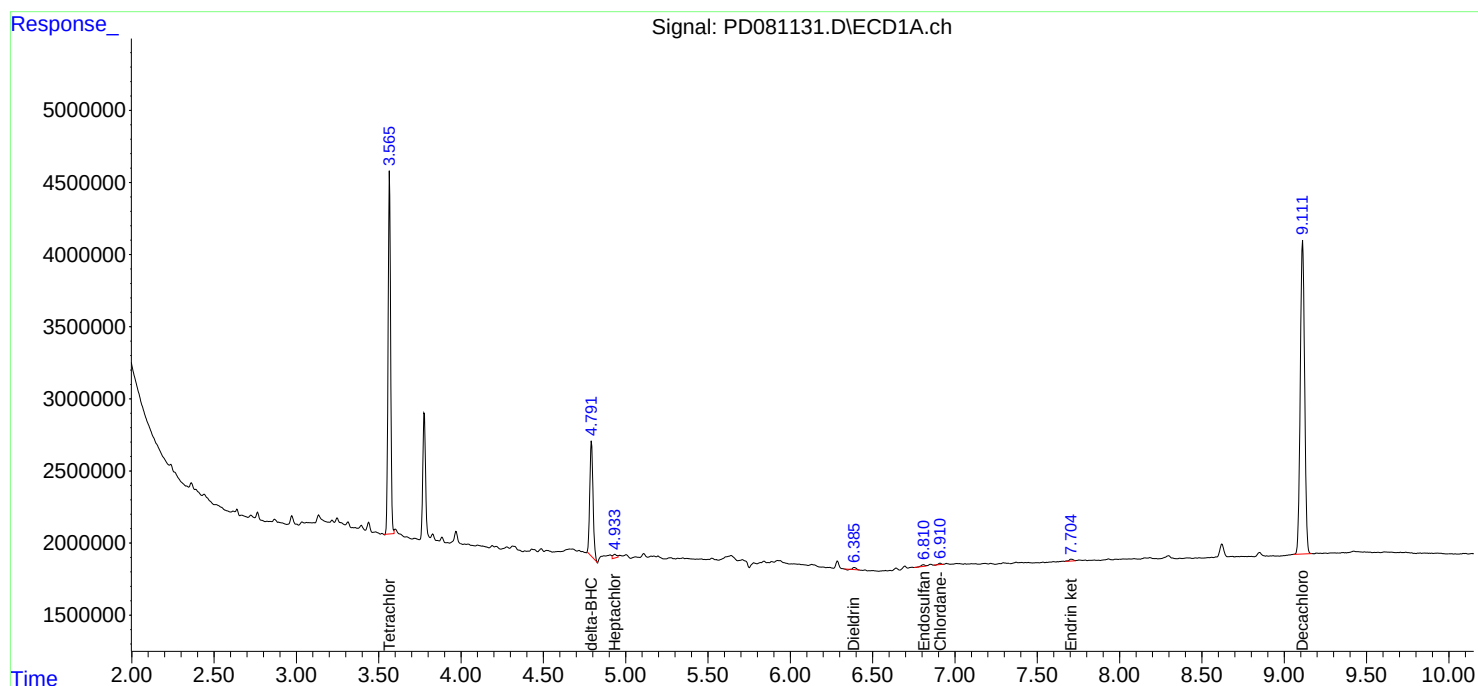


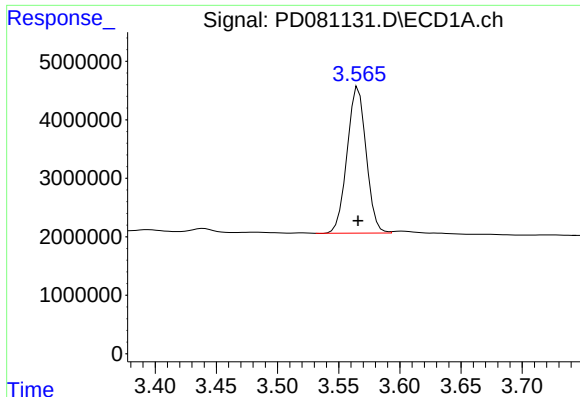

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 27049540
Conc: 19.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-3-2-4

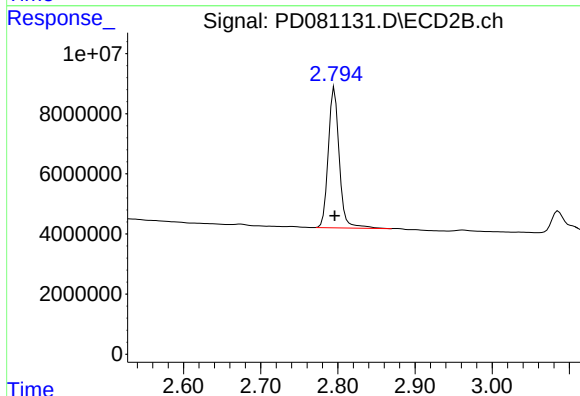


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 46281188
Conc: 19.35 ng/ml

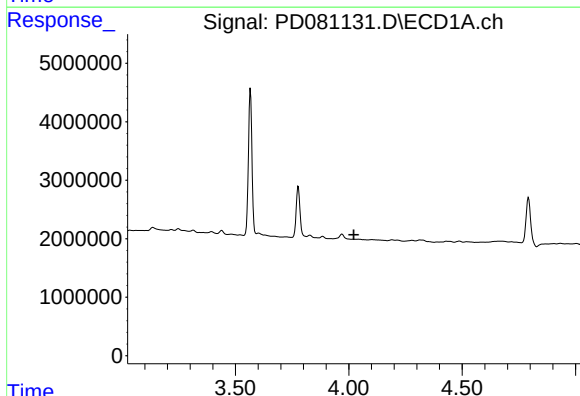


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 4.022 min
Response: 0
Conc: N.D.

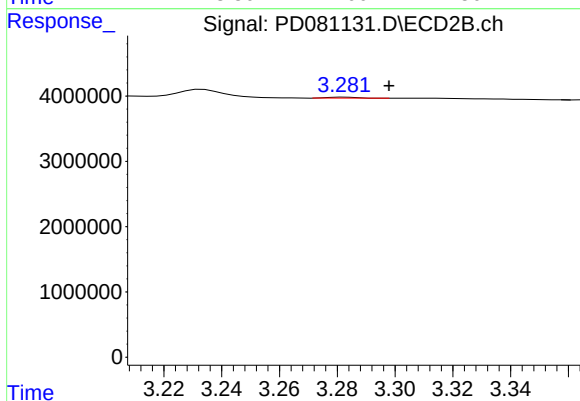

#2 alpha-BHC


R.T.: 3.283 min
Delta R.T.: -0.015 min
Response: 104033
Conc: 0.03 ng/ml

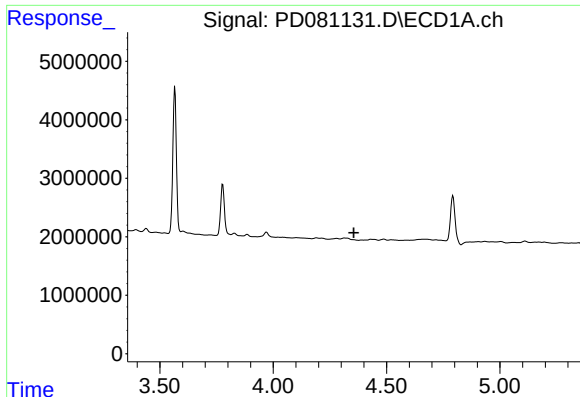

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.355 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
EB-3-2-4

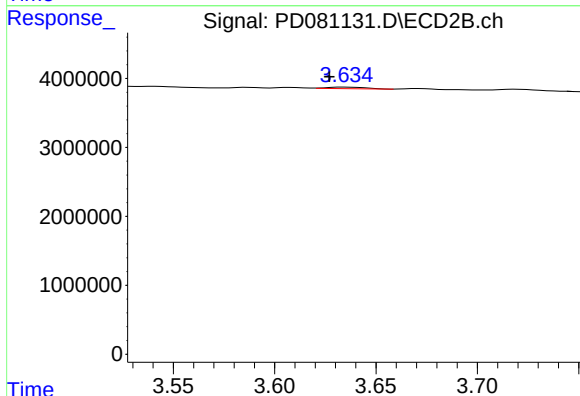


#3 gamma-BHC (Lindane)

R.T.: 3.634 min
Delta R.T.: 0.007 min
Response: 296000
Conc: 0.08 ng/ml

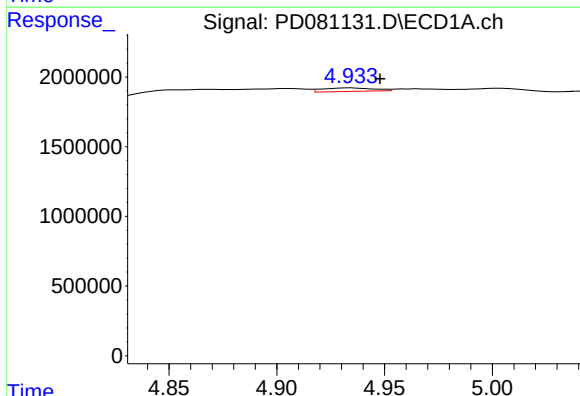


#4 Heptachlor

R.T.: 4.934 min
Delta R.T.: -0.014 min
Response: 431381
Conc: 0.17 ng/ml

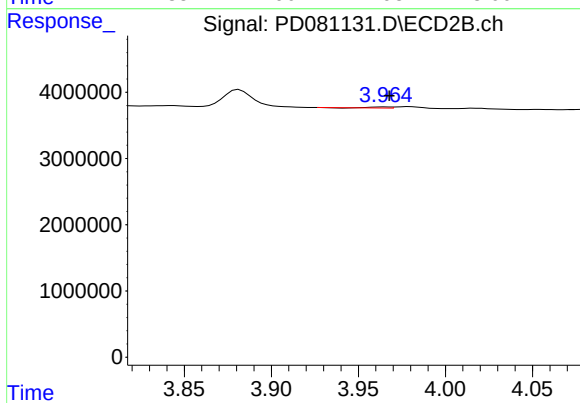

#4 Heptachlor


R.T.: 3.966 min
Delta R.T.: -0.002 min
Response: 135257
Conc: 0.04 ng/ml

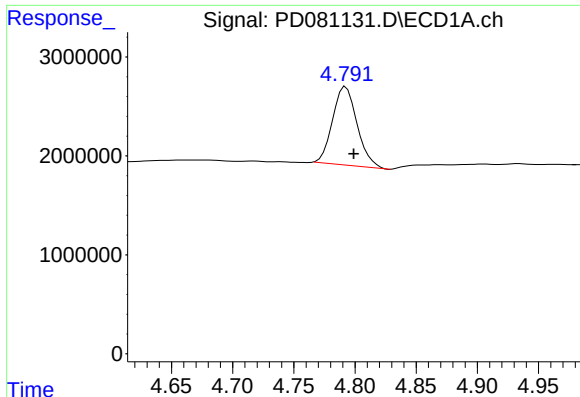

#7 delta-BHC


R.T.: 4.793 min
Delta R.T.: -0.006 min
Response: 11043994
Conc: 4.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-3-2-4

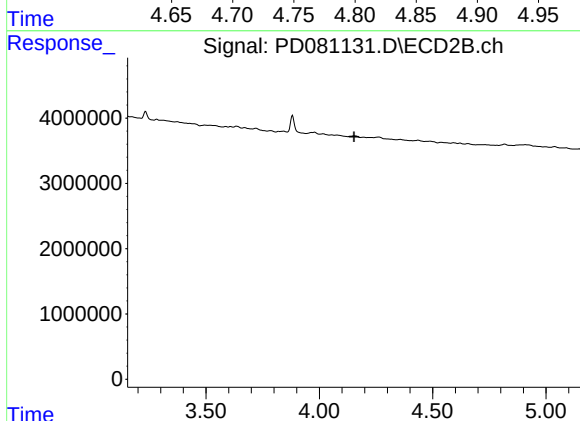


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.153 min
Response: 0
Conc: N.D.

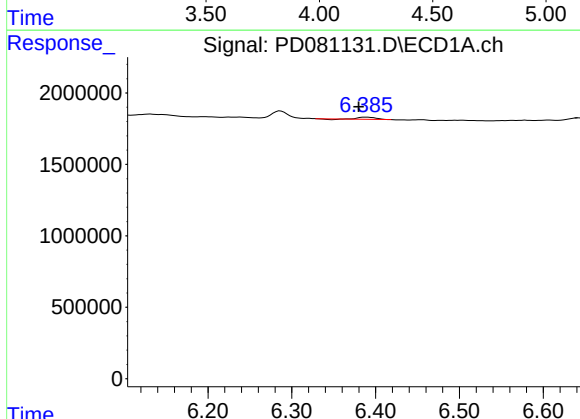


#13 Dieldrin

R.T.: 6.388 min
Delta R.T.: 0.008 min
Response: 176066
Conc: 0.08 ng/ml

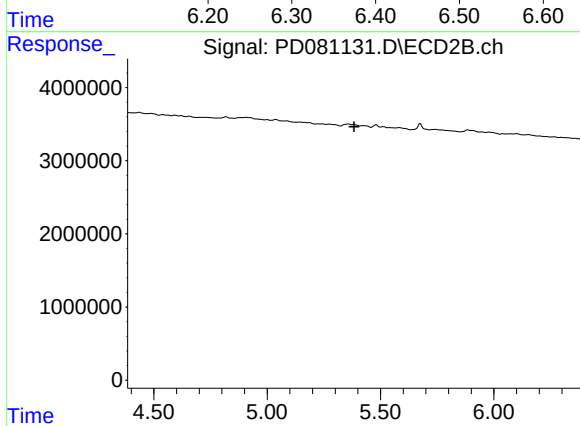

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 5.384 min
Response: 0
Conc: N.D.

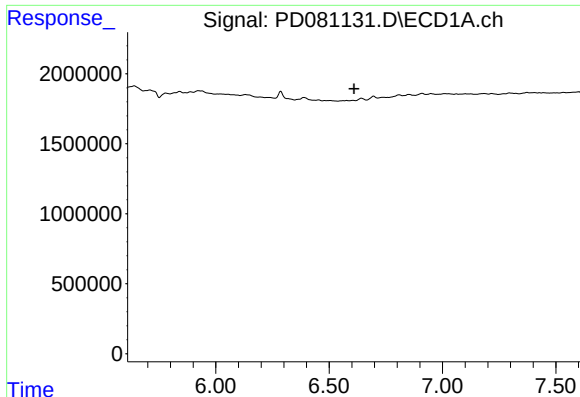

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.610 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
EB-3-2-4

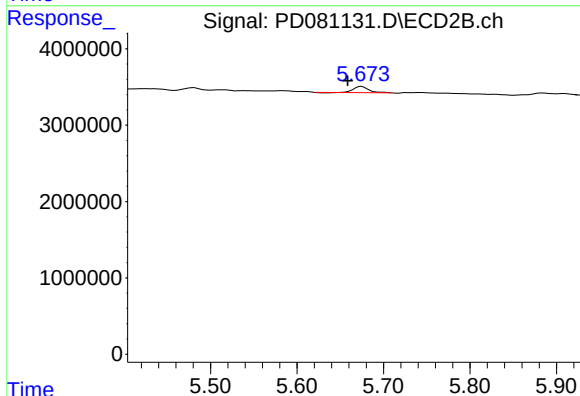


#14 Endrin

R.T.: 5.675 min
Delta R.T.: 0.016 min
Response: 970761
Conc: 0.33 ng/ml

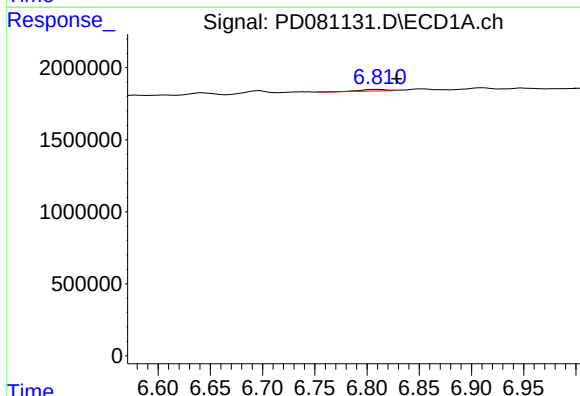


#15 Endosulfan II

R.T.: 6.809 min
Delta R.T.: -0.019 min
Response: 162431
Conc: 0.08 ng/ml

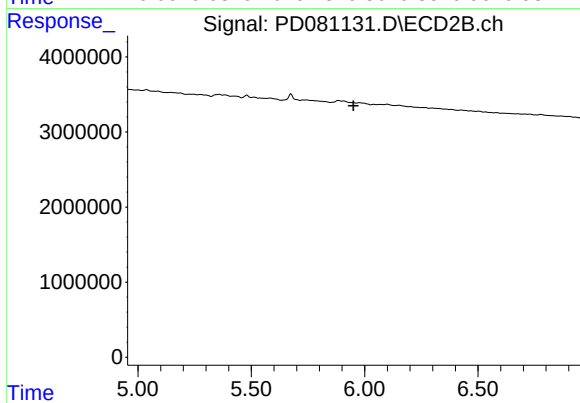

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.951 min
Response: 0
Conc: N.D.

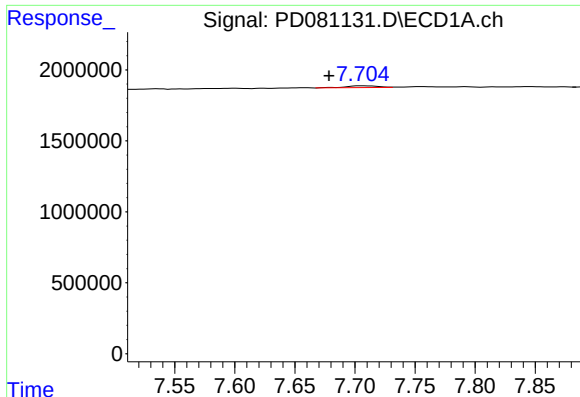

#21 Endrin ketone


R.T.: 7.706 min
Delta R.T.: 0.028 min
Response: 243935
Conc: 0.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-3-2-4

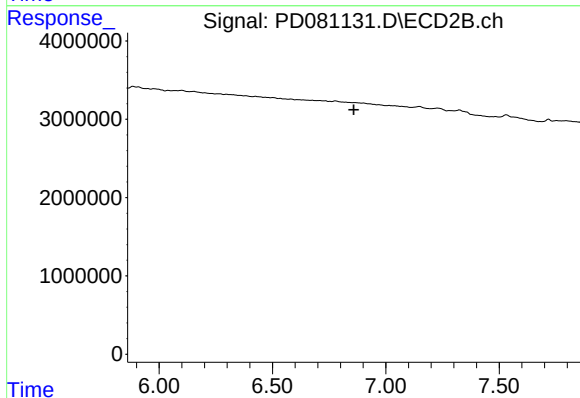


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.859 min
Response: 0
Conc: N.D.

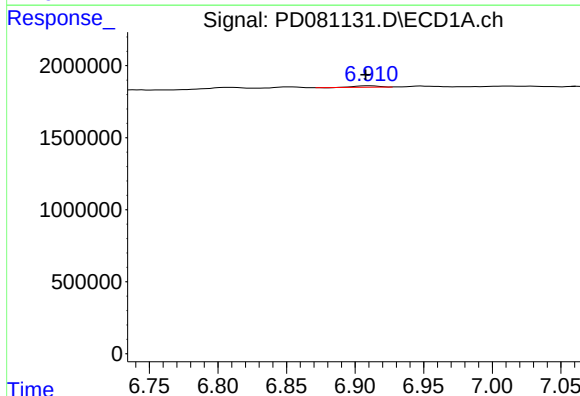


#27 Chlordane-5

R.T.: 6.911 min
Delta R.T.: 0.003 min
Response: 111831
Conc: 1.60 ng/ml

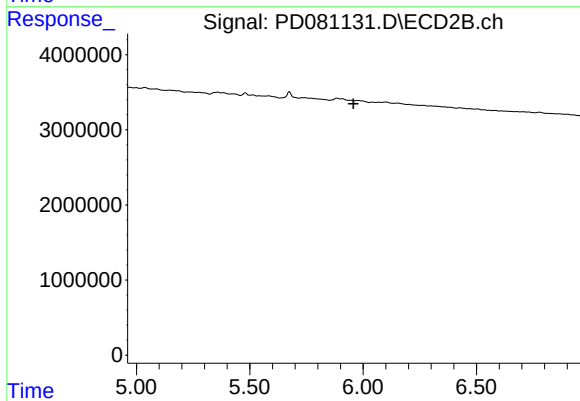

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 5.957 min
Response: 0
Conc: N.D.

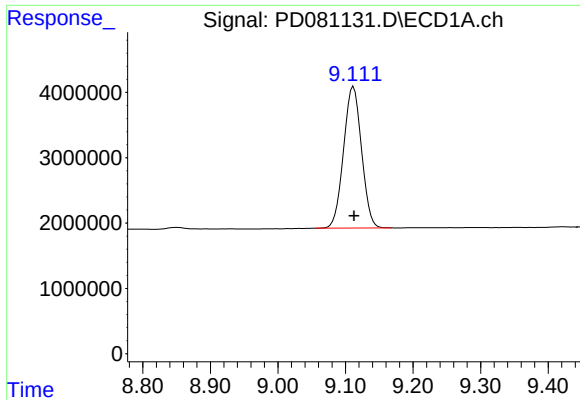

#28 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: -0.001 min
Response: 39914635
Conc: 19.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-3-2-4

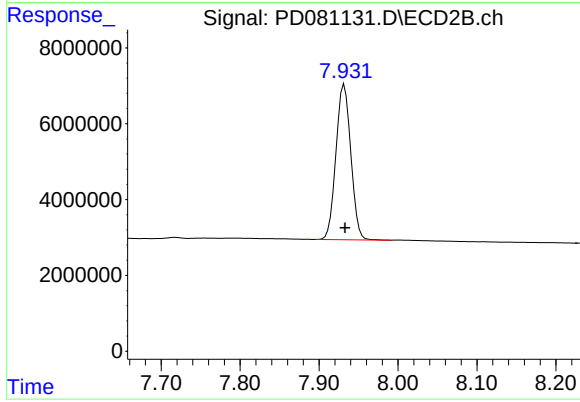

#28 Decachlorobiphenyl

R.T.: 7.932 min
Delta R.T.: -0.001 min
Response: 53559322
Conc: 20.11 ng/ml