

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020624\
 Data File : PD081135.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2024 18:53
 Operator : AR\AJ
 Sample : P1366-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EB-2-6-8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 21:09:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.796	27223184	45907897	19.177	19.191
28)	SA Decachlor...	9.112	7.932	40441808	52841194	20.096	19.838
Target Compounds							
3)	MA gamma-BHC...	0.000	3.636	0	275871	N.D.	0.074 #
4)	MA Heptachlor	4.934	0.000	440542	0	0.179	N.D. #
5)	MB Aldrin	0.000	4.267f	0	286179	N.D.	0.079 #
7)	B delta-BHC	4.793	0.000	12833511	0	5.115	N.D. #
9)	A Endosulfan I	6.127f	5.093f	97291	288422	0.047	0.094 #
11)	B alpha-Chl...	0.000	5.039f	0	272958	N.D.	0.083 #
14)	MA Endrin	0.000	5.675f	0	377668	N.D.	0.127 #
26)	Chlordane-4	0.000	5.039f	0	272958	N.D.	0.859 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020624\
Data File : PD081135.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2024 18:53
Operator : AR\AJ
Sample : P1366-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
EB-2-6-8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 21:09:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

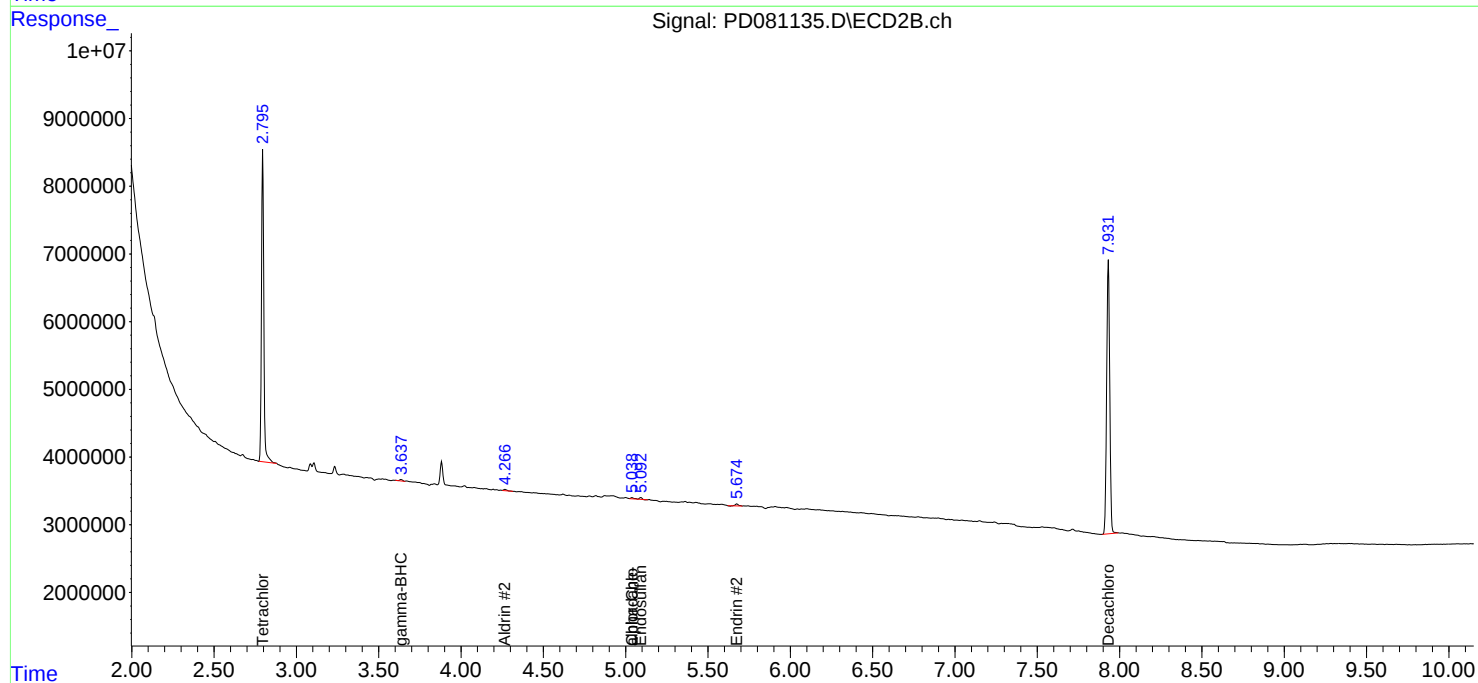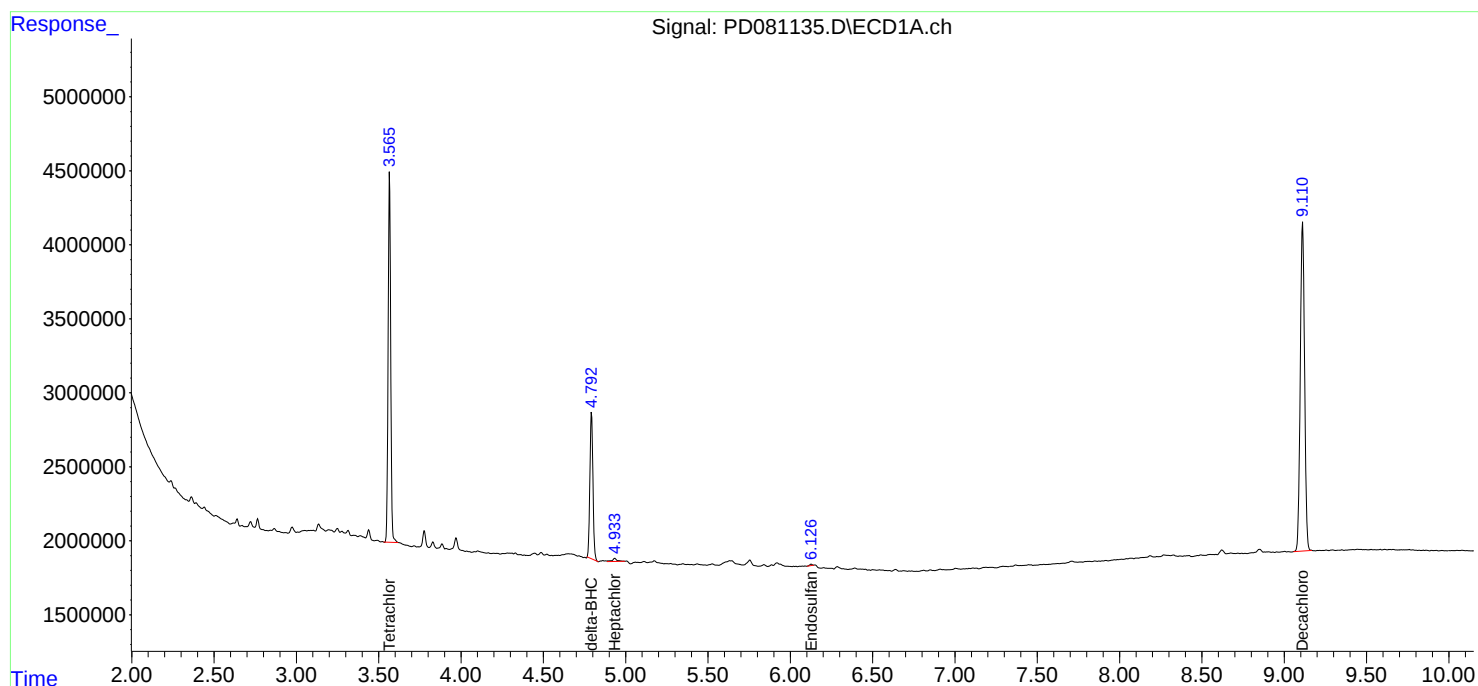


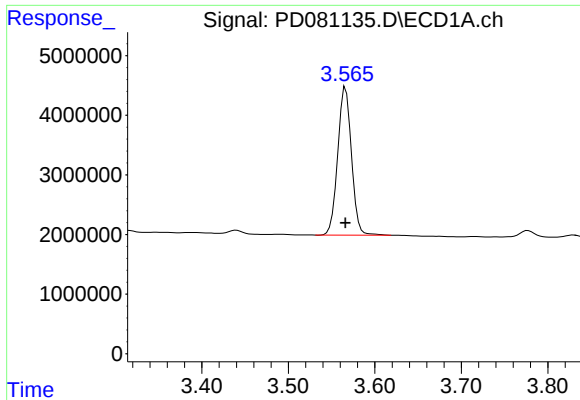

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 27223184
Conc: 19.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-2-6-8

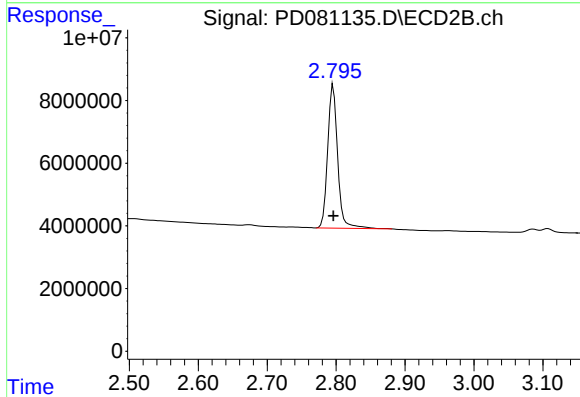


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 45907897
Conc: 19.19 ng/ml

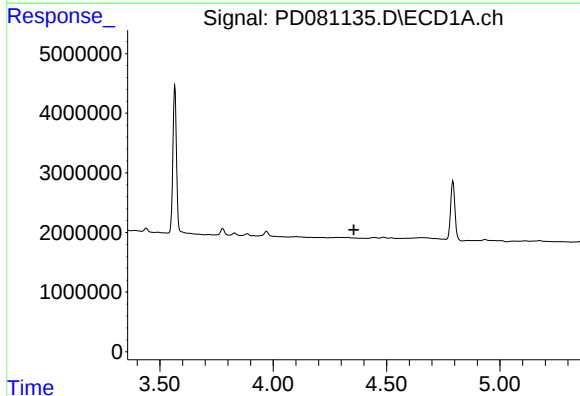


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.355 min
Response: 0
Conc: N.D.

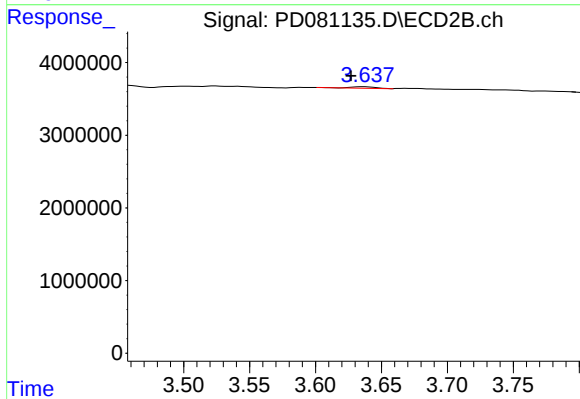

#3 gamma-BHC (Lindane)


R.T.: 3.636 min
Delta R.T.: 0.009 min
Response: 275871
Conc: 0.07 ng/ml

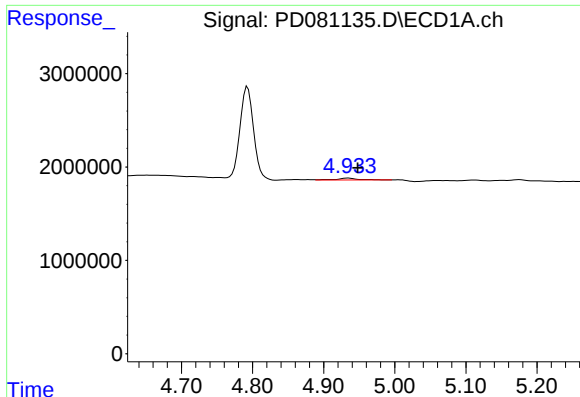

#4 Heptachlor


R.T.: 4.934 min
Delta R.T.: -0.014 min
Response: 440542
Conc: 0.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-2-6-8

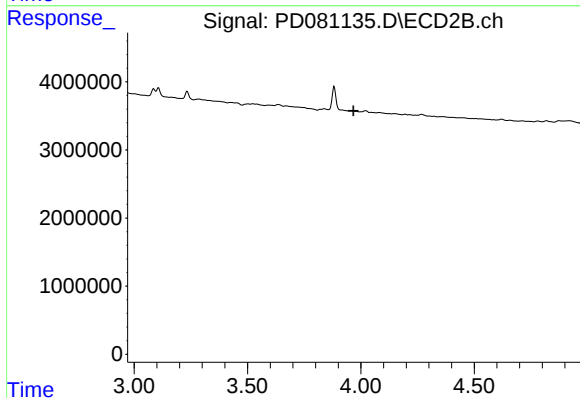


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 3.968 min
Response: 0
Conc: N.D.

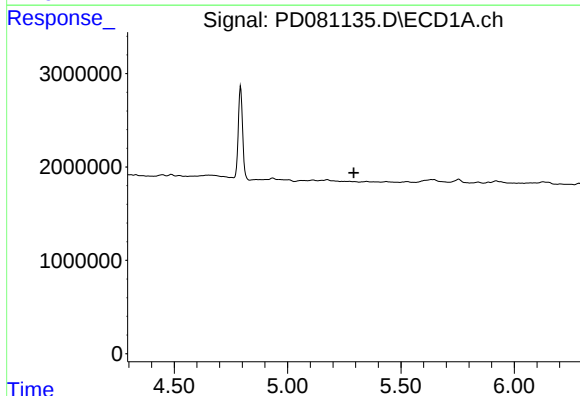


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.292 min
Response: 0
Conc: N.D.

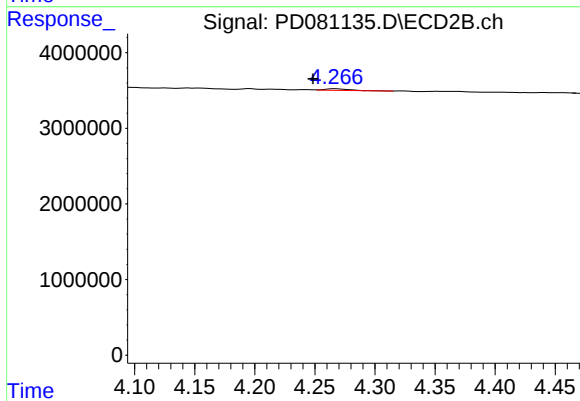

#5 Aldrin


R.T.: 4.267 min
Delta R.T.: 0.019 min
Response: 286179
Conc: 0.08 ng/ml

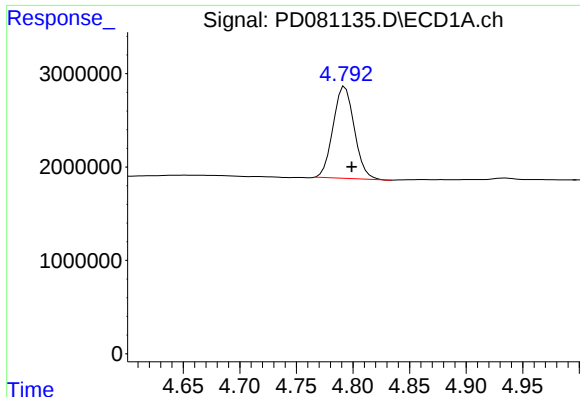

#7 delta-BHC


R.T.: 4.793 min
Delta R.T.: -0.006 min
Response: 12833511
Conc: 5.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-2-6-8

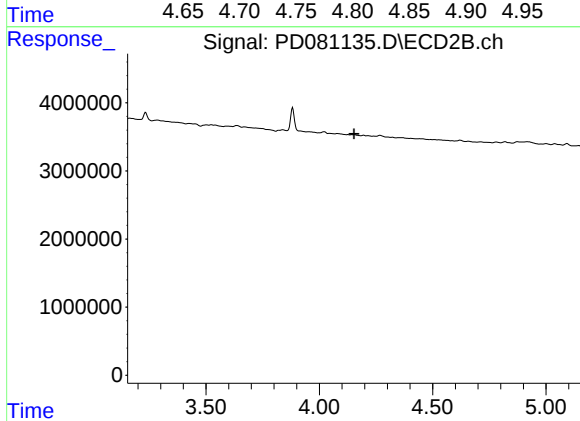


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.153 min
Response: 0
Conc: N.D.

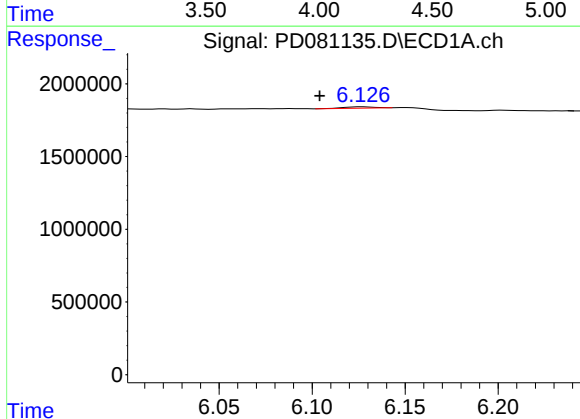


#9 Endosulfan I

R.T.: 6.127 min
Delta R.T.: 0.023 min
Response: 97291
Conc: 0.05 ng/ml

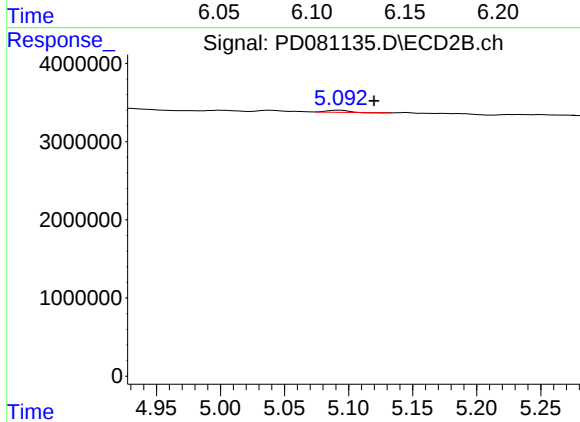

#9 Endosulfan I


R.T.: 5.093 min
Delta R.T.: -0.027 min
Response: 288422
Conc: 0.09 ng/ml

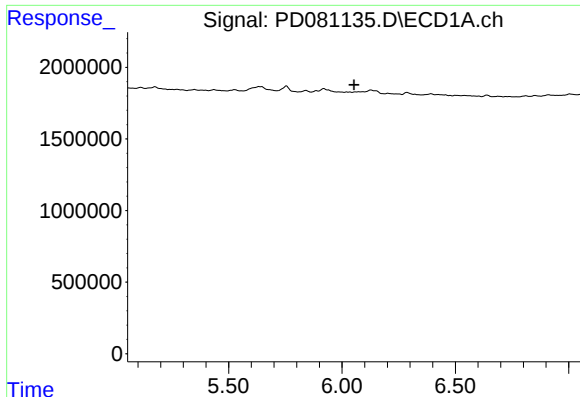

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.053 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
EB-2-6-8

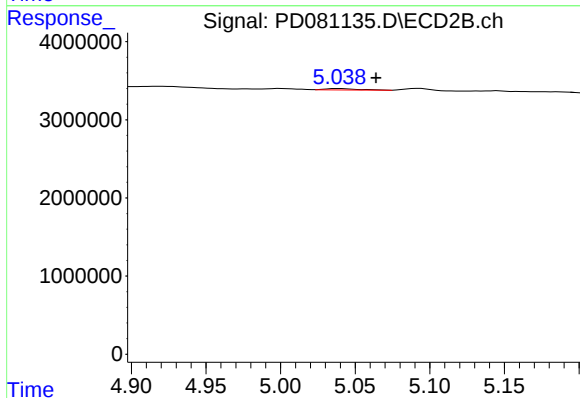


#11 alpha-Chlordane

R.T.: 5.039 min
Delta R.T.: -0.025 min
Response: 272958
Conc: 0.08 ng/ml

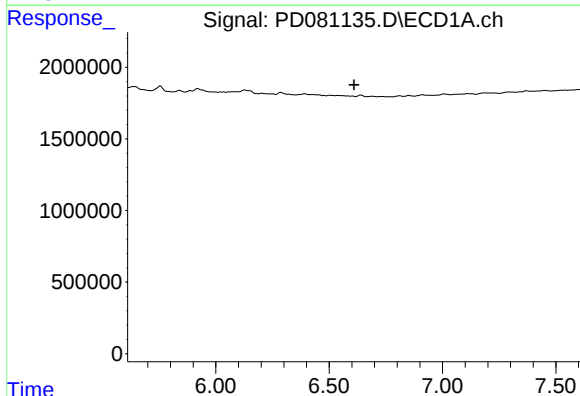


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.610 min
Response: 0
Conc: N.D.

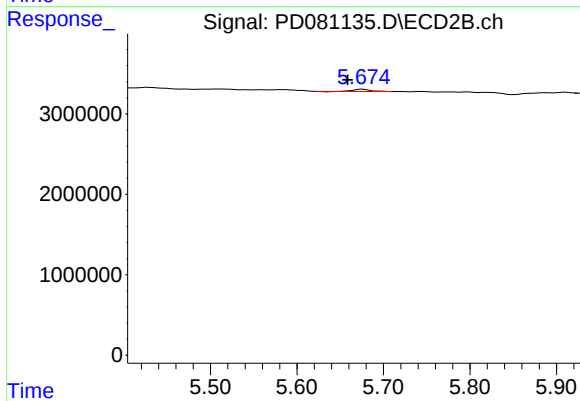

#14 Endrin


R.T.: 5.675 min
Delta R.T.: 0.017 min
Response: 377668
Conc: 0.13 ng/ml

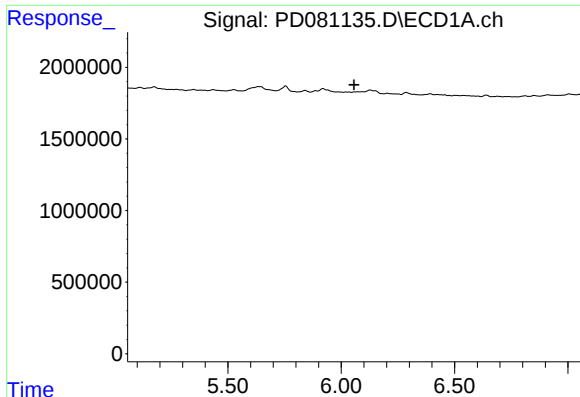

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 6.057 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
EB-2-6-8

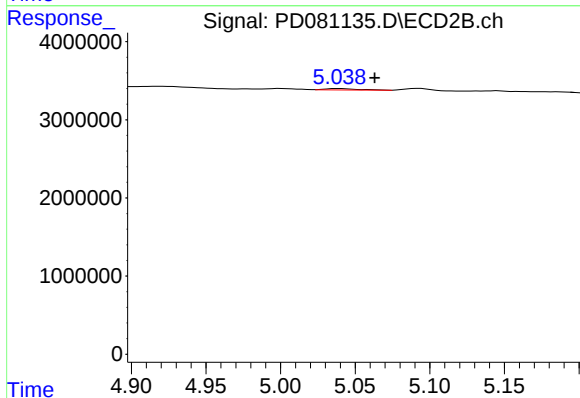


#26 Chlordane-4

R.T.: 5.039 min
Delta R.T.: -0.024 min
Response: 272958
Conc: 0.86 ng/ml

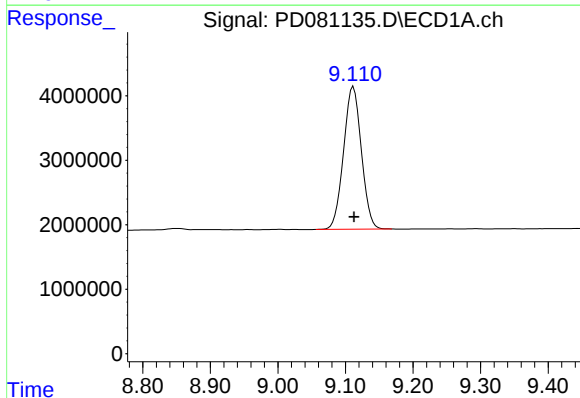

#28 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: -0.001 min
Response: 40441808
Conc: 20.10 ng/ml

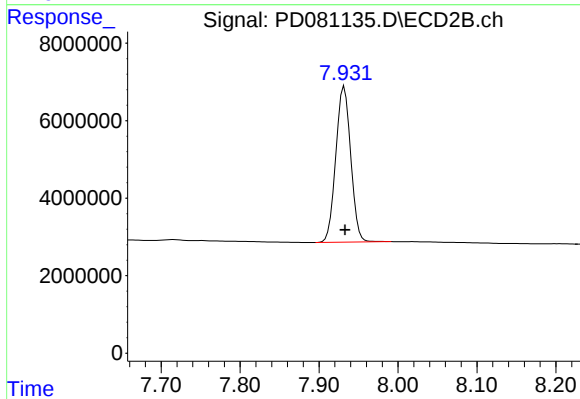

#28 Decachlorobiphenyl

R.T.: 7.932 min
Delta R.T.: 0.000 min
Response: 52841194
Conc: 19.84 ng/ml