

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020624\
 Data File : PD081140.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2024 20:00
 Operator : AR\AJ
 Sample : P1366-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EB-1-4-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 21:11:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.796	28676153	48174923	20.201	20.139
28)	SA Decachlor...	9.111	7.932	41750644	55102929	20.746	20.687
Target Compounds							
4)	MA Heptachlor	4.933	0.000	155029	0	0.063	N.D. #
7)	B delta-BHC	4.793	0.000	9293255	0	3.704	N.D. #
10)	B gamma-Chl...	0.000	4.997	0	301537	N.D.	0.092 #
11)	B alpha-Chl...	0.000	5.040f	0	1187929	N.D.	0.363 #
14)	MA Endrin	0.000	5.673	0	300018	N.D.	0.101 #
15)	B Endosulfa...	6.852f	5.979f	328186	463161	0.169	0.161
21)	B Endrin ke...	7.709f	0.000	272181	0	0.130	N.D. #
25)	Chlordane-3	0.000	4.997	0	301537	N.D.	0.898 #
26)	Chlordane-4	0.000	5.040f	0	1187929	N.D.	3.739 #
27)	Chlordane-5	0.000	5.979f	0	463161	N.D.	3.820 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020624\
Data File : PD081140.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2024 20:00
Operator : AR\AJ
Sample : P1366-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
EB-1-4-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 21:11:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

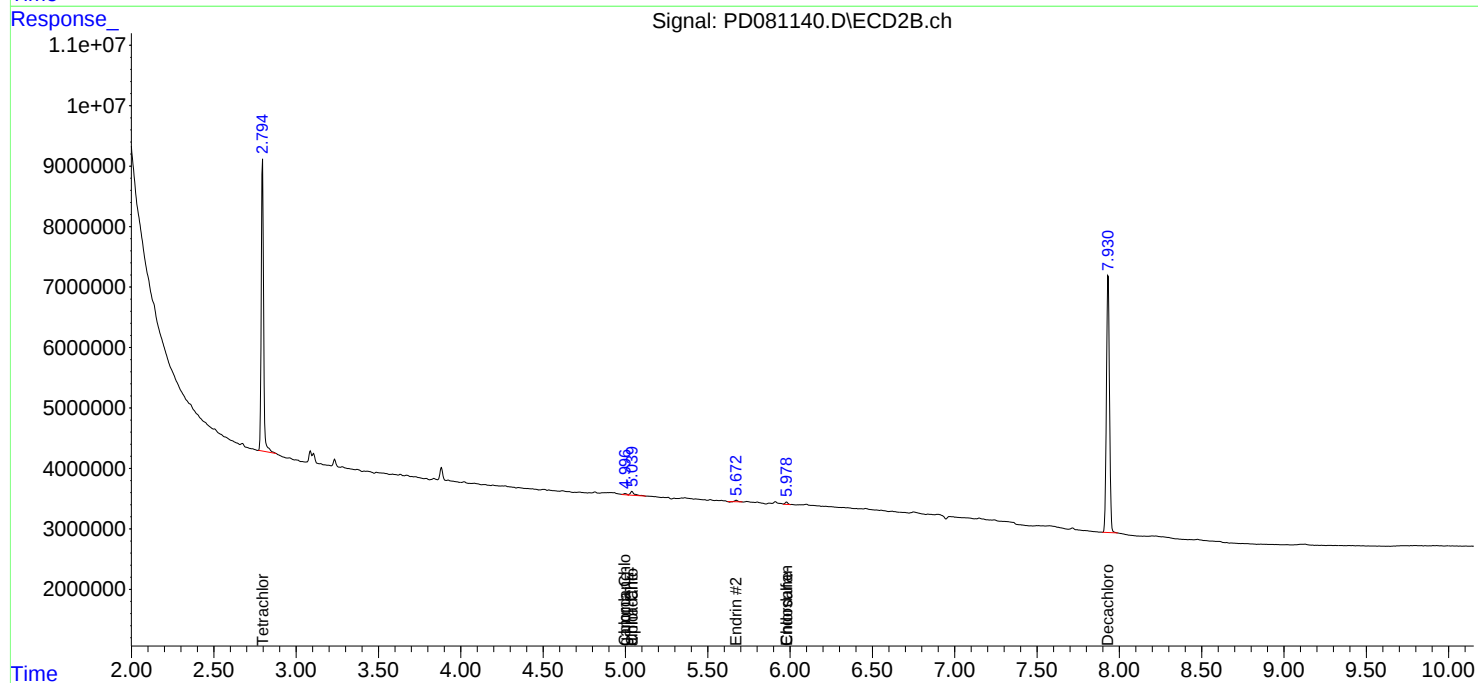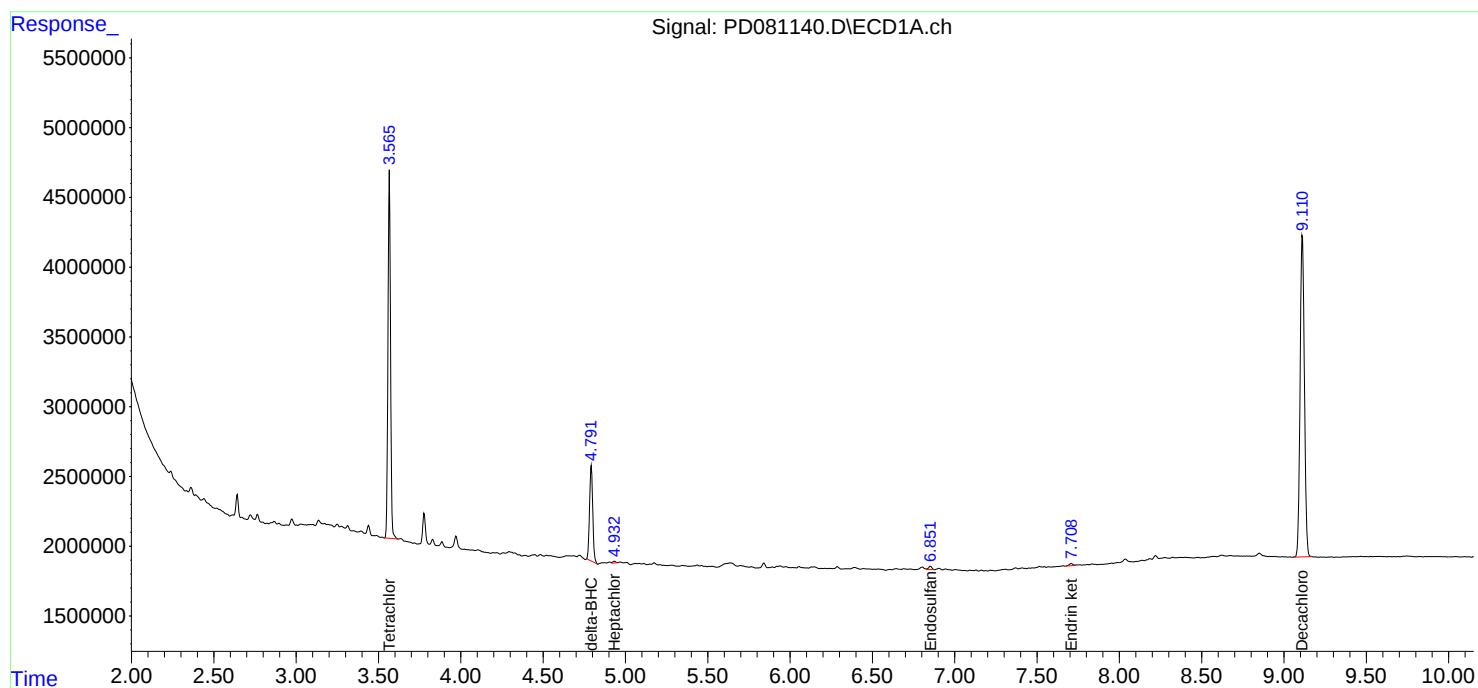


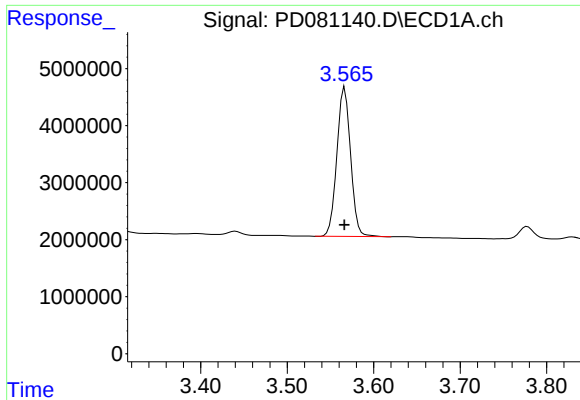

#1 Tetrachloro-m-xylene


R.T.: 3.567 min
Delta R.T.: 0.000 min
Response: 28676153
Conc: 20.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-1-4-6

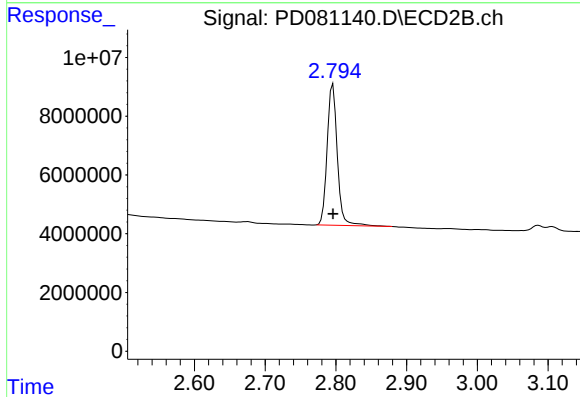


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 48174923
Conc: 20.14 ng/ml

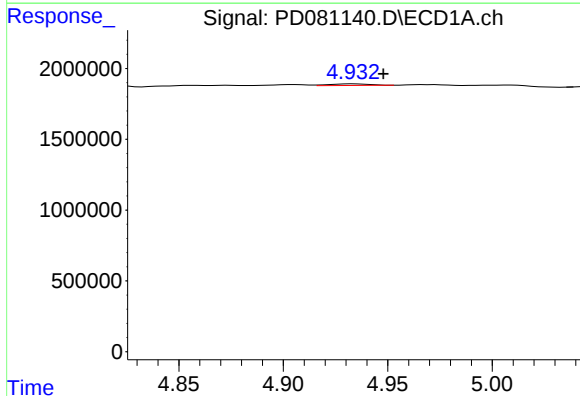


#4 Heptachlor

R.T.: 4.933 min
Delta R.T.: -0.014 min
Response: 155029
Conc: 0.06 ng/ml

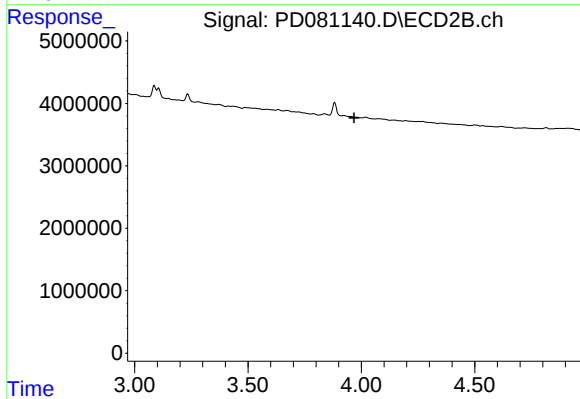

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 3.968 min
Response: 0
Conc: N.D.

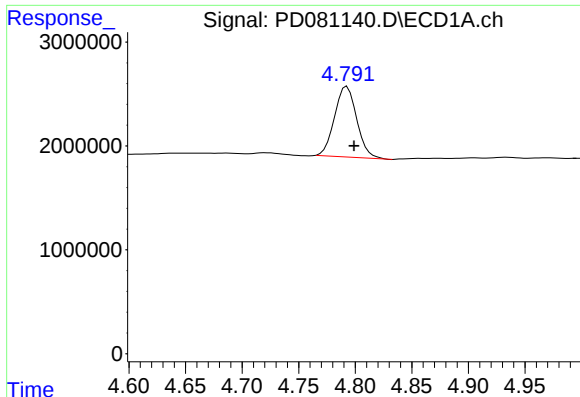

#7 delta-BHC


R.T.: 4.793 min
Delta R.T.: -0.006 min
Response: 9293255
Conc: 3.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-1-4-6

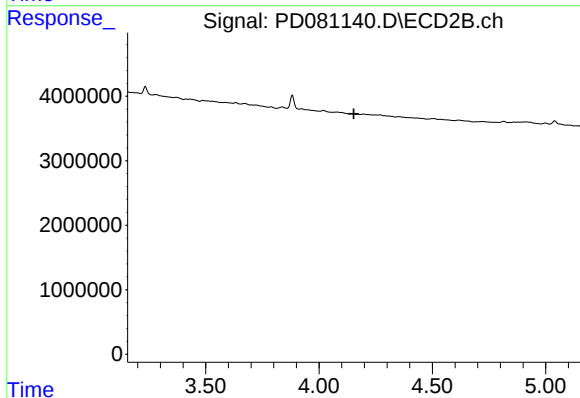


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.153 min
Response: 0
Conc: N.D.

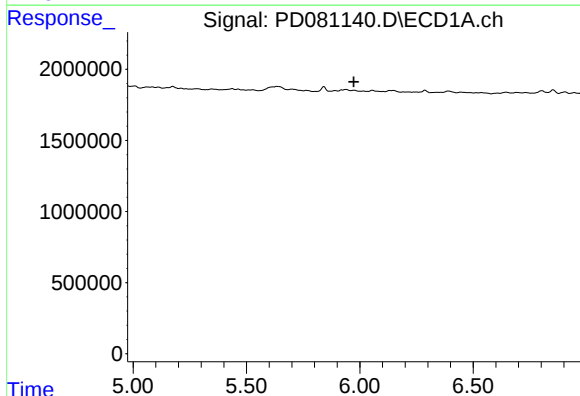


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.974 min
Response: 0
Conc: N.D.

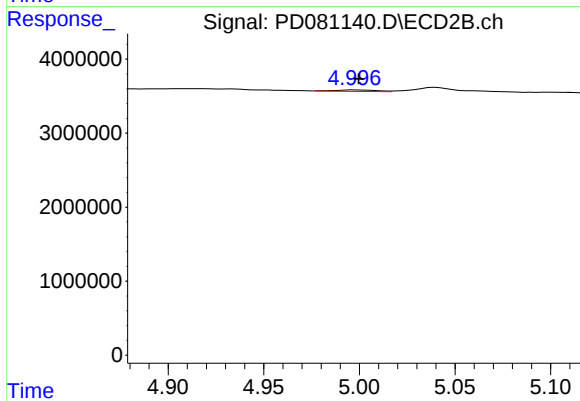

#10 gamma-Chlordane


R.T.: 4.997 min
Delta R.T.: -0.002 min
Response: 301537
Conc: 0.09 ng/ml

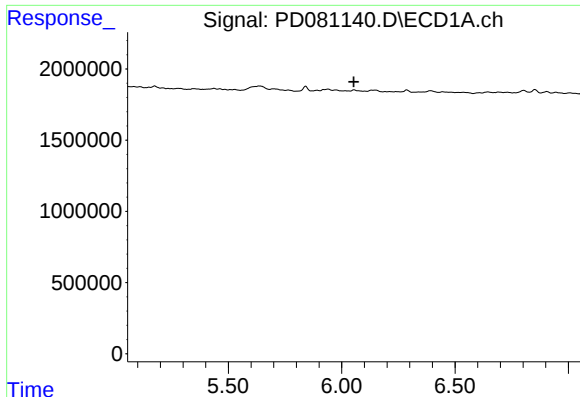

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.053 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
EB-1-4-6

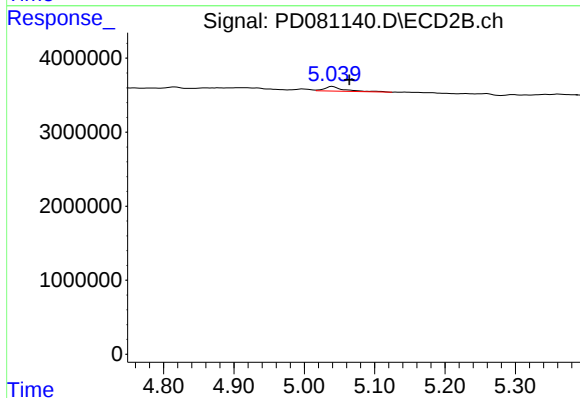


#11 alpha-Chlordane

R.T.: 5.040 min
Delta R.T.: -0.024 min
Response: 1187929
Conc: 0.36 ng/ml

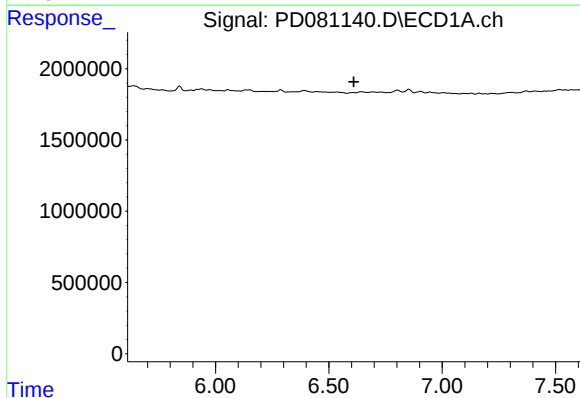


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.610 min
Response: 0
Conc: N.D.

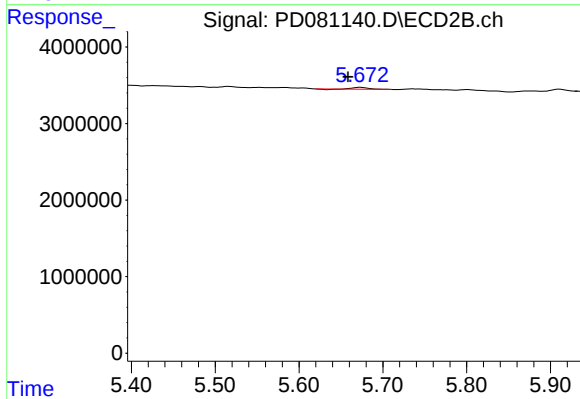

#14 Endrin


R.T.: 5.673 min
Delta R.T.: 0.015 min
Response: 300018
Conc: 0.10 ng/ml

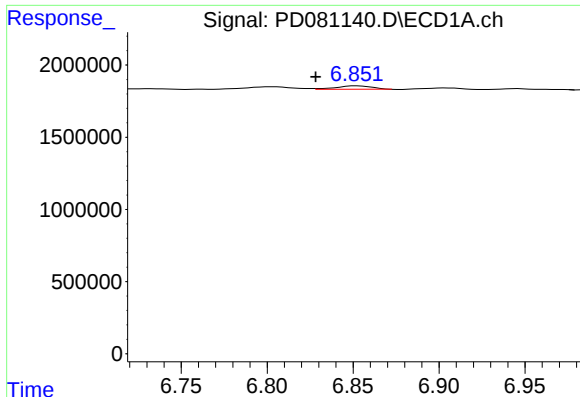

#15 Endosulfan II


R.T.: 6.852 min
Delta R.T.: 0.024 min
Response: 328186
Conc: 0.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-1-4-6

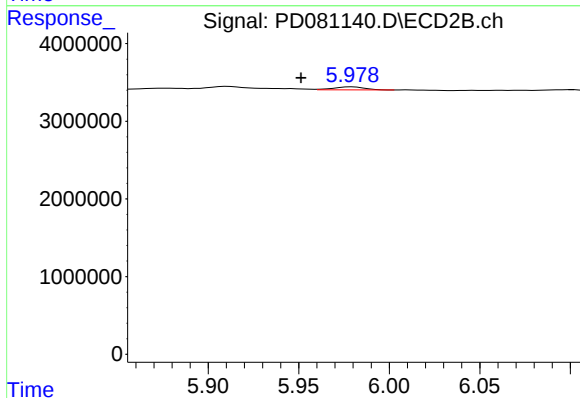


#15 Endosulfan II

R.T.: 5.979 min
Delta R.T.: 0.028 min
Response: 463161
Conc: 0.16 ng/ml

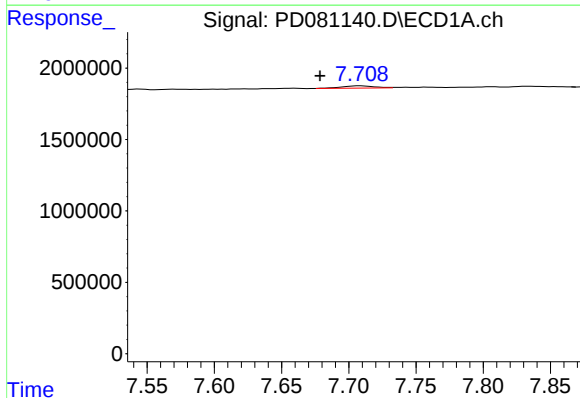


#21 Endrin ketone

R.T.: 7.709 min
Delta R.T.: 0.030 min
Response: 272181
Conc: 0.13 ng/ml

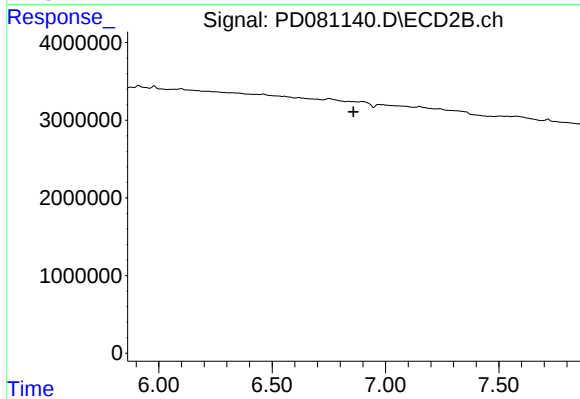

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.859 min
Response: 0
Conc: N.D.

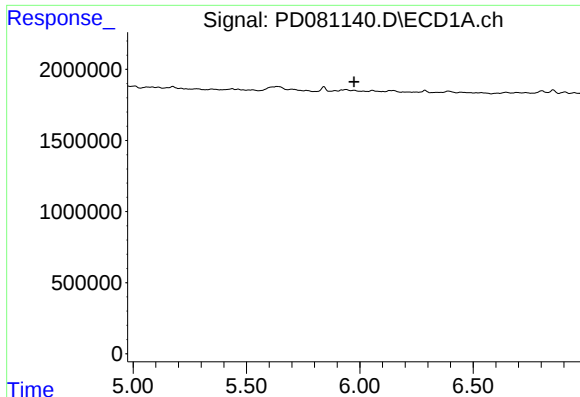

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.974 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
EB-1-4-6

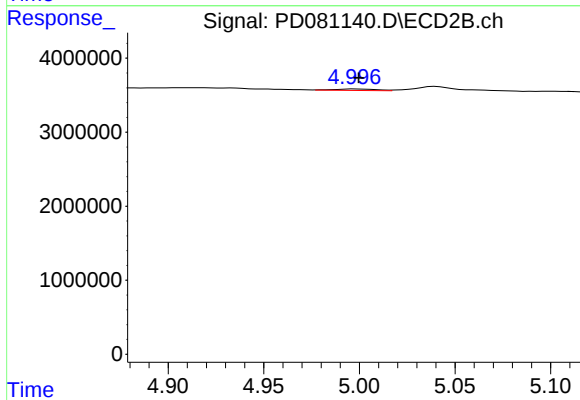


#25 Chlordane-3

R.T.: 4.997 min
Delta R.T.: -0.002 min
Response: 301537
Conc: 0.90 ng/ml

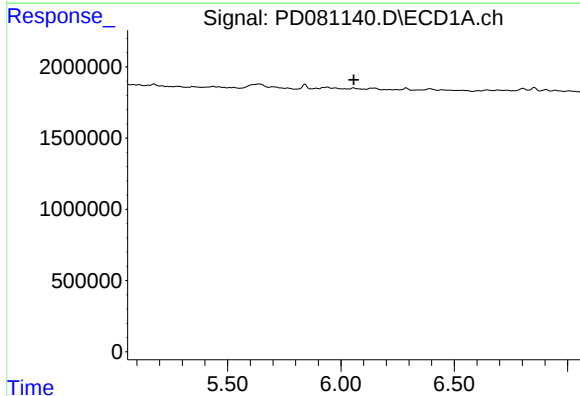


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.057 min
Response: 0
Conc: N.D.

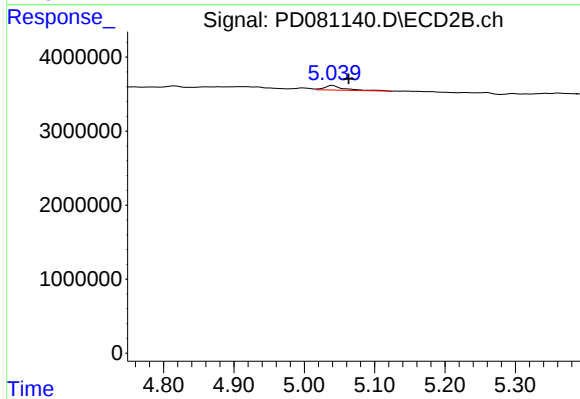

#26 Chlordane-4


R.T.: 5.040 min
Delta R.T.: -0.023 min
Response: 1187929
Conc: 3.74 ng/ml

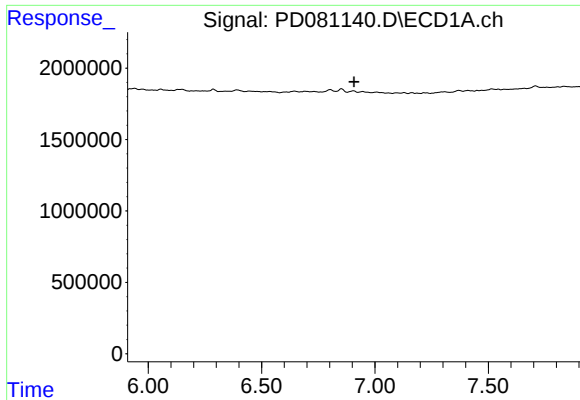

#27 Chlorodane-5


R.T.: 0.000 min
Exp R.T.: 6.908 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
EB-1-4-6

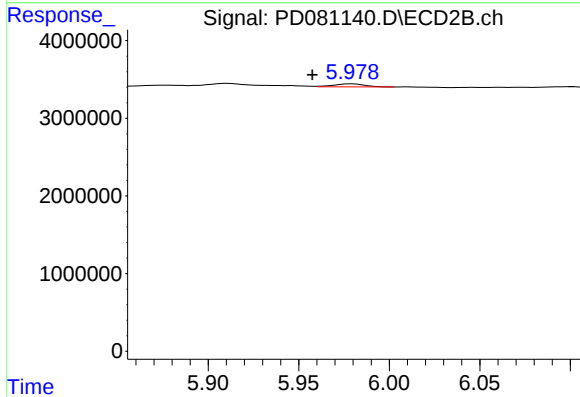


#27 Chlorodane-5

R.T.: 5.979 min
Delta R.T.: 0.022 min
Response: 463161
Conc: 3.82 ng/ml

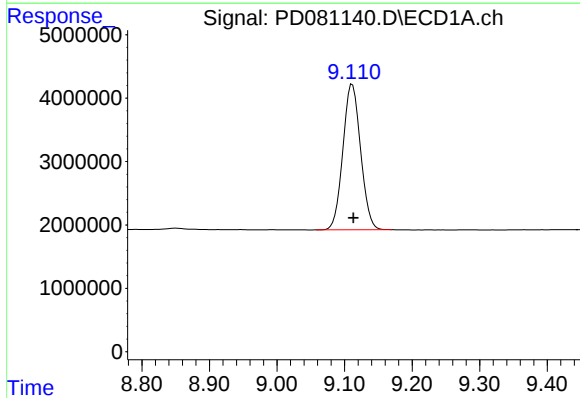

#28 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: -0.002 min
Response: 41750644
Conc: 20.75 ng/ml

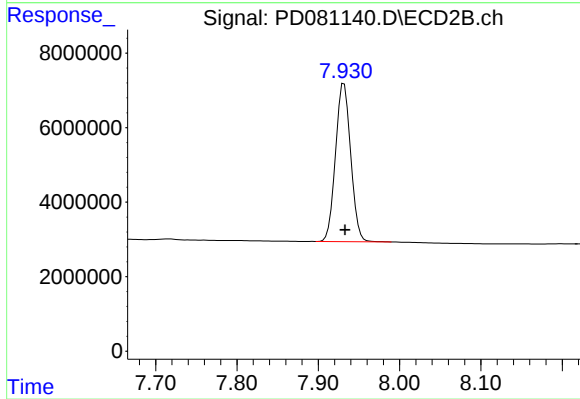

#28 Decachlorobiphenyl

R.T.: 7.932 min
Delta R.T.: -0.001 min
Response: 55102929
Conc: 20.69 ng/ml