

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020624\
 Data File : PD081141.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2024 20:13
 Operator : AR\AJ
 Sample : P1367-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EB-6-0-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 21:11:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.796	26921516	48909089	18.965	20.446
28)	SA Decachlor...	9.110	7.932	41109972	54633234	20.428	20.511
Target Compounds							
2)	A alpha-BHC	4.044f	0.000	117508	0	0.047	N.D. #
3)	MA gamma-BHC...	0.000	3.634	0	356328	N.D.	0.095 #
7)	B delta-BHC	4.793	0.000	6538130	0	2.606	N.D. #
10)	B gamma-Chl...	5.941f	0.000	263350	0	0.120	N.D. #
11)	B alpha-Chl...	0.000	5.037f	0	447934	N.D.	0.137 #
14)	MA Endrin	0.000	5.673	0	990535	N.D.	0.334 #
19)	B Endosulfa...	7.220f	0.000	152022	0	0.080	N.D. #
21)	B Endrin ke...	7.697f	0.000	280458	0	0.134	N.D. #
26)	Chlordane-4	0.000	5.037f	0	447934	N.D.	1.410 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020624\
Data File : PD081141.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2024 20:13
Operator : AR\AJ
Sample : P1367-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
EB-6-0-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 21:11:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

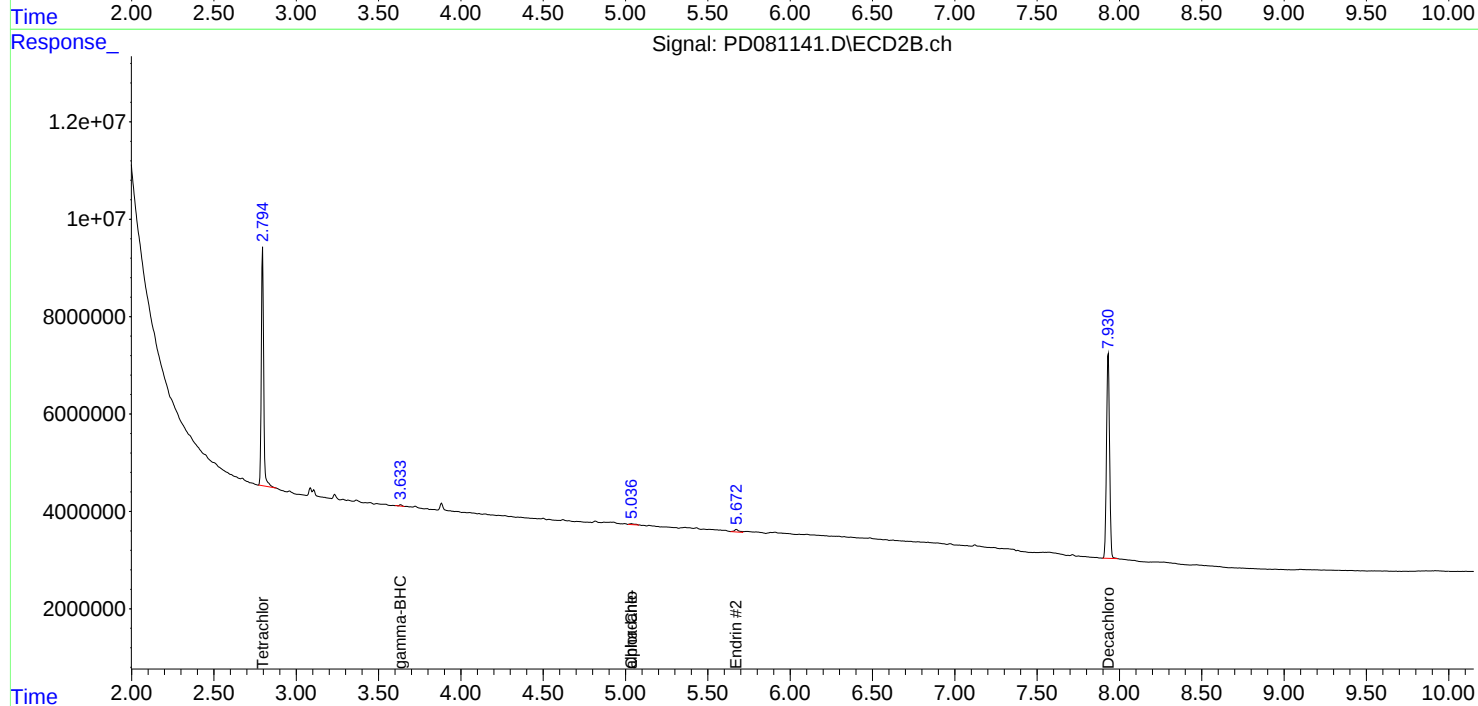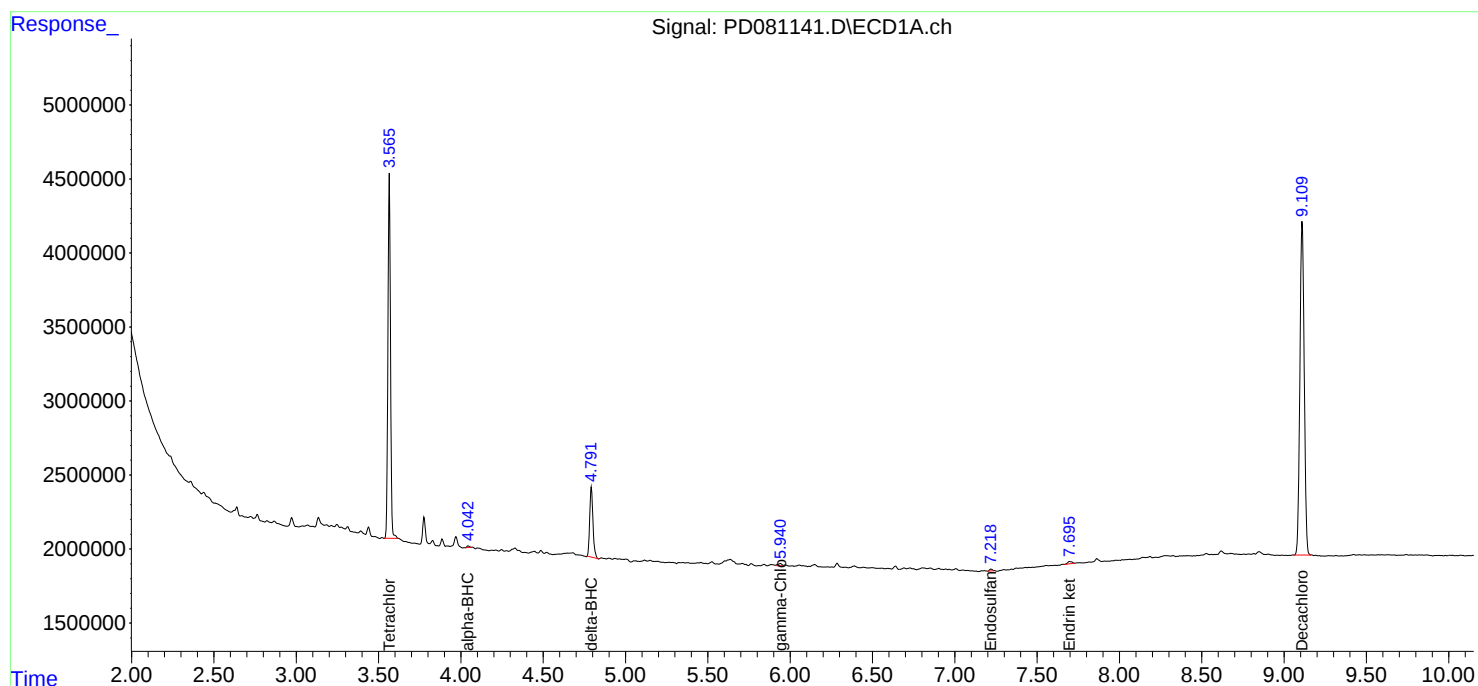


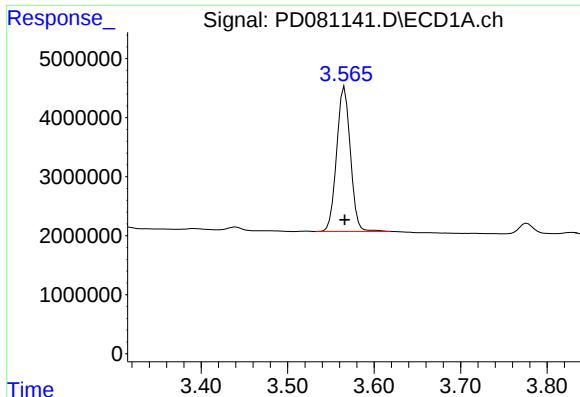

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 26921516
Conc: 18.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-6-0-2

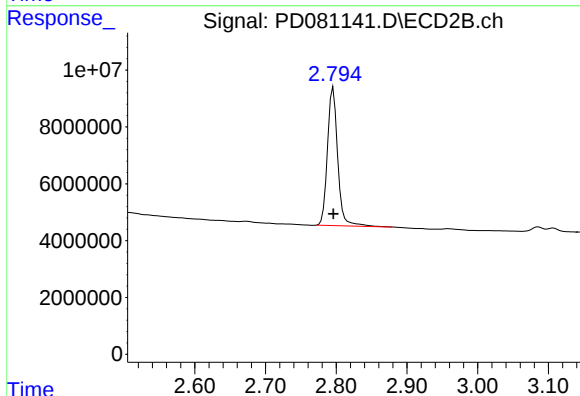


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 48909089
Conc: 20.45 ng/ml

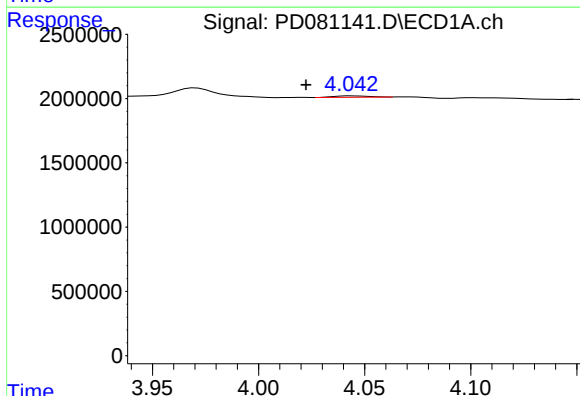


#2 alpha-BHC

R.T.: 4.044 min
Delta R.T.: 0.022 min
Response: 117508
Conc: 0.05 ng/ml

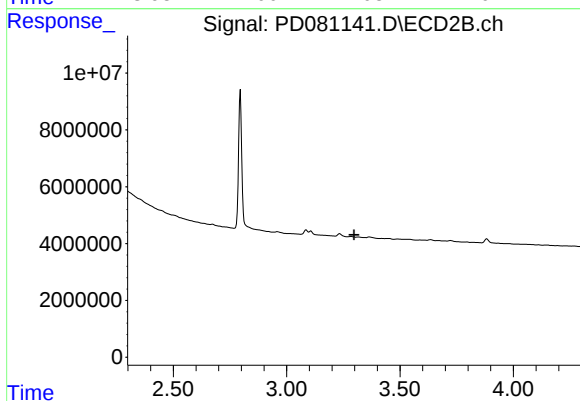

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 3.298 min
Response: 0
Conc: N.D.

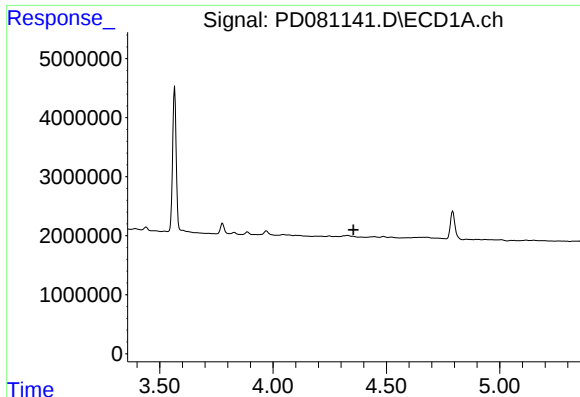

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.355 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
EB-6-0-2

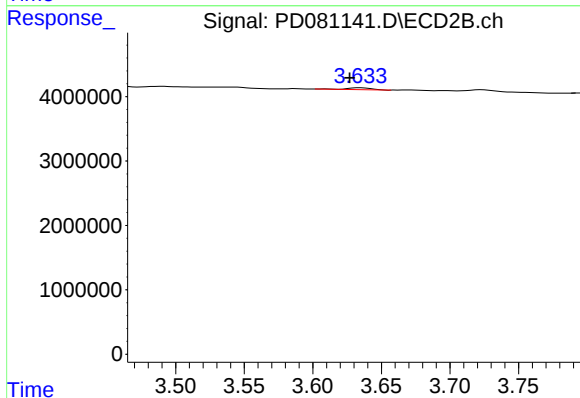


#3 gamma-BHC (Lindane)

R.T.: 3.634 min
Delta R.T.: 0.007 min
Response: 356328
Conc: 0.10 ng/ml

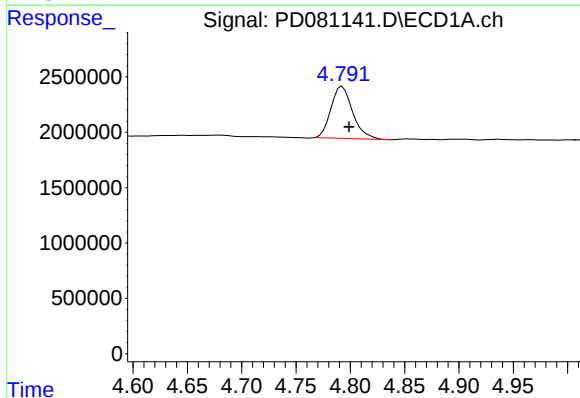


#7 delta-BHC

R.T.: 4.793 min
Delta R.T.: -0.006 min
Response: 6538130
Conc: 2.61 ng/ml

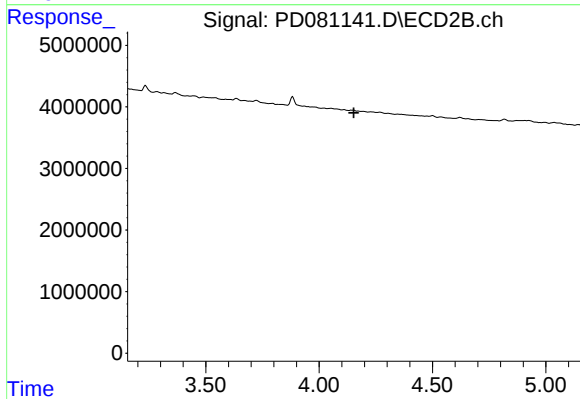

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.153 min
Response: 0
Conc: N.D.

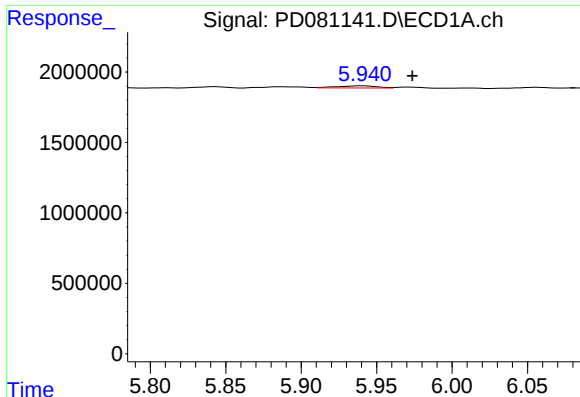

#10 gamma-Chlordane


R.T.: 5.941 min
Delta R.T.: -0.032 min
Response: 263350
Conc: 0.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-6-0-2

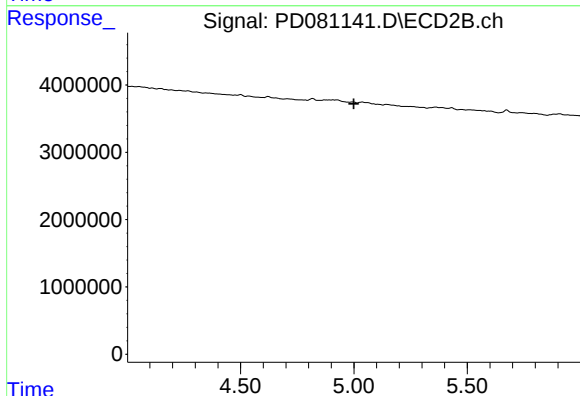


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.000 min
Response: 0
Conc: N.D.

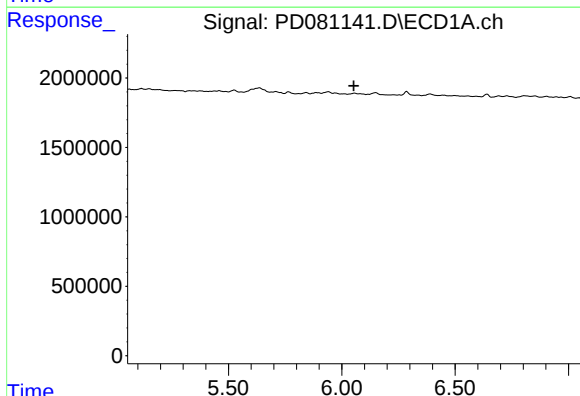


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.053 min
Response: 0
Conc: N.D.

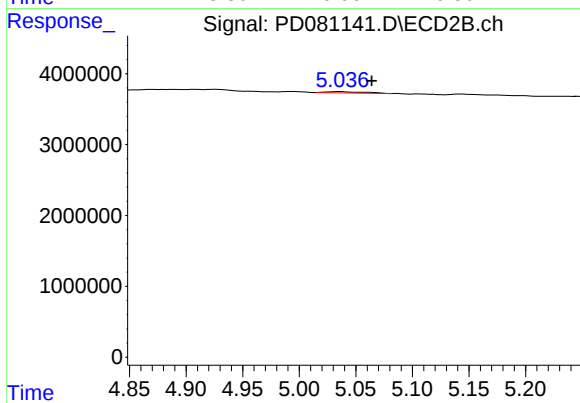

#11 alpha-Chlordane


R.T.: 5.037 min
Delta R.T.: -0.027 min
Response: 447934
Conc: 0.14 ng/ml

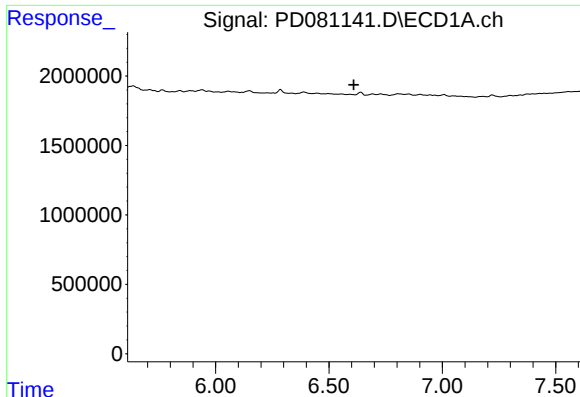

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.610 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
EB-6-0-2

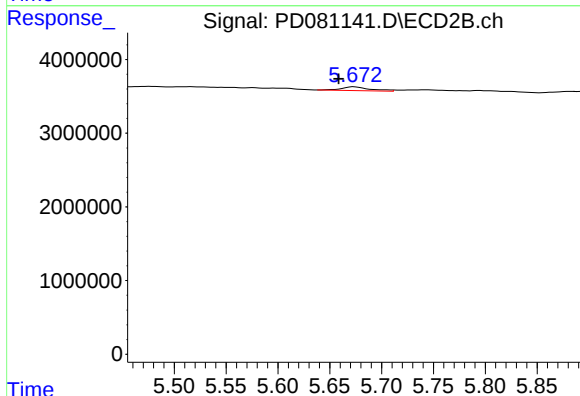


#14 Endrin

R.T.: 5.673 min
Delta R.T.: 0.015 min
Response: 990535
Conc: 0.33 ng/ml

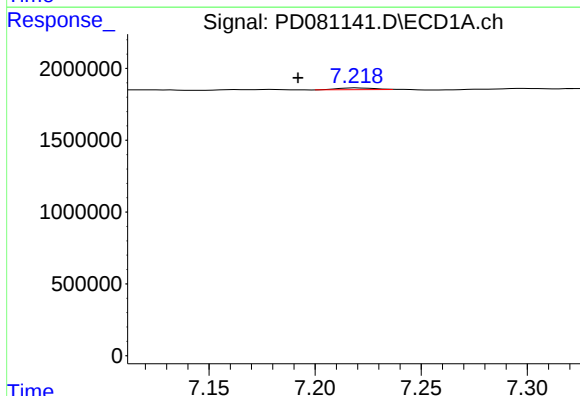


#19 Endosulfan Sulfate

R.T.: 7.220 min
Delta R.T.: 0.028 min
Response: 152022
Conc: 0.08 ng/ml

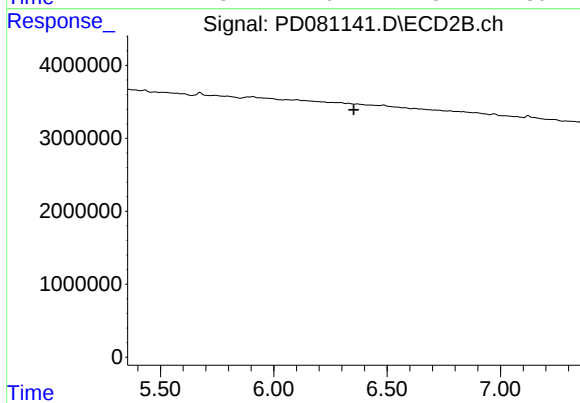

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.353 min
Response: 0
Conc: N.D.

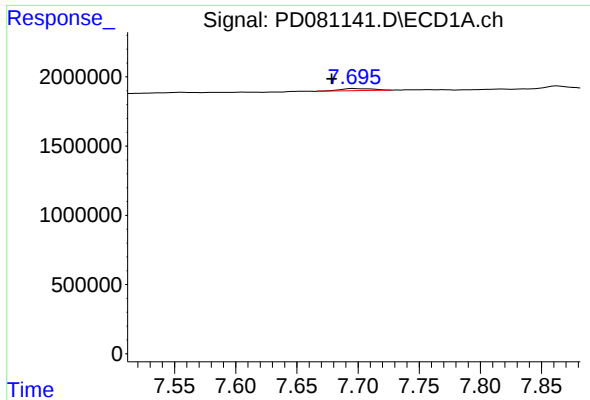

#21 Endrin ketone


R.T.: 7.697 min
Delta R.T.: 0.018 min
Response: 280458
Conc: 0.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-6-0-2

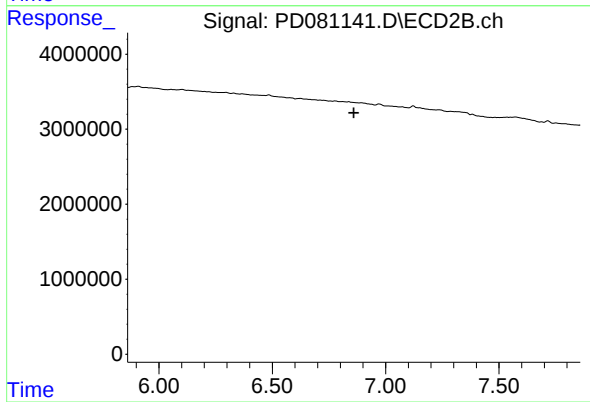


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.859 min
Response: 0
Conc: N.D.

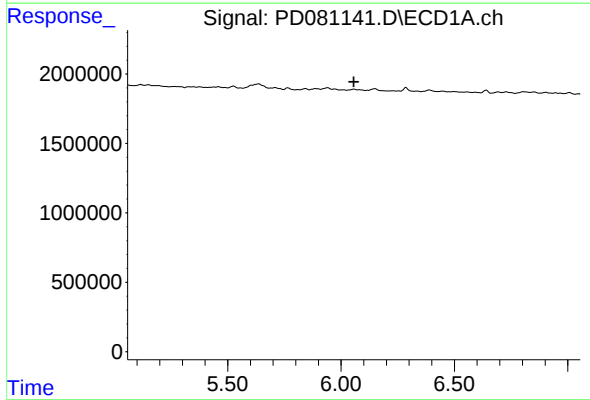


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.057 min
Response: 0
Conc: N.D.

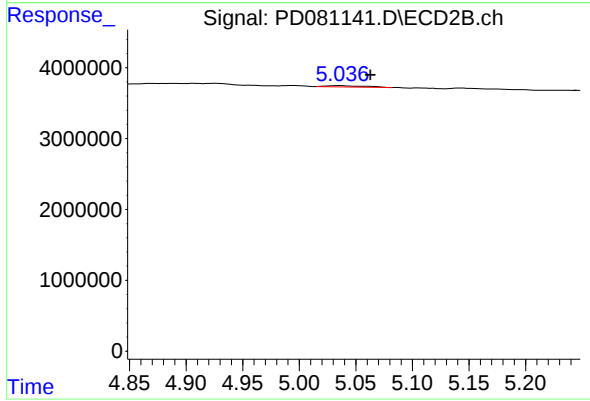

#26 Chlordane-4


R.T.: 5.037 min
Delta R.T.: -0.026 min
Response: 447934
Conc: 1.41 ng/ml

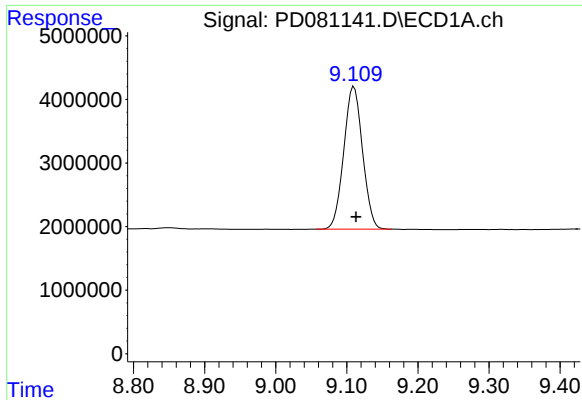

#28 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: -0.003 min
Response: 41109972
Conc: 20.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-6-0-2

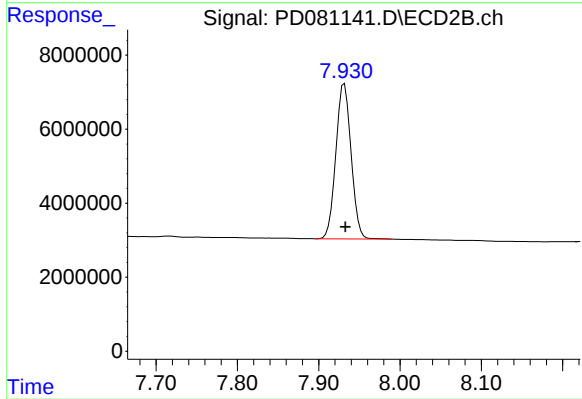

#28 Decachlorobiphenyl

R.T.: 7.932 min
Delta R.T.: -0.001 min
Response: 54633234
Conc: 20.51 ng/ml