

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020624\
 Data File : PD081142.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2024 20:27
 Operator : AR\AJ
 Sample : P1367-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EB-7-0-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 00:06:43 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.796	29877798	50704445	21.047	21.196
28)	SA Decachlor...	9.111	7.932	41277330	54710756	20.511	20.540
Target Compounds							
2)	A alpha-BHC	4.046f	3.286	814519	646057	0.328	0.168 #
3)	MA gamma-BHC...	4.351	3.633	77529	683585	0.032	0.183 #
4)	MA Heptachlor	4.972f	3.960	284021	545819	0.115	0.158 #
7)	B delta-BHC	4.793	0.000	2146186	0	0.855	N.D. #
9)	A Endosulfan I	6.106	5.147f	175221	369051	0.084	0.120 #
11)	B alpha-Chl...	0.000	5.039f	0	279547	N.D.	0.086 #
13)	MA Dieldrin	6.368	5.390	261526	229471	0.118	0.067 #
14)	MA Endrin	6.639f	5.674f	147021	724812	0.079	0.245 #
15)	B Endosulfa...	6.803f	0.000	173134	0	0.089	N.D. #
21)	B Endrin ke...	7.709f	0.000	102949	0	0.049	N.D. #
26)	Chlordane-4	0.000	5.039f	0	279547	N.D.	0.880 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD020624\
Data File : PD081142.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2024 20:27
Operator : AR\AJ
Sample : P1367-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
EB-7-0-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 00:06:43 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

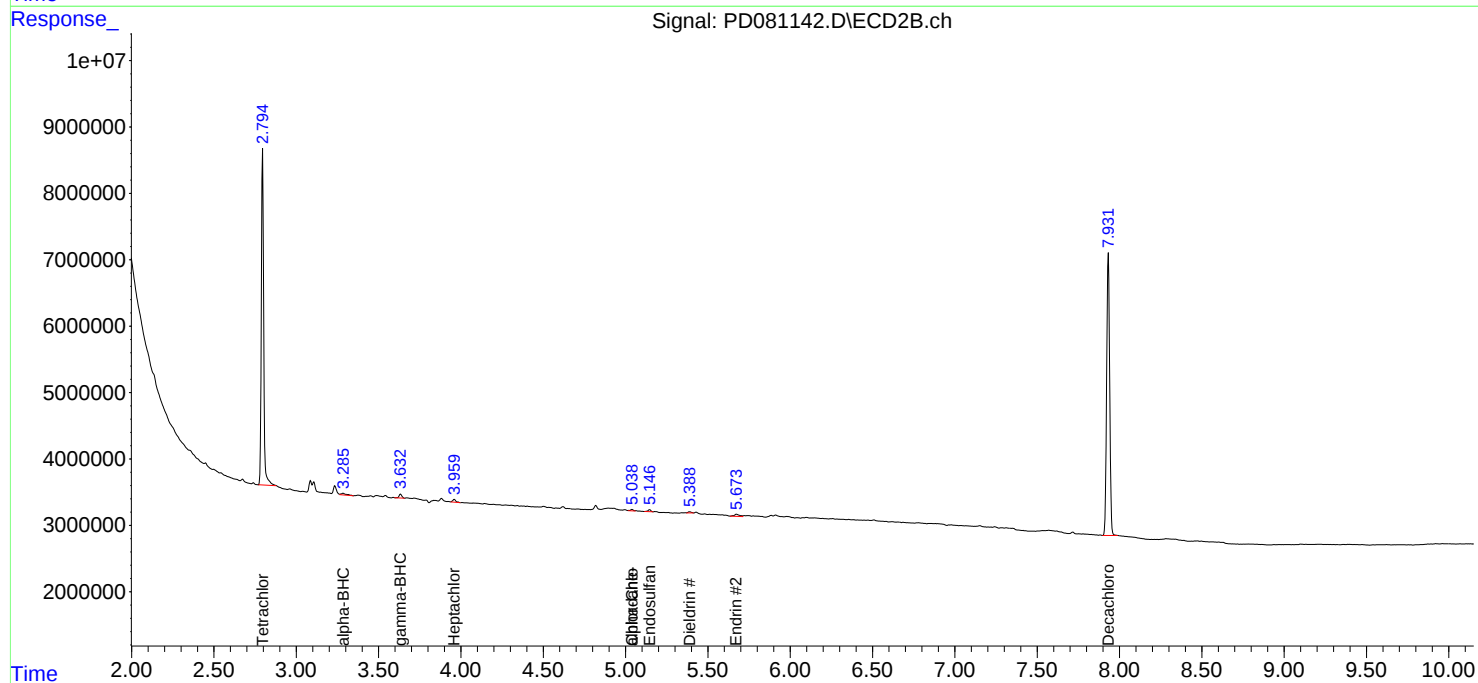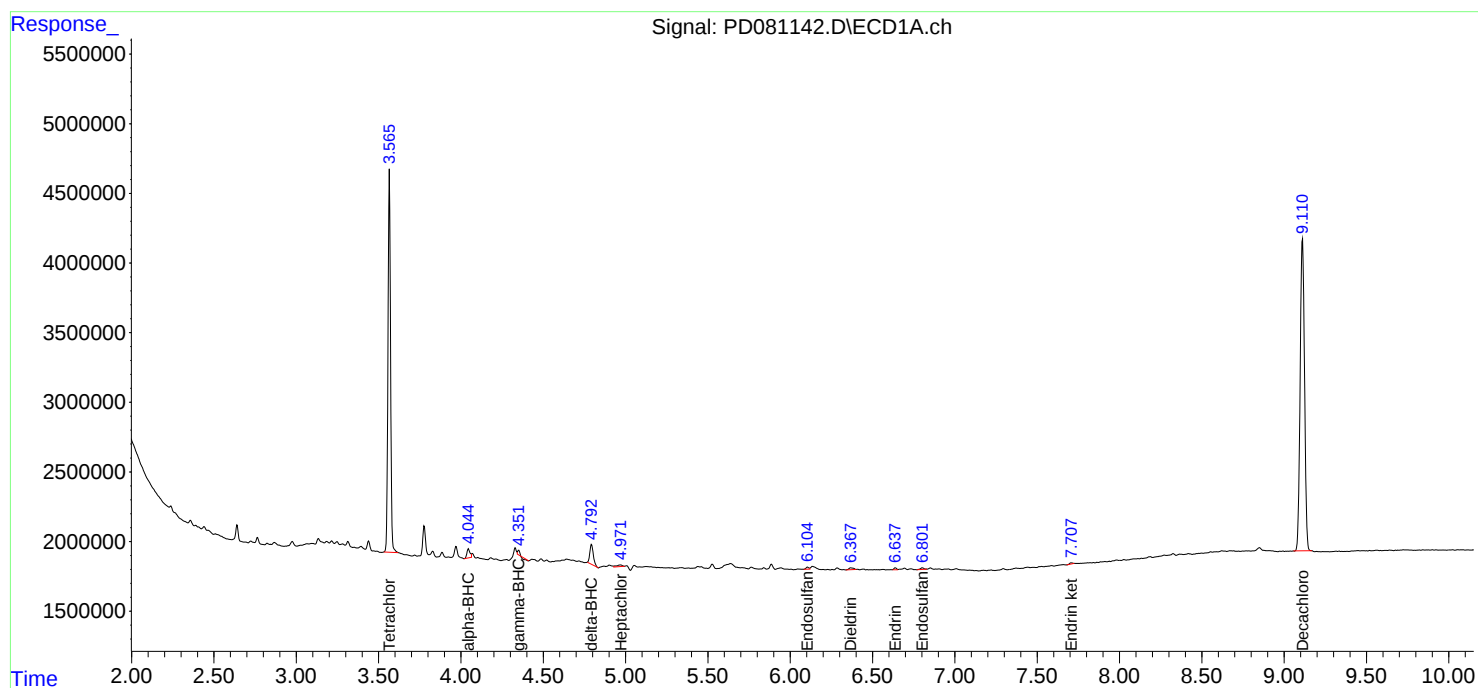


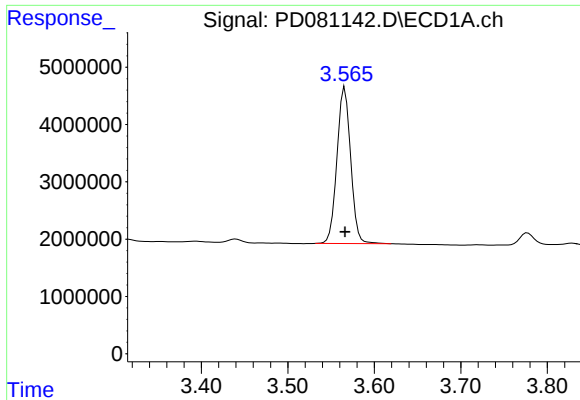

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 29877798
Conc: 21.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-7-0-2

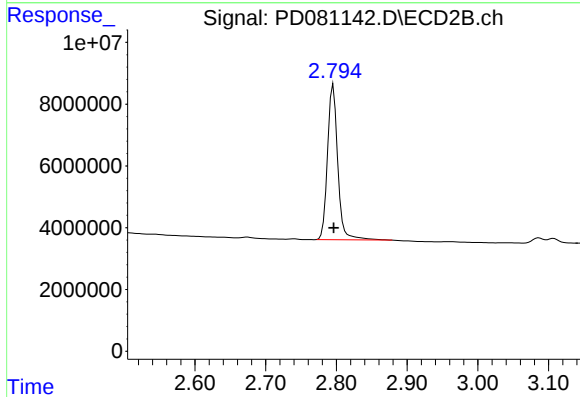


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 50704445
Conc: 21.20 ng/ml

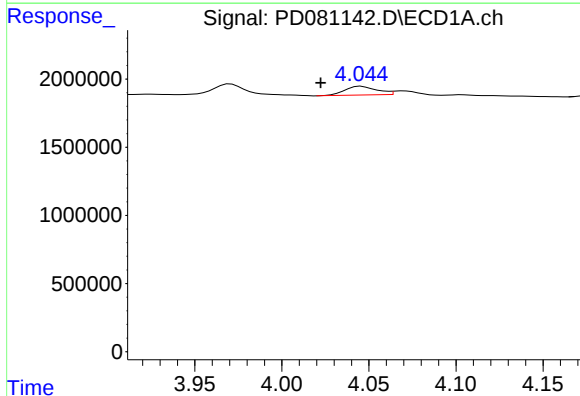


#2 alpha-BHC

R.T.: 4.046 min
Delta R.T.: 0.023 min
Response: 814519
Conc: 0.33 ng/ml

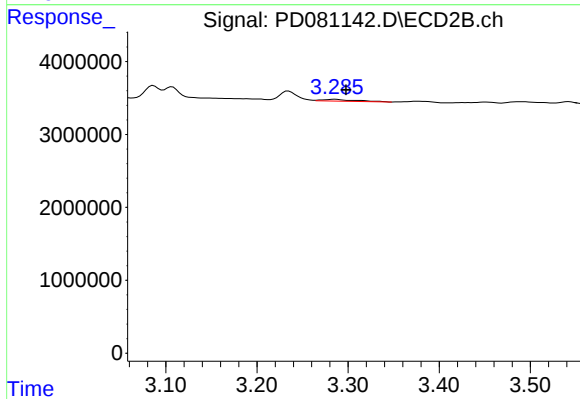

#2 alpha-BHC


R.T.: 3.286 min
Delta R.T.: -0.012 min
Response: 646057
Conc: 0.17 ng/ml

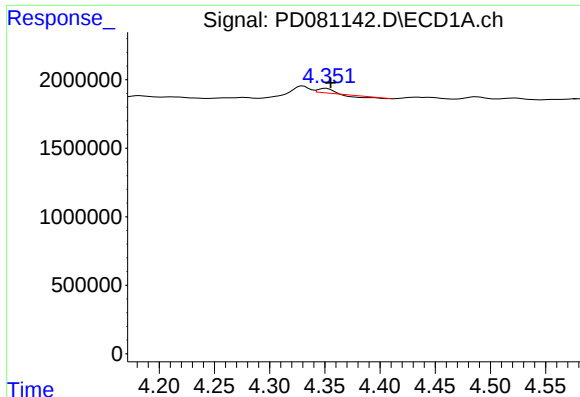

#3 gamma-BHC (Lindane)


R.T.: 4.351 min
Delta R.T.: -0.004 min
Response: 77529
Conc: 0.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-7-0-2

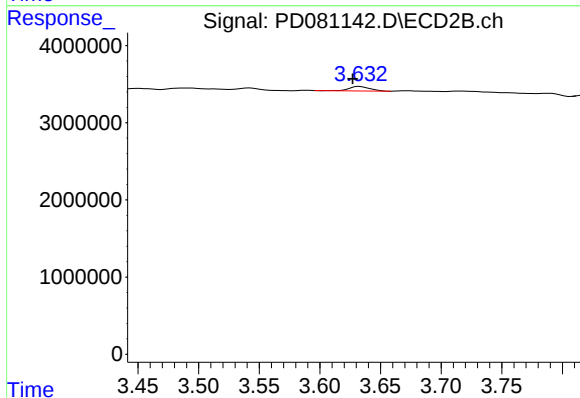


#3 gamma-BHC (Lindane)

R.T.: 3.633 min
Delta R.T.: 0.006 min
Response: 683585
Conc: 0.18 ng/ml

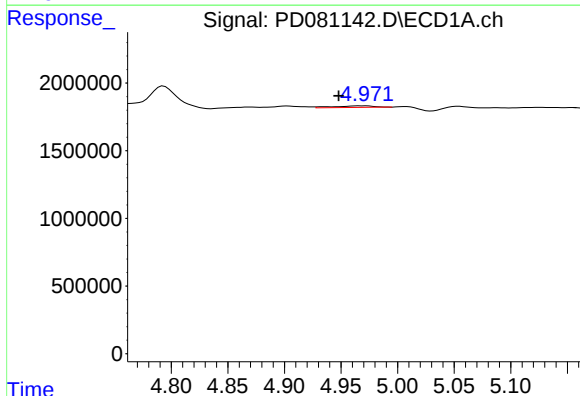


#4 Heptachlor

R.T.: 4.972 min
Delta R.T.: 0.024 min
Response: 284021
Conc: 0.12 ng/ml

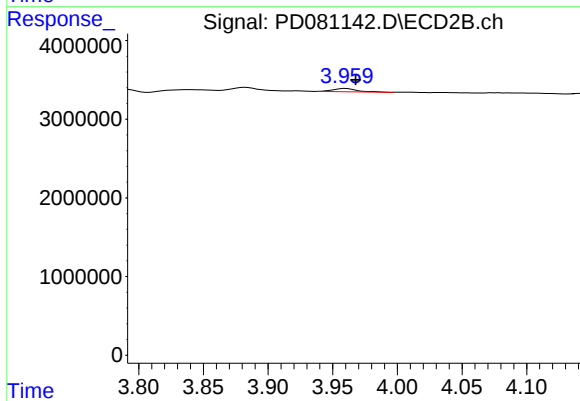

#4 Heptachlor


R.T.: 3.960 min
Delta R.T.: -0.008 min
Response: 545819
Conc: 0.16 ng/ml

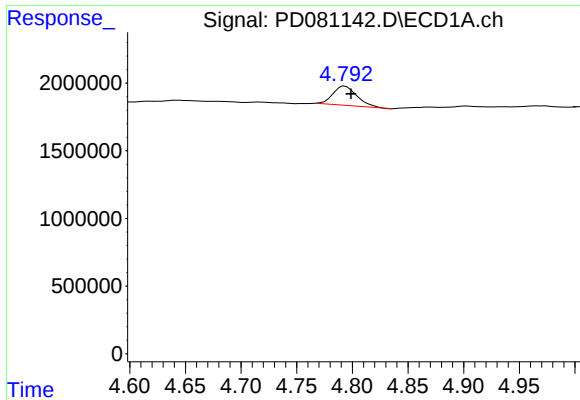

#7 delta-BHC


R.T.: 4.793 min
Delta R.T.: -0.006 min
Response: 2146186
Conc: 0.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-7-0-2

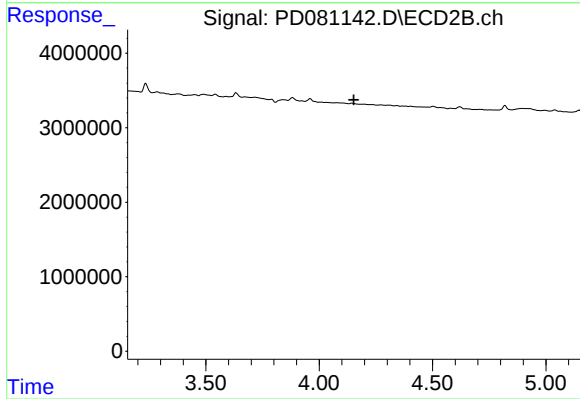


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.153 min
Response: 0
Conc: N.D.

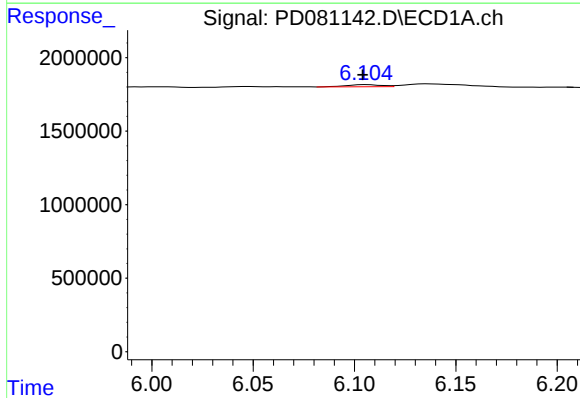


#9 Endosulfan I

R.T.: 6.106 min
Delta R.T.: 0.002 min
Response: 175221
Conc: 0.08 ng/ml

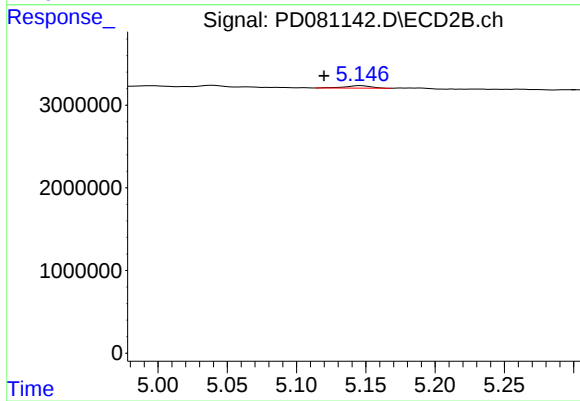

#9 Endosulfan I


R.T.: 5.147 min
Delta R.T.: 0.027 min
Response: 369051
Conc: 0.12 ng/ml

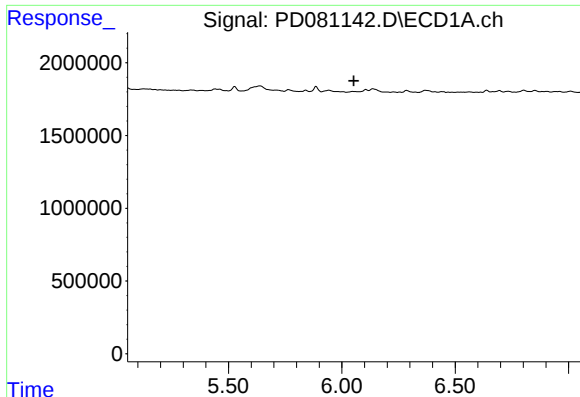

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.053 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
EB-7-0-2

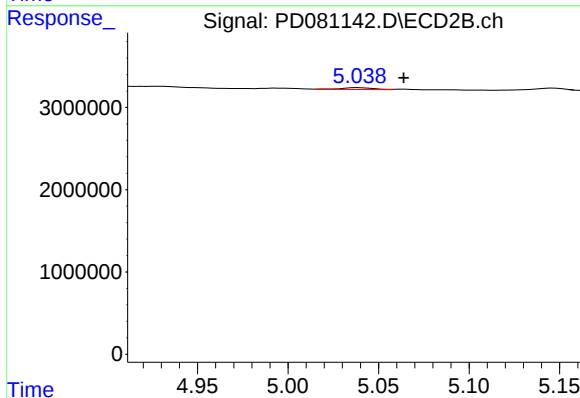


#11 alpha-Chlordane

R.T.: 5.039 min
Delta R.T.: -0.025 min
Response: 279547
Conc: 0.09 ng/ml

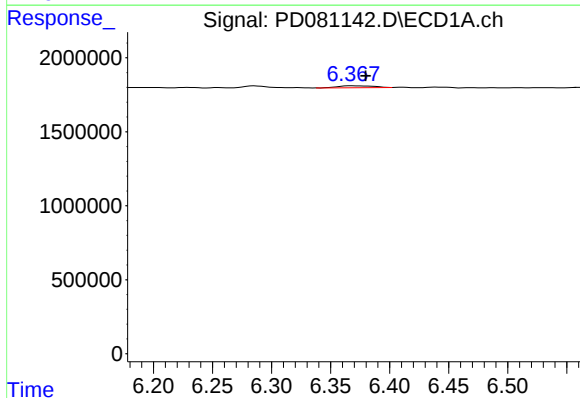


#13 Dieldrin

R.T.: 6.368 min
Delta R.T.: -0.012 min
Response: 261526
Conc: 0.12 ng/ml

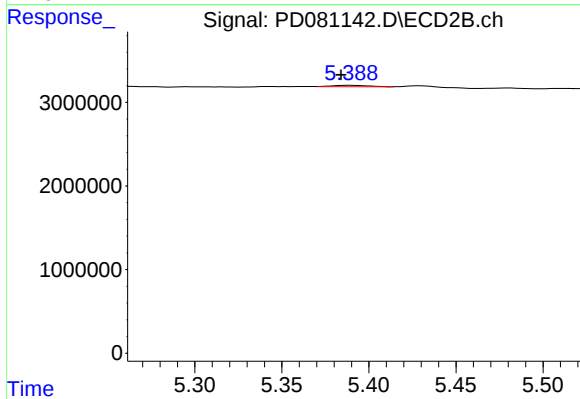

#13 Dieldrin


R.T.: 5.390 min
Delta R.T.: 0.006 min
Response: 229471
Conc: 0.07 ng/ml

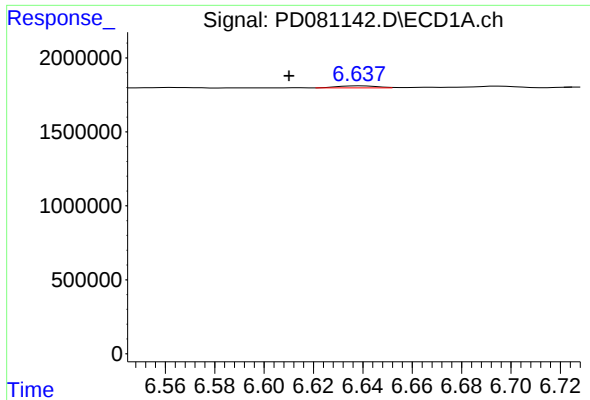

#14 Endrin


R.T.: 6.639 min
Delta R.T.: 0.029 min
Response: 147021
Conc: 0.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-7-0-2

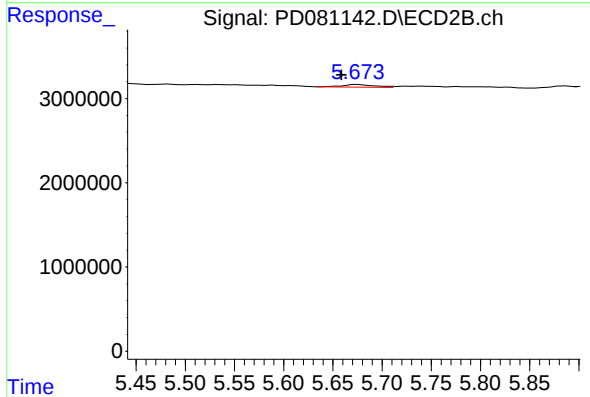


#14 Endrin

R.T.: 5.674 min
Delta R.T.: 0.015 min
Response: 724812
Conc: 0.24 ng/ml

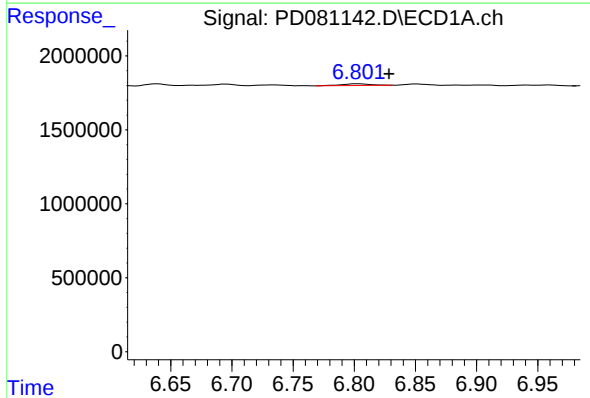


#15 Endosulfan II

R.T.: 6.803 min
Delta R.T.: -0.025 min
Response: 173134
Conc: 0.09 ng/ml

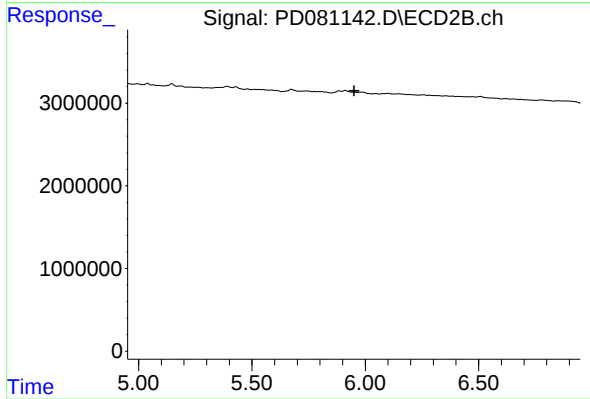

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.951 min
Response: 0
Conc: N.D.

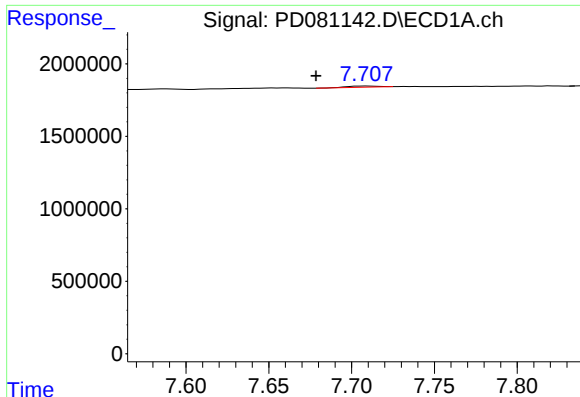

#21 Endrin ketone


R.T.: 7.709 min
Delta R.T.: 0.030 min
Response: 102949
Conc: 0.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-7-0-2

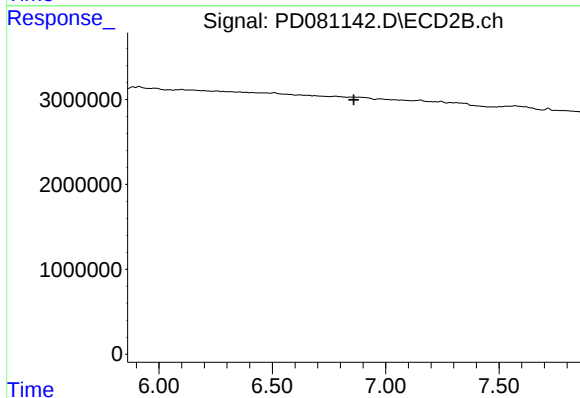


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.859 min
Response: 0
Conc: N.D.

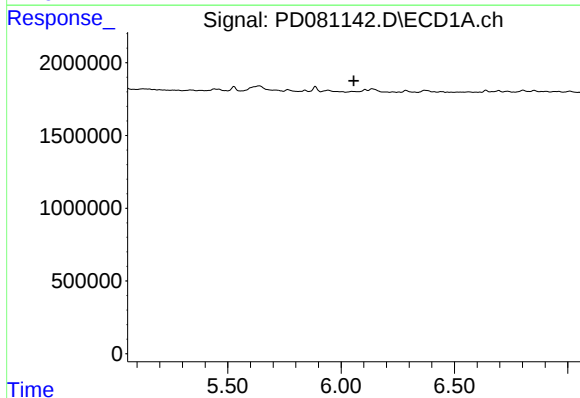


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.057 min
Response: 0
Conc: N.D.

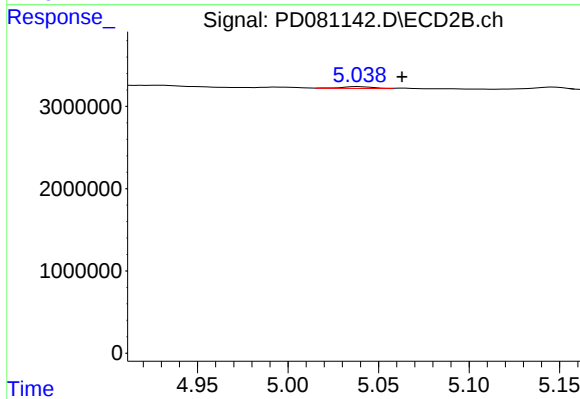

#26 Chlordane-4


R.T.: 5.039 min
Delta R.T.: -0.024 min
Response: 279547
Conc: 0.88 ng/ml

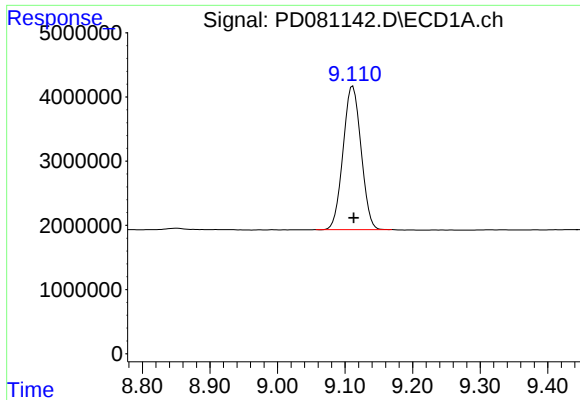

#28 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: -0.002 min
Response: 41277330
Conc: 20.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-7-0-2

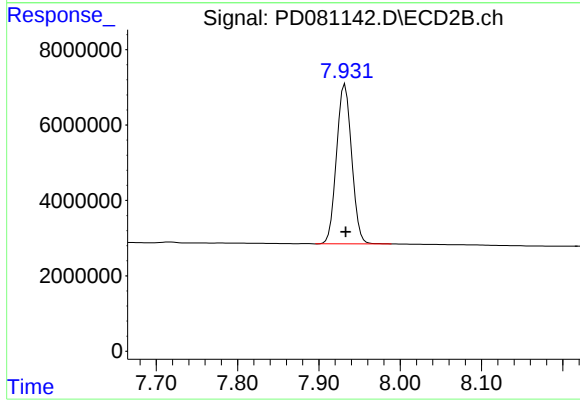

#28 Decachlorobiphenyl

R.T.: 7.932 min
Delta R.T.: 0.000 min
Response: 54710756
Conc: 20.54 ng/ml